


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011922\
 Data File : BM033775.D
 Acq On : 19 Jan 2022 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 17 16:30:56 2022

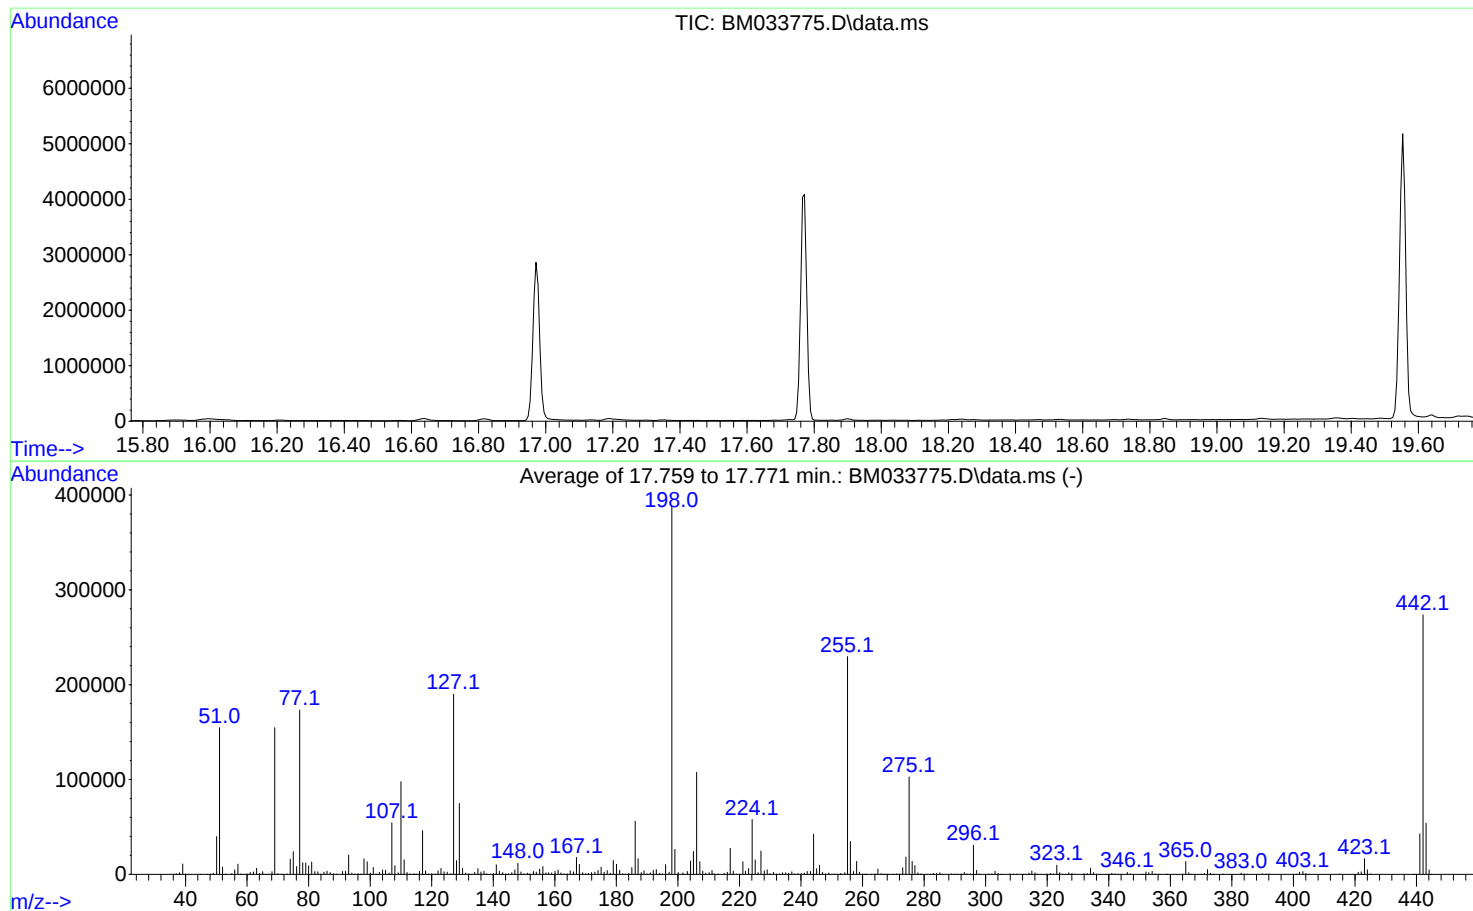




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	154796	PASS
68	69	0.00	2	1.9	2894	PASS
69	198	0.00	100	39.9	154651	PASS
70	69	0.00	2	0.5	814	PASS
127	198	10	80	49.0	189973	PASS
197	198	0.00	2	0.6	2379	PASS
198	198	100	100	100.0	387883	PASS
199	198	5	9	6.8	26296	PASS
275	198	10	60	26.5	102749	PASS
365	198	1	100	3.5	13555	PASS
441	198	0.01	100	11.0	42685	PASS
442	442	50	100	100.0	273699	PASS
443	442	15	24	19.7	54013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011922\
 Data File : BM033775.D
 Acq On : 19 Jan 2022 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 19 17:38:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 17 16:30:56 2022
 Response via : Initial Calibration

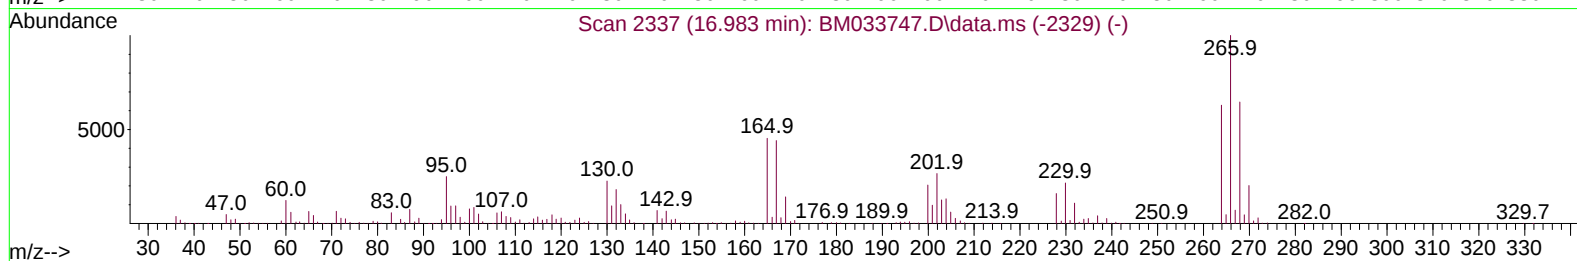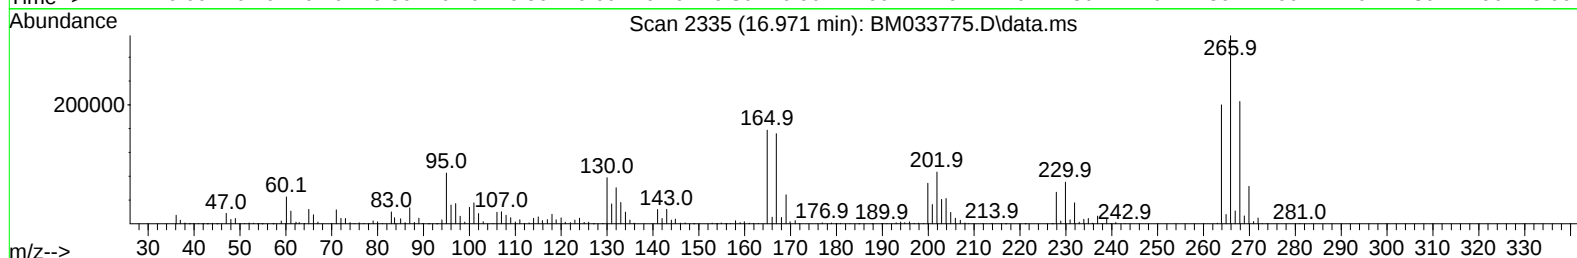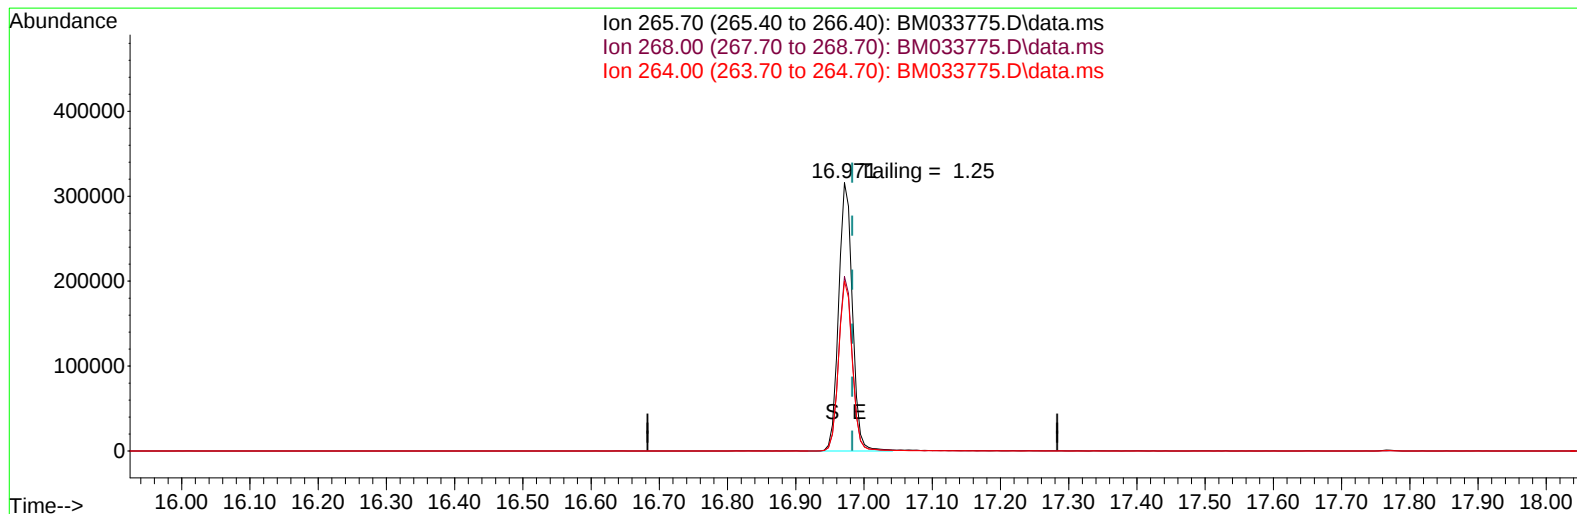

TIC: BM033775.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.012) 156917.78 ng




response 444064

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.02
264.00	61.40	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011922\
Data File : BM033775.D
Acq On : 19 Jan 2022 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 19 17:38:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 17 16:30:56 2022
Response via : Initial Calibration

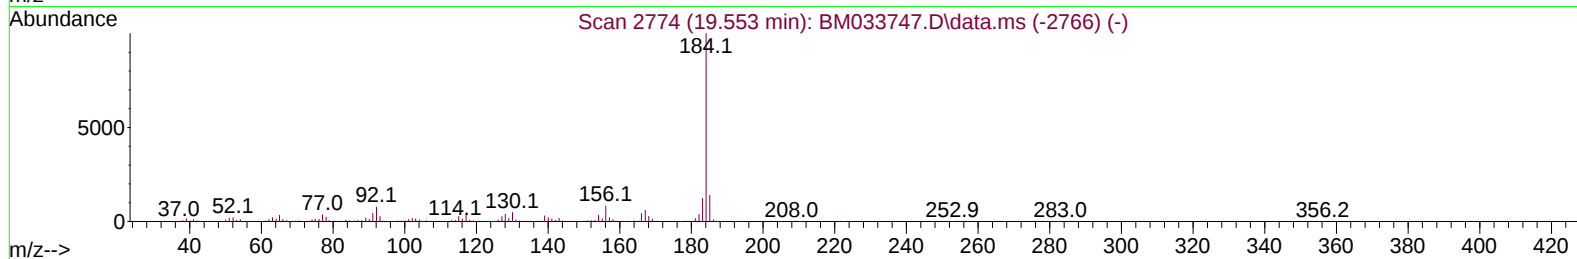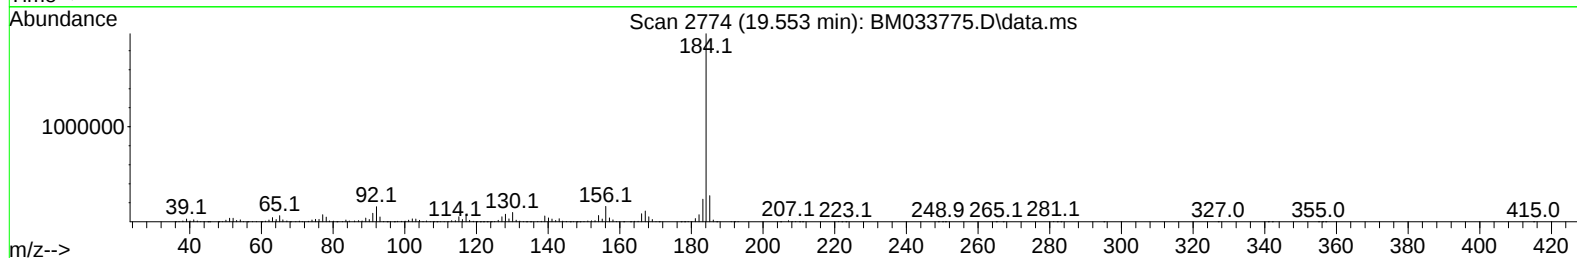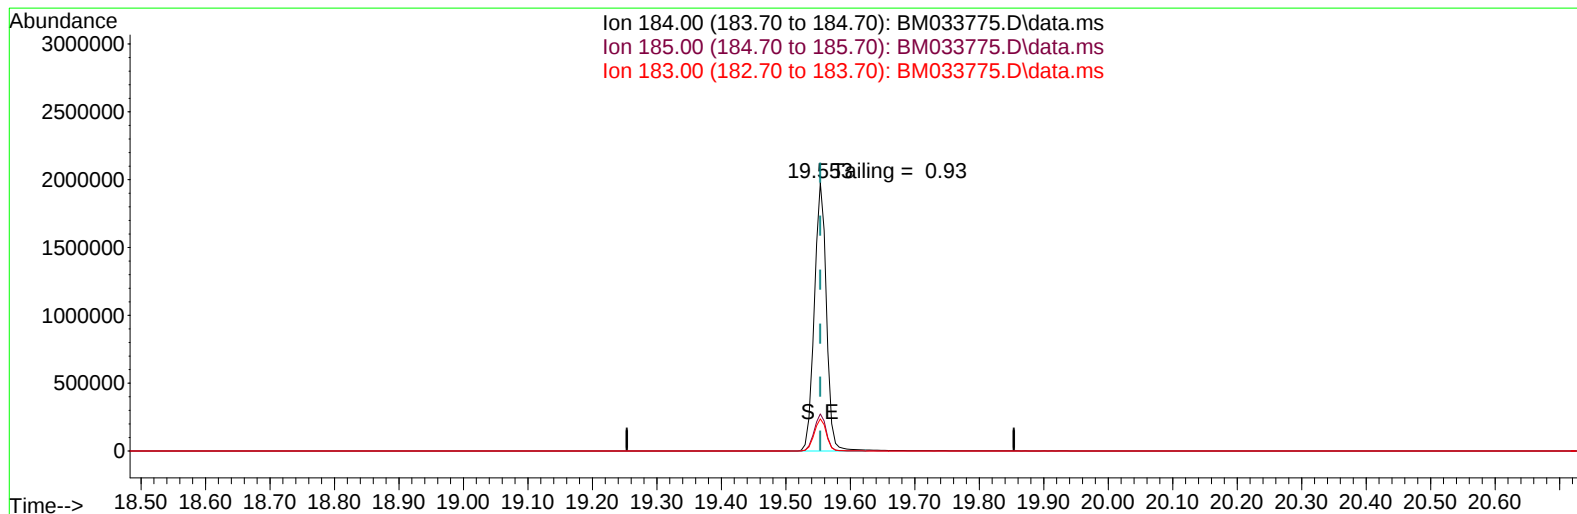

TIC: BM033775.D\data.ms

(77) Benzidine

19.553min (+ 0.000) 12455.07 ng

response 2605424

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.84
183.00	12.10	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/19/2022	BNA_M	<u>BM033775.D</u>
Compound Name	Response	Retention Time
DDT	1424349	20.78
DDD	11085	20.34
DDE	4072	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15157	1439506	1.05

Instrument :
BNA_M
ClientSampleId :
DFTPP