
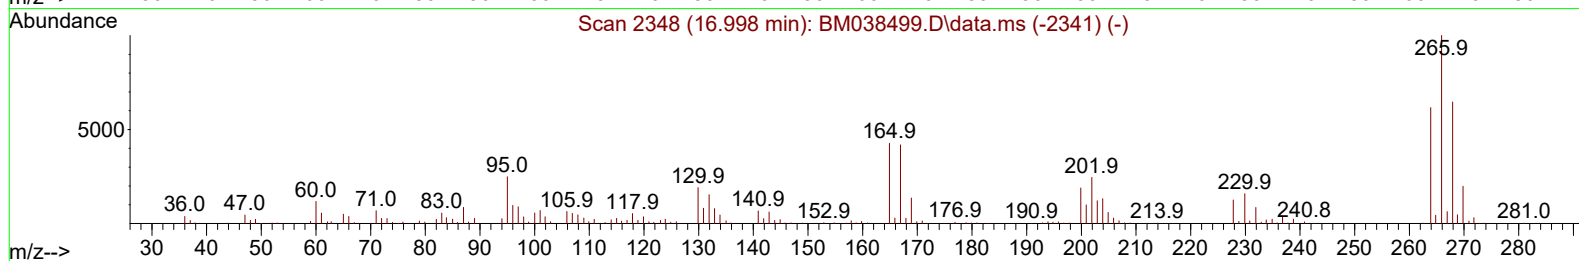
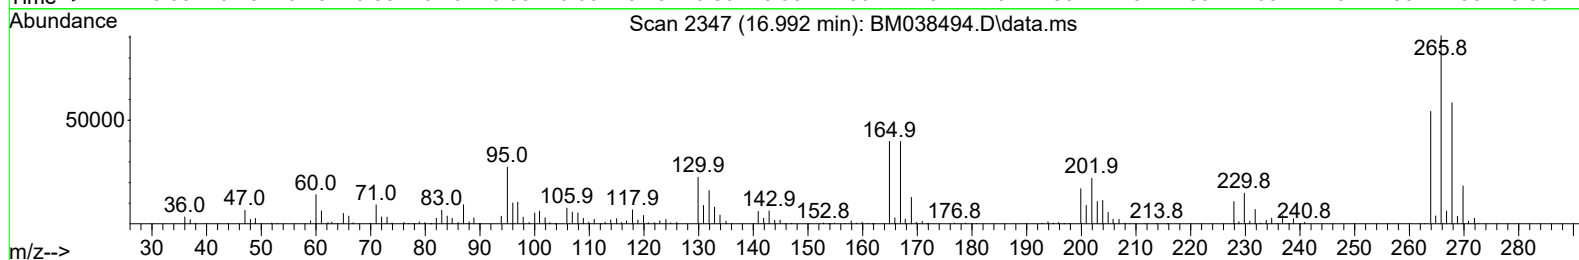


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
 Data File : BM038494.D
 Acq On : 20 Jan 2023 11:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 11:04:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 21 01:21:49 2023
 Response via : Initial Calibration

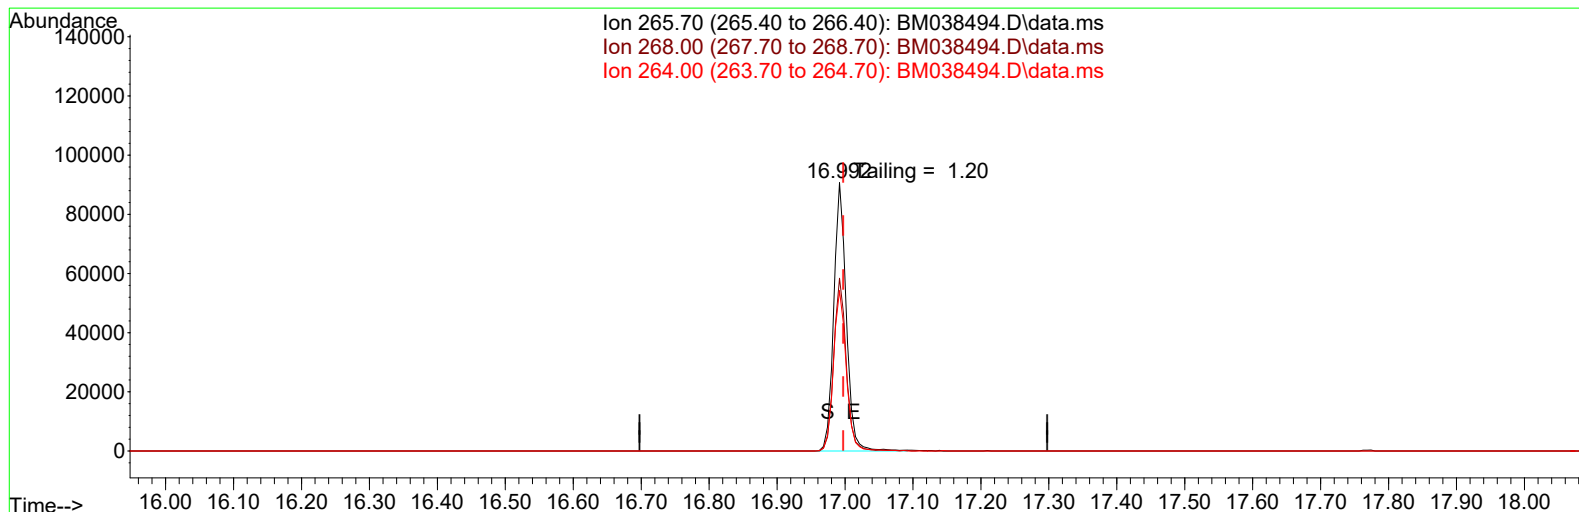

TIC: BM038494.D\data.ms




(70) Pentachlorophenol (C)

16.992min (-0.006) 0.00 ng

response 115884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.37
264.00	61.70	59.78
0.00	0.00	0.00

Quant Time: Jan 23 11:04:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 21 01:21:49 2023
Response via : Initial Calibration

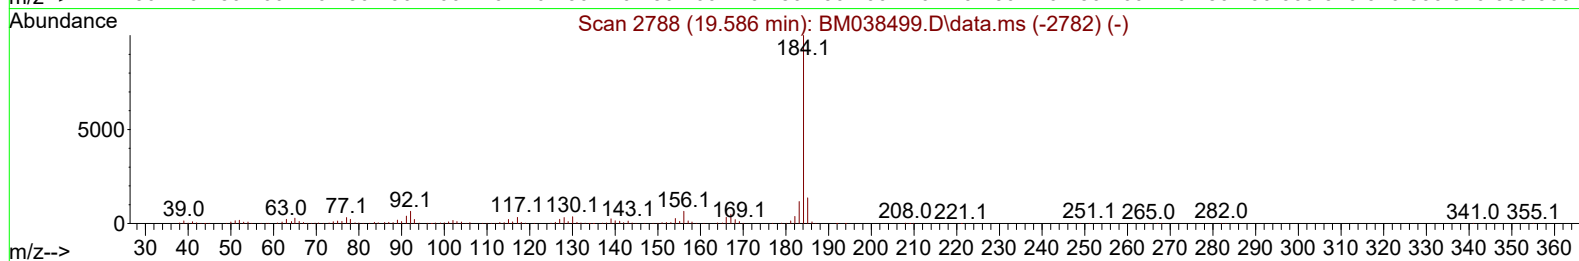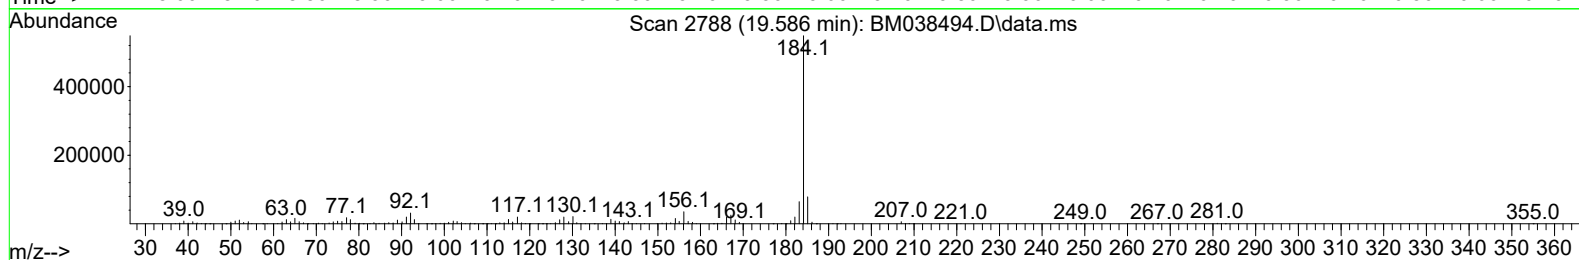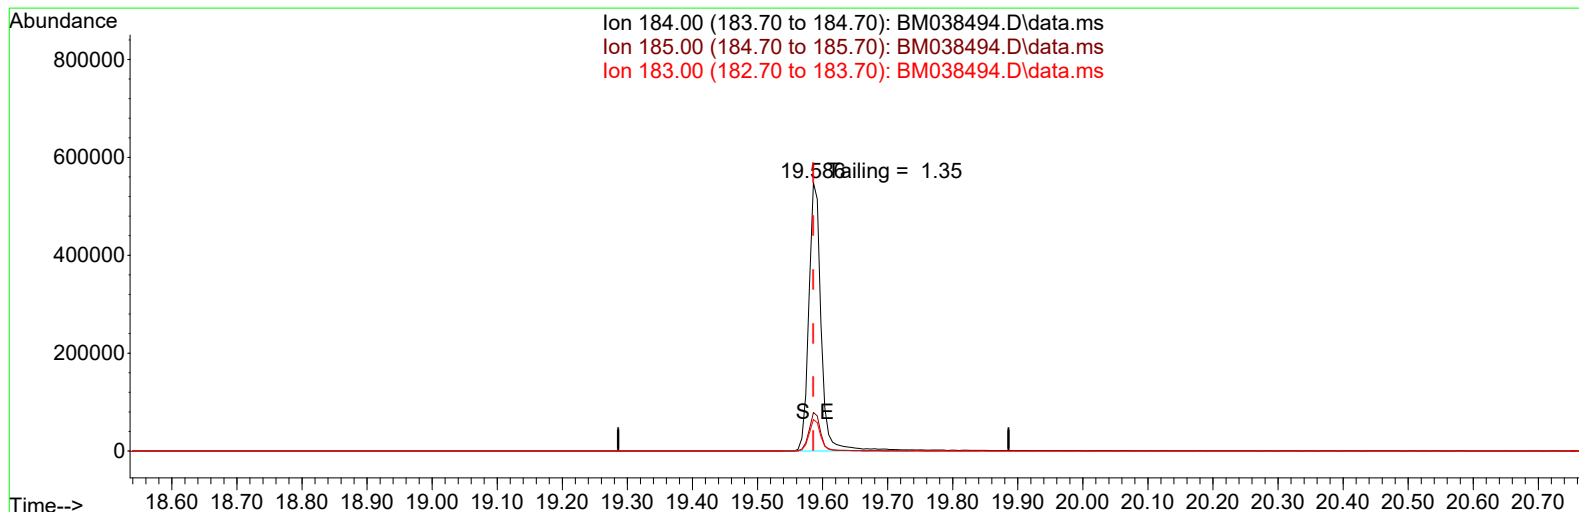

TIC: BM038494.D\data.ms

(77) Benzidine

19.586min (+ 0.000) 162838.10 ng

response 727301

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.37
183.00	11.60	11.78
0.00	0.00	0.00