

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
 Data File : BM038504.D
 Acq On : 20 Jan 2023 17:51
 Operator : CG/JU
 Sample : PB150235BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150235BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	312	317	326	rBV	373936	508347	14.61%	2.941%
2	5.522	390	397	411	rBV	1149219	1578026	45.34%	9.131%
3	7.134	664	671	685	rBV	1393757	2142420	61.56%	12.397%
4	7.969	807	813	820	rBV	262179	400459	11.51%	2.317%
5	9.145	1004	1013	1027	rBV	804627	1279813	36.77%	7.405%
6	10.780	1285	1291	1302	rBV	279214	460210	13.22%	2.663%
7	13.233	1701	1708	1722	rBV	2053245	2860852	82.20%	16.554%
8	14.604	1935	1941	1948	rBV	392830	554111	15.92%	3.206%
9	16.092	2187	2194	2206	rBV	1503576	2072653	59.55%	11.993%
10	17.345	2401	2407	2417	rBV	442668	610300	17.54%	3.531%
11	19.956	2846	2851	2859	rBV	3085812	3480289	100.00%	20.138%
12	21.515	3112	3116	3123	rBV	482325	621427	17.86%	3.596%
13	23.932	3521	3527	3536	rBV	366562	713467	20.50%	4.128%




Sum of corrected areas: 17282374

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
Data File : BM038504.D
Acq On : 20 Jan 2023 17:51
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

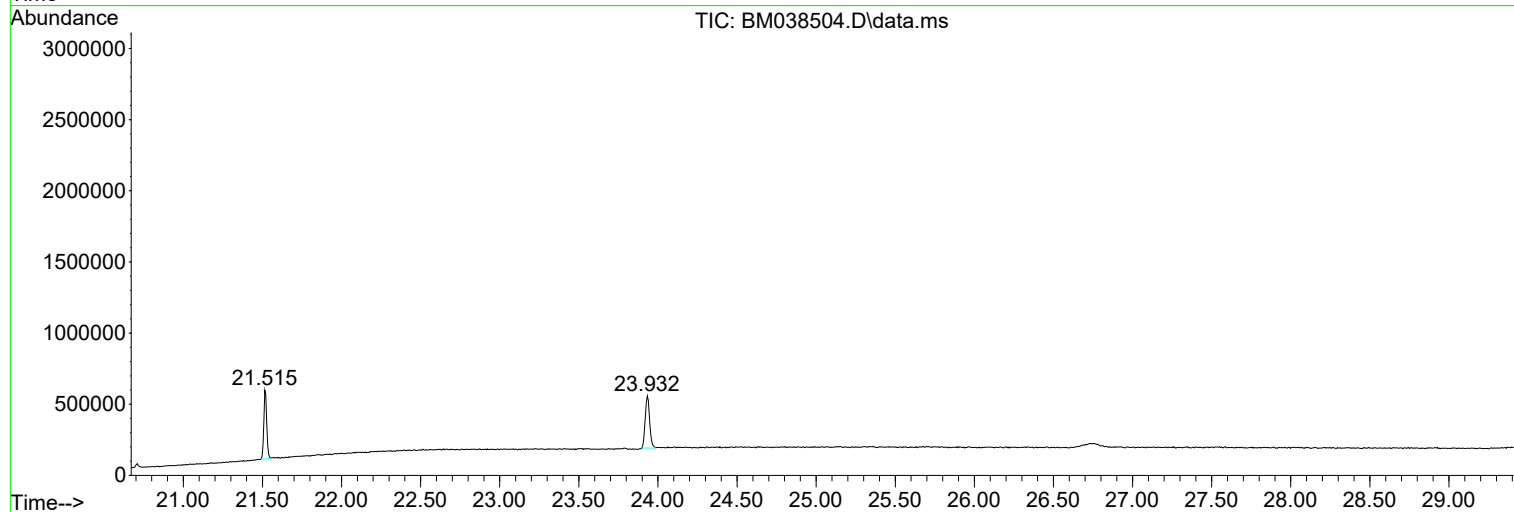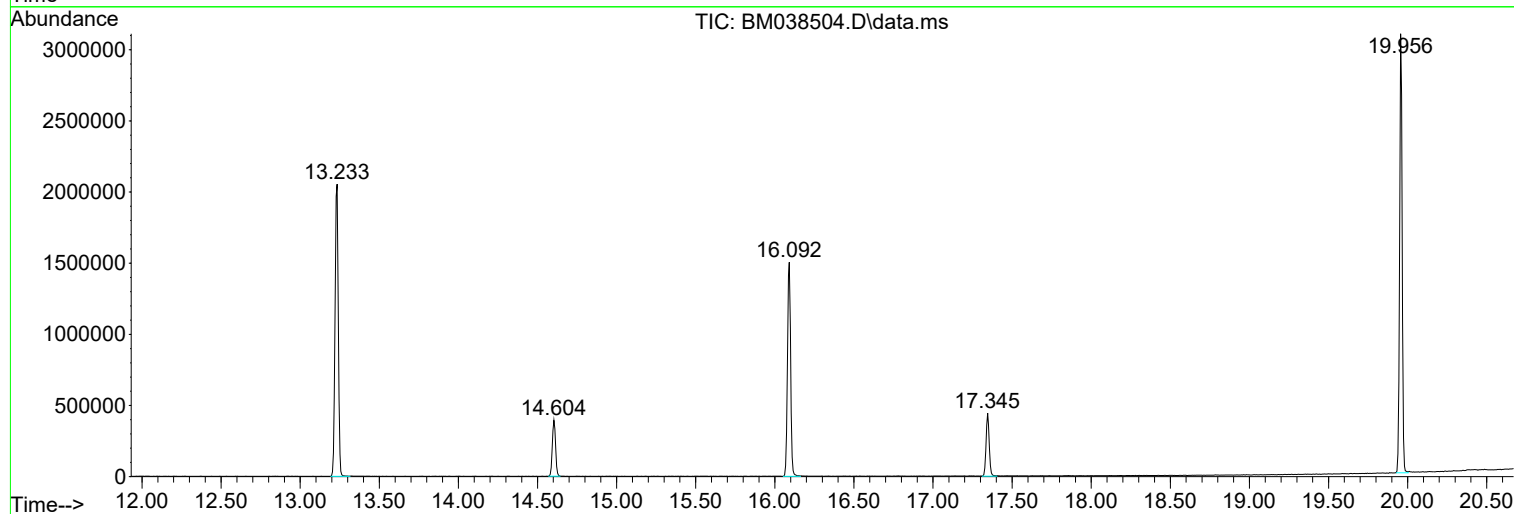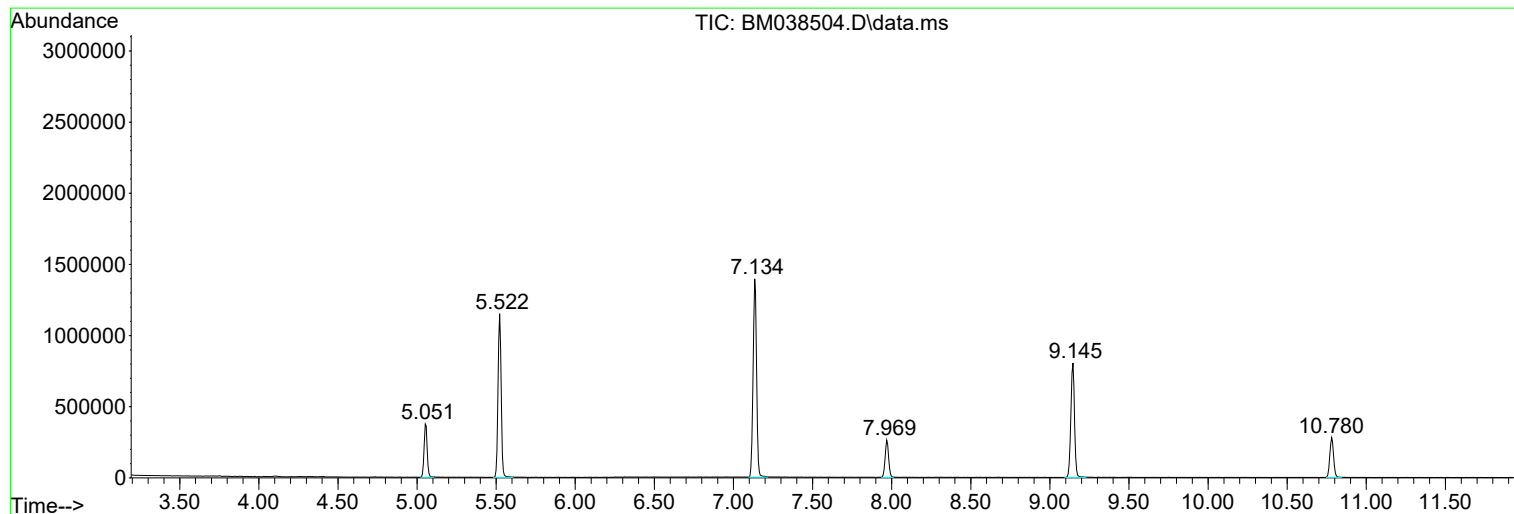

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
Data File : BM038504.D
Acq On : 20 Jan 2023 17:51
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150235BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.051	25.39 ng	508347	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	47		
3	Propane, 1,1-dipropoxy-	160	C9H20O2	004744-11-0	38		
4	Dimethadione	129	C5H7NO3	000695-53-4	28		
5	Succinic acid, heptyl 2-methoxye...	274	C14H26O5	1000325-80-7	28		

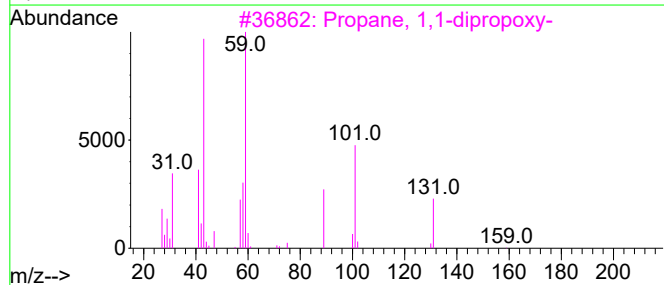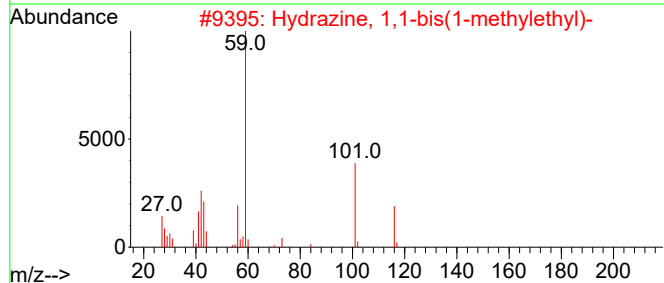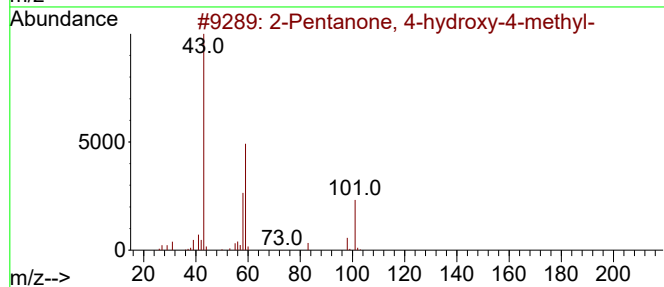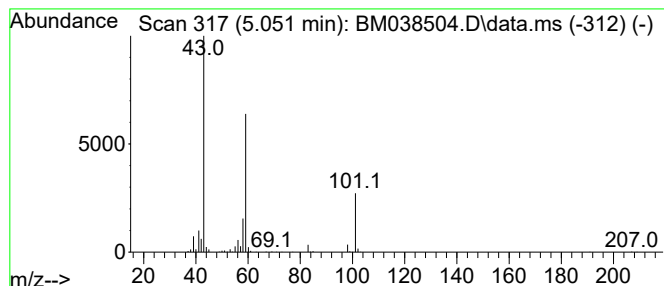

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
Data File : BM038504.D
Acq On : 20 Jan 2023 17:51
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.051	25.4	ng	508347	1	7.969	400459	20.0