
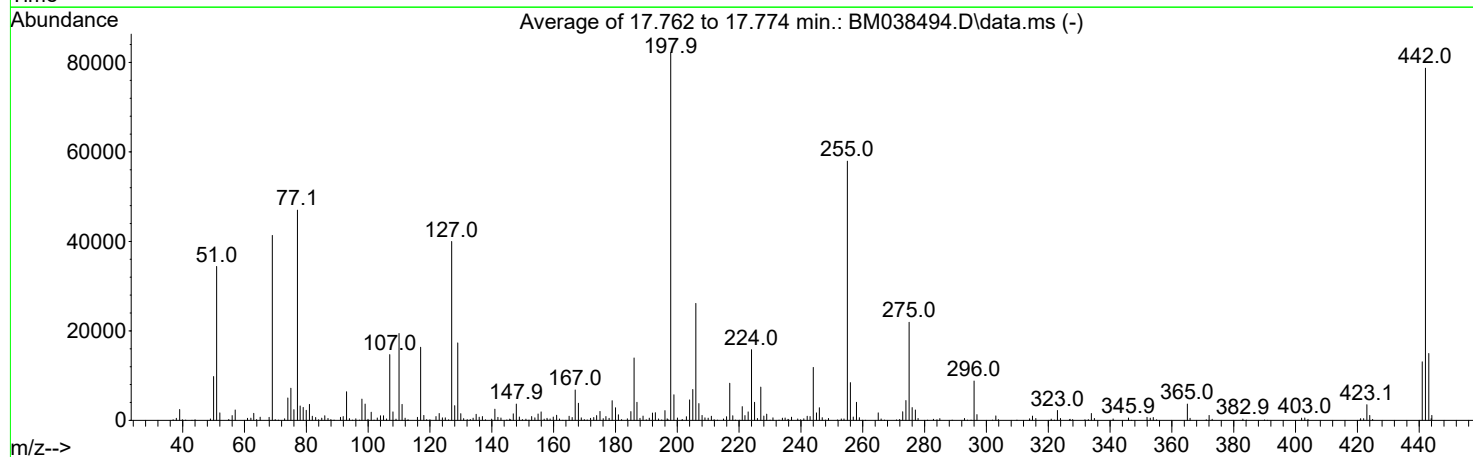


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
 Data File : BM038494.D
 Acq On : 20 Jan 2023 11:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 21 01:21:49 2023

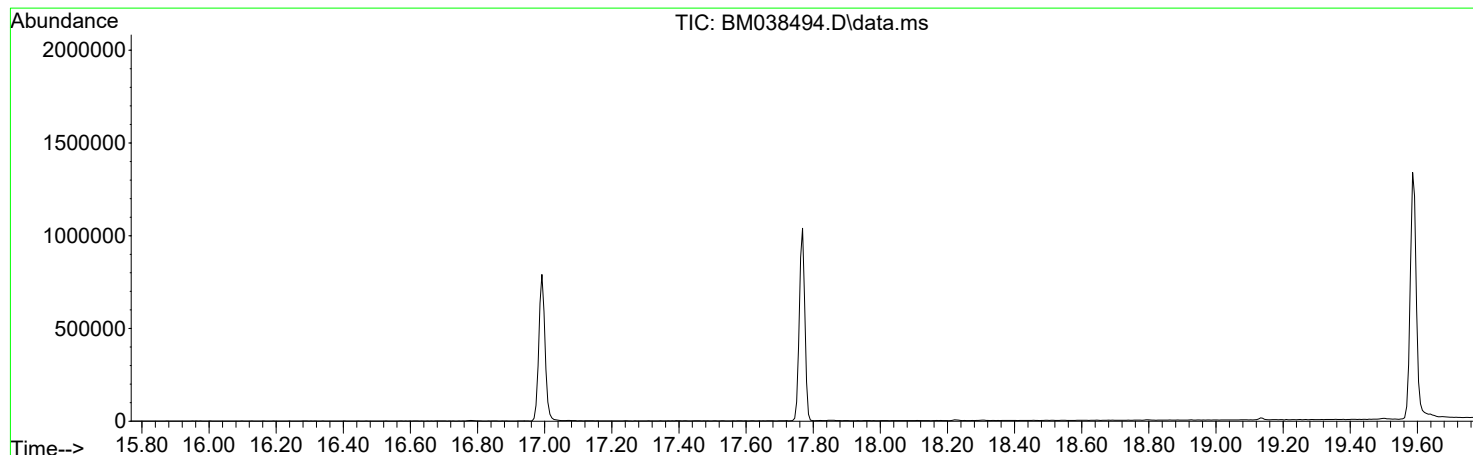




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	34403	PASS
68	69	0.00	2	1.6	673	PASS
69	198	0.00	100	50.3	41331	PASS
70	69	0.00	2	0.4	167	PASS
127	198	10	80	48.6	39992	PASS
197	198	0.00	2	0.4	344	PASS
198	198	100	100	100.0	82227	PASS
199	198	5	9	7.0	5735	PASS
275	198	10	60	26.7	21915	PASS
365	198	1	100	4.5	3664	PASS
441	198	0.01	100	15.9	13088	PASS
442	442	50	100	100.0	78712	PASS
443	442	15	24	19.0	14946	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
 Data File : BM038494.D
 Acq On : 20 Jan 2023 11:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 23 11:04:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 21 01:21:49 2023
 Response via : Initial Calibration

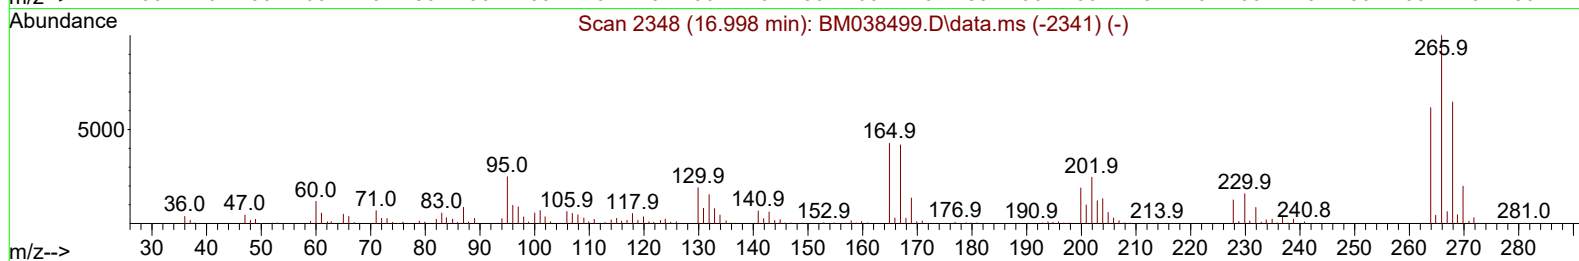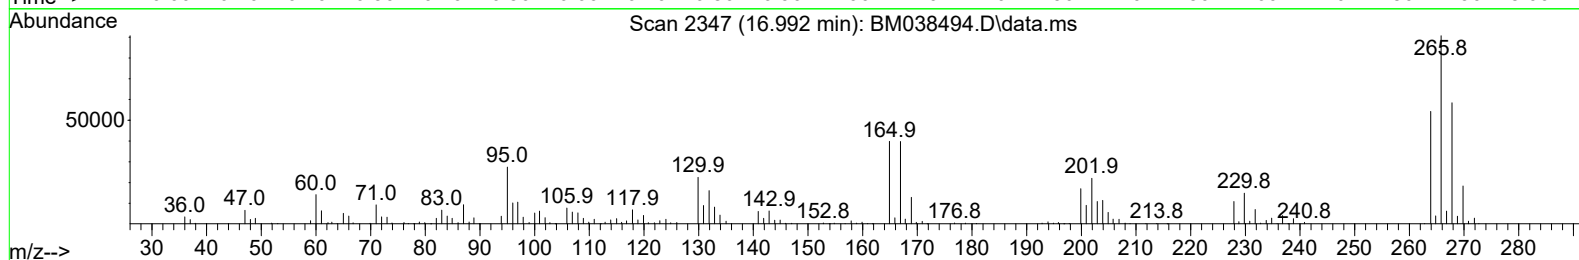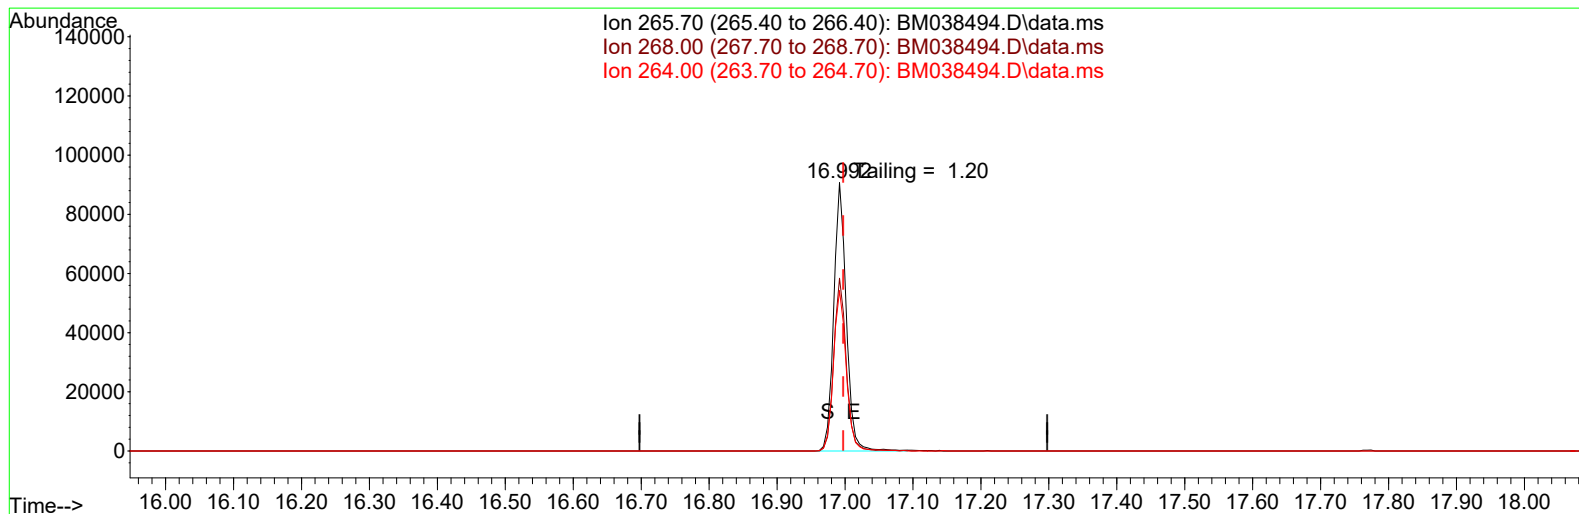

TIC: BM038494.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.006) 0.00 ng




response 115884

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.37
264.00	61.70	59.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012023\
Data File : BM038494.D
Acq On : 20 Jan 2023 11:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 23 11:04:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 21 01:21:49 2023
Response via : Initial Calibration

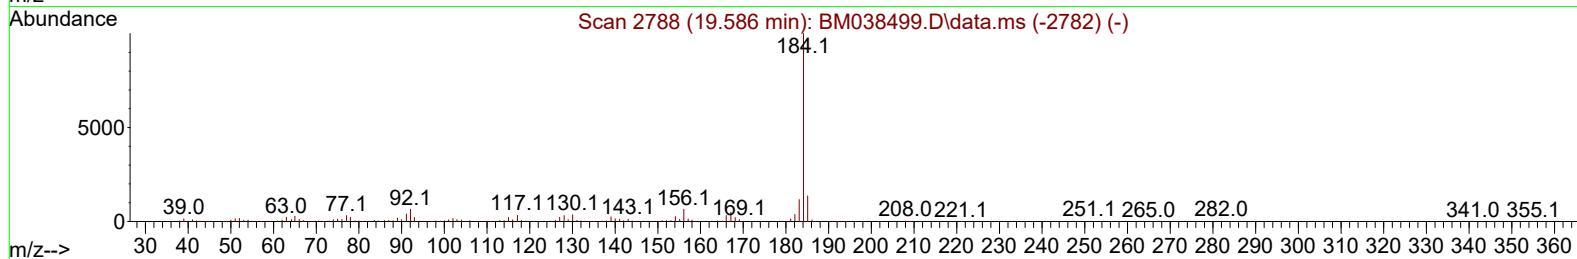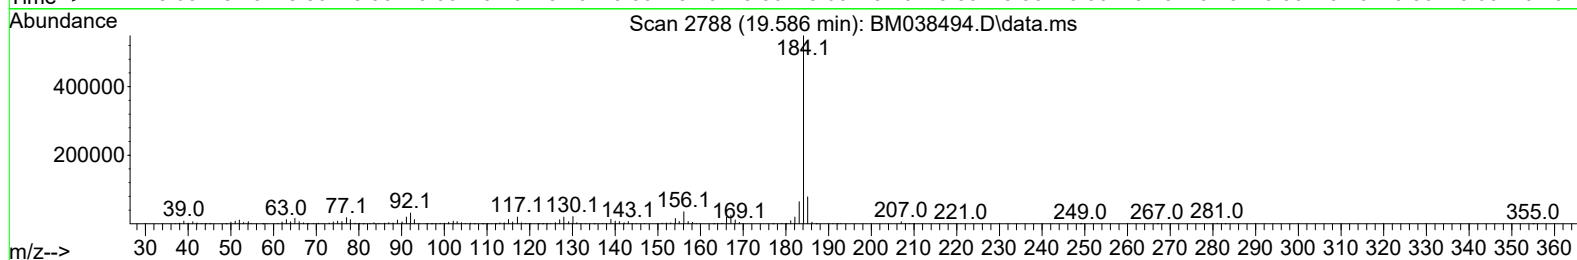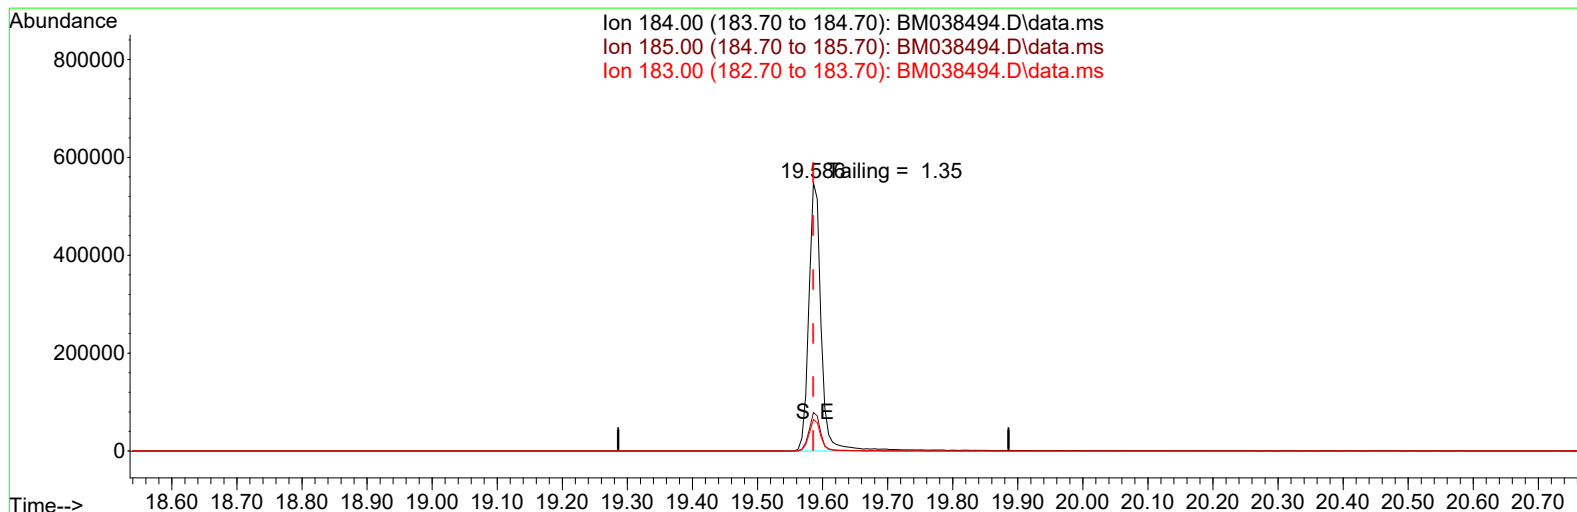

TIC: BM038494.D\data.ms

(77) Benzidine

19.586min (+ 0.000) 162838.10 ng

response 727301

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.37
183.00	11.60	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/20/2023	BNA_M	<u>BM038494.D</u>
Compound Name	Response	Retention Time
DDT	382515	20.809
DDD	2464	20.421
DDE	63	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2527	385042	0.66

Instrument :
BNA_M
ClientSampleId :
DFTPP