
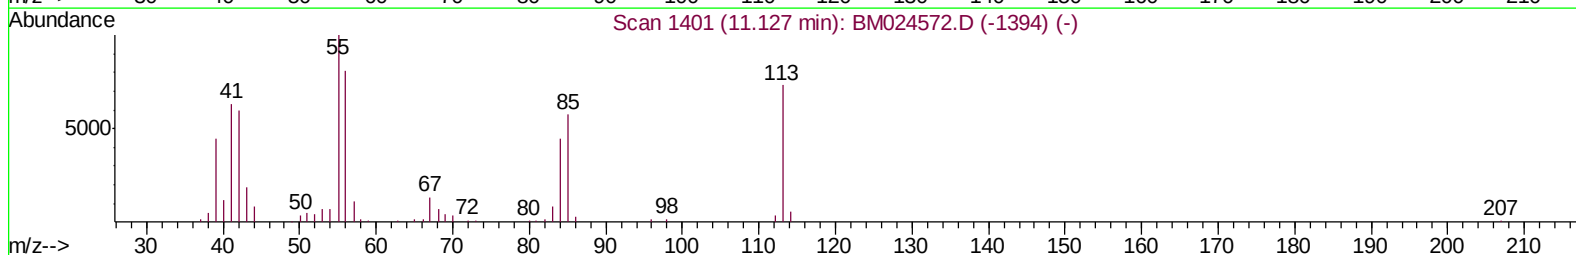
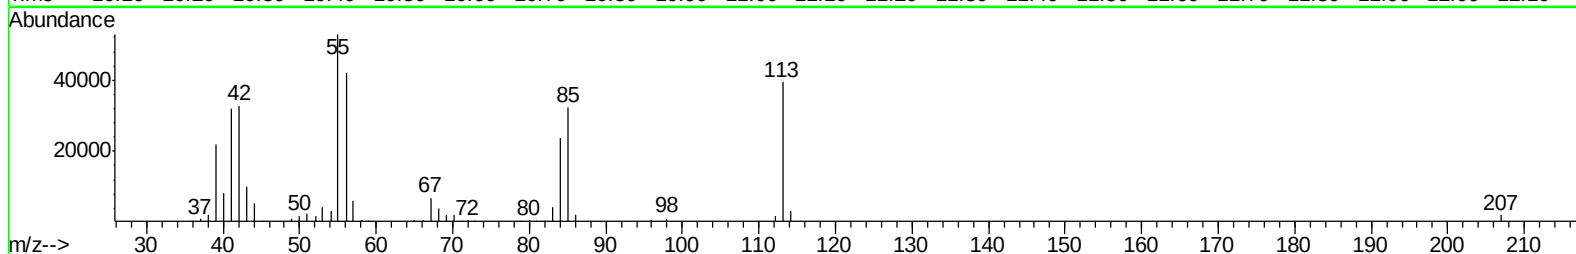


Data File : BM024598.D
Acq On : 23 Jan 2020 00:54
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jan 23 01:29:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 23 01:22:36 2020
Response via : Initial Calibration

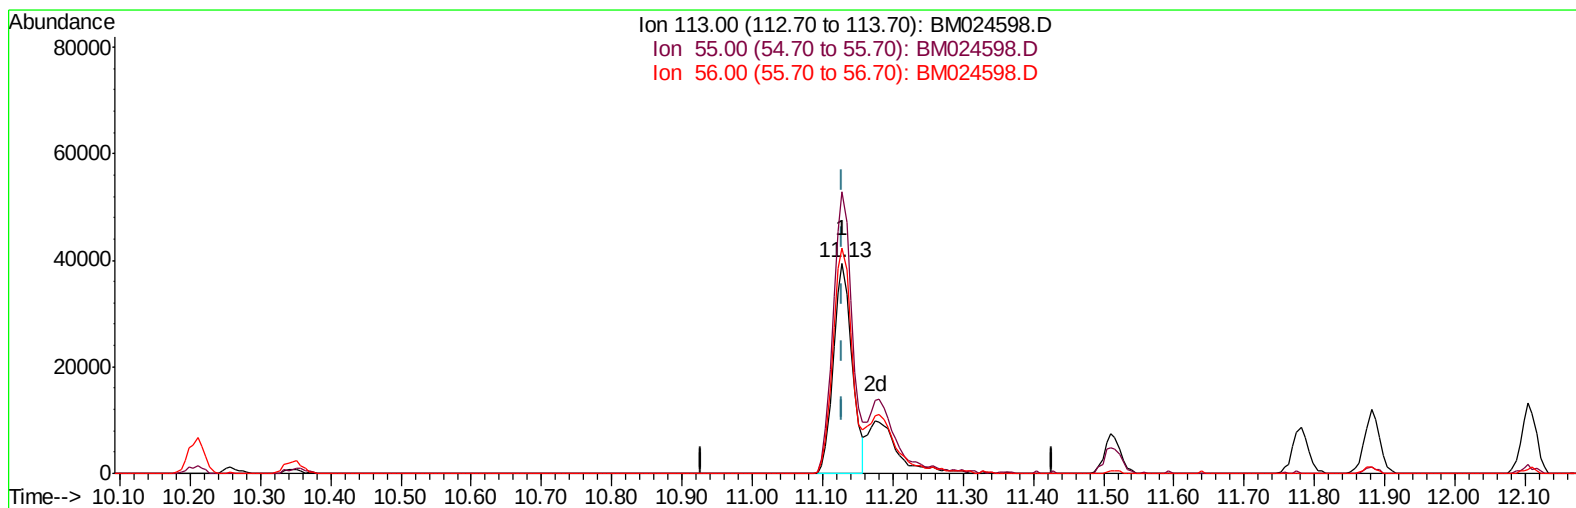

TIC: BM024598.D

(32) Caprolactam

11.128min (+0.000) 15.28ng/ul

response 72340

Ion	Exp%	Act%
113.00	100	100
55.00	147.90	133.99
56.00	113.50	107.00
0.00	0.00	0.00