

Data File : BM024598.D

Acq On : 23 Jan 2020 00:54

Operator : JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Jan 23 01:29:46 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Jan 23 01:22:36 2020

Response via : Initial Calibration

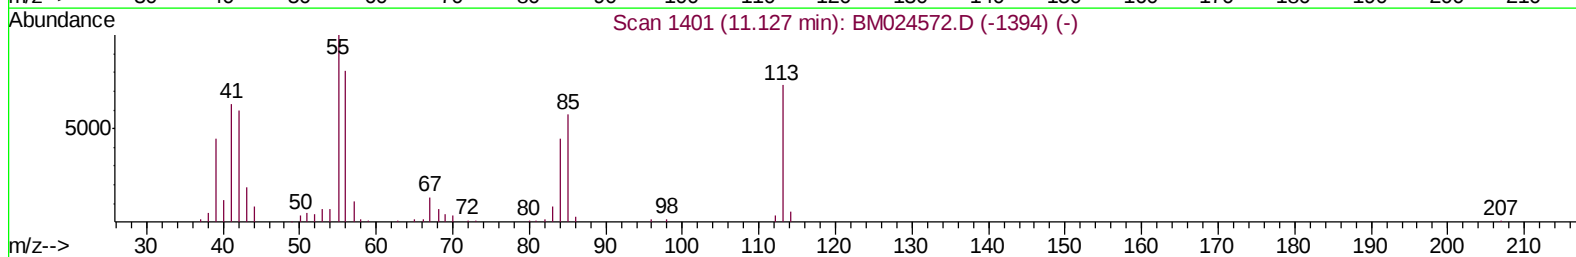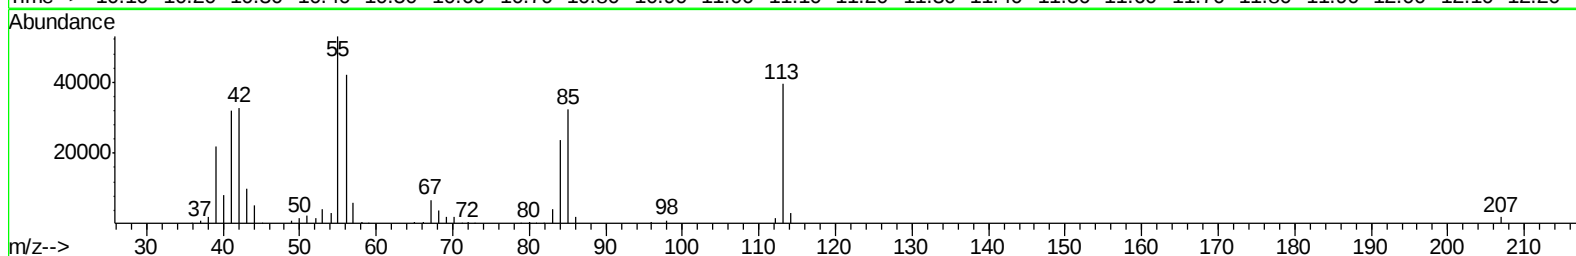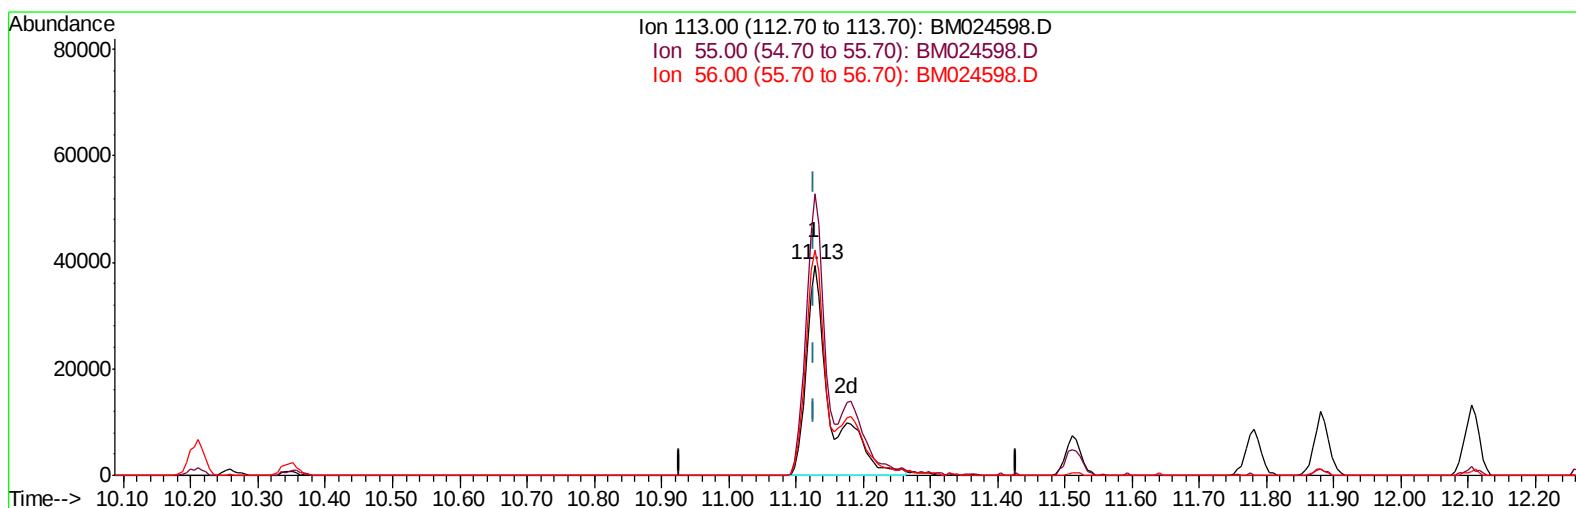

TIC: BM024598.D

(32) Caprolactam

11.128min (+0.000) 21.14ng/ul m

response 100122

Ion	Exp%	Act%
113.00	100	100
55.00	147.90	133.99
56.00	113.50	107.00
0.00	0.00	0.00