

Data File : BM024588.D
Acq On : 22 Jan 2020 18:57
Operator : JU
Sample : L1118-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASK3

Quant Time: Jan 23 01:25:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 23 01:22:36 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	255307	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	1123370	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.10	164	784367	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1780520	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	1565687	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	1405420	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	20999	4.02	ng/uL	0.00
5) Phenol-d5	6.65	99	470060	24.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	271926	25.87	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	423604	26.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	423979	24.30	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	222658	28.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	260334	30.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	478937	24.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	528979	24.73	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	1566576	25.49	ng/ul	0.00
47) Acenaphthylene-d8	13.79	160	1953400	27.62	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	249359	24.31	ng/ul	0.00
58) Fluorene-d10	15.10	176	1440463	26.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	221457	21.79	ng/ul	0.00
71) Anthracene-d10	16.94	188	2287714	27.63	ng/ul	0.00
79) Pyrene-d10	19.25	212	2556422	30.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	1985185	27.23	ng/ul	0.00


Target Compounds					Qvalue
6) Phenol	6.67	94	50024	2.601 ng/ul	93
45) Dimethylphthalate	13.57	163	369442	5.913 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM024588.D
Acq On : 22 Jan 2020 18:57
Operator : JU
Sample : L1118-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GASK3

Quant Time: Jan 23 01:25:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 23 01:22:36 2020
Response via : Initial Calibration

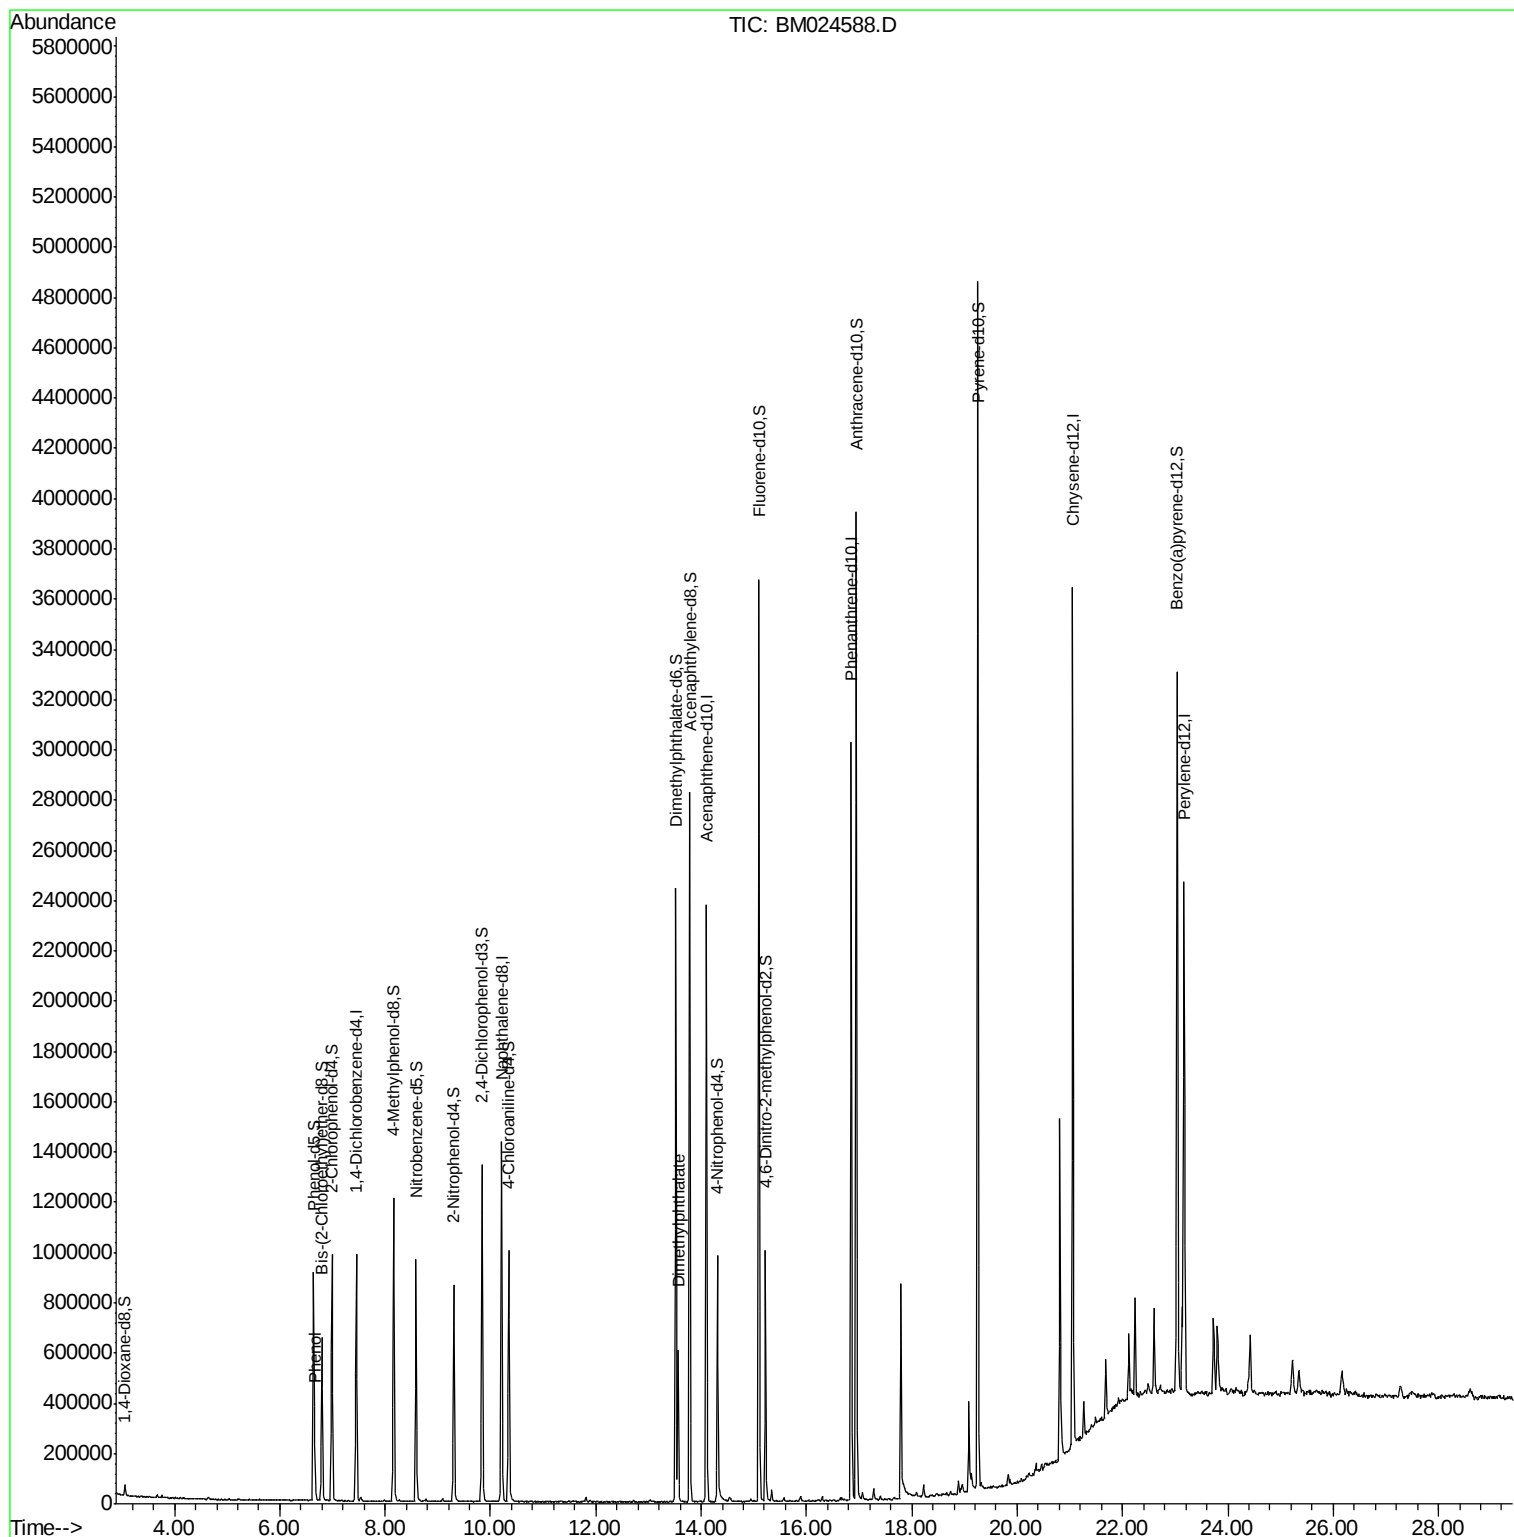

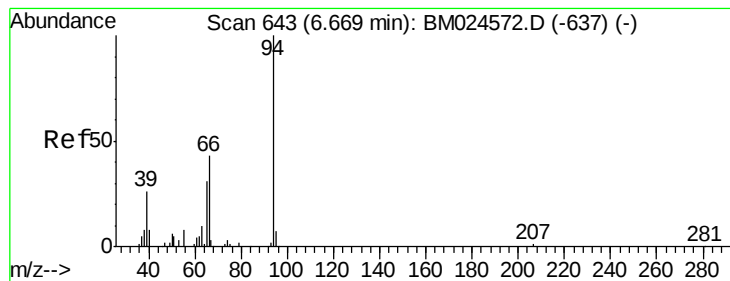

#6

Phenol

Concen: 2.601 ng/ul

RT: 6.67 min Scan# 643

Delta R.T. -0.00 min

Lab File: BM024588.D

Acq: 22 Jan 2020 18:57

Instrument :

BNA_M

ClientSampleId :

GASK3


Tgt Ion: 94 Resp: 50024

Ion Ratio Lower Upper

94 100

65 28.2 26.7 40.1




66 43.4 38.1 57.1

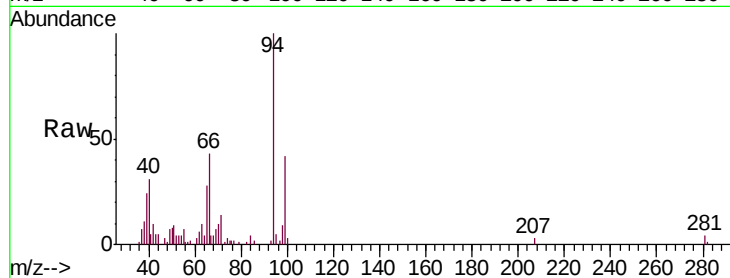

Abundance Ion 94.00 (93.70 to 94.70): BM024572.D (-637) (-)

Ion 65.00 (64.70 to 65.70): BM024572.D (-637) (-)

Ion 66.00 (65.70 to 66.70): BM024572.D (-637) (-)

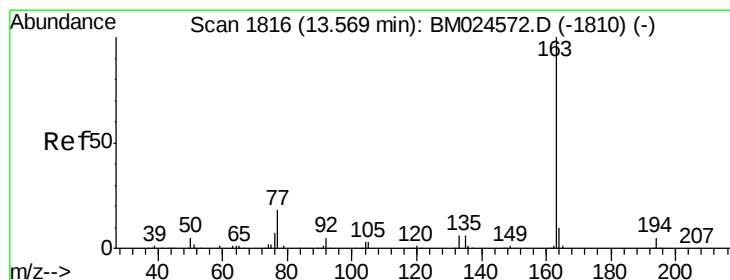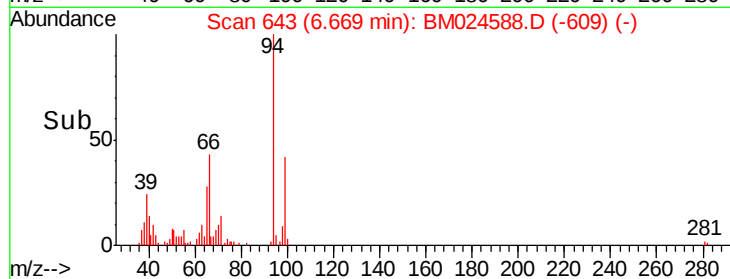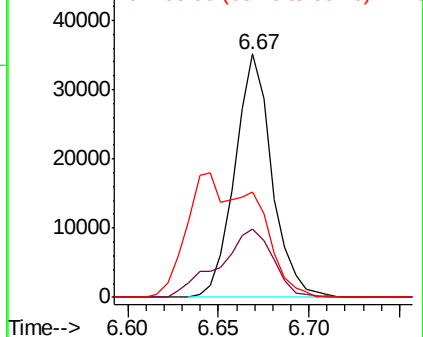

#45

Dimethylphthalate

Concen: 5.913 ng/ul

RT: 13.57 min Scan# 1816

Delta R.T. -0.00 min

Lab File: BM024588.D

Acq: 22 Jan 2020 18:57


Tgt Ion: 163 Resp: 369442

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 9.6 8.0 12.0

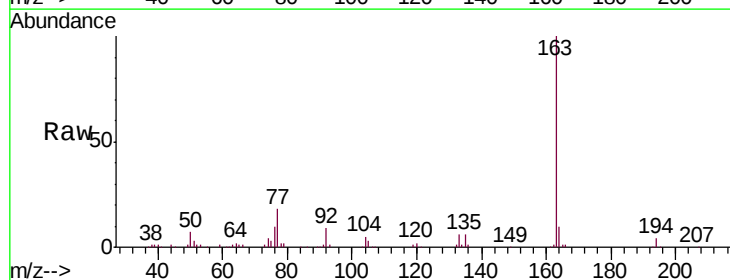

Abundance Ion 163.00 (162.70 to 163.70): BM024572.D (-1810) (-)

Ion 194.00 (193.70 to 194.70): BM024572.D (-1810) (-)

Ion 164.00 (163.70 to 164.70): BM024572.D (-1810) (-)

