

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012323\
 Data File : BM038507.D
 Acq On : 23 Jan 2023 12:30
 Operator : CG/JU
 Sample : PB150201BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150201BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038507.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	311	317	329	rBV	657085	866605	24.43%	4.399%
2	5.522	390	397	412	rBV	1868615	2660156	75.00%	13.503%
3	7.134	664	671	688	rBV	1654495	2473353	69.73%	12.555%
4	7.969	806	813	822	rBV	281530	433716	12.23%	2.202%
5	9.139	1005	1012	1027	rBV	905478	1467511	41.37%	7.449%
6	10.775	1283	1290	1301	rBV	296541	494835	13.95%	2.512%
7	13.227	1700	1707	1719	rBV	2337319	3175771	89.54%	16.120%
8	14.604	1934	1941	1948	rBV	397354	568820	16.04%	2.887%
9	16.086	2187	2193	2204	rBV	1616069	2162335	60.96%	10.976%
10	17.345	2399	2407	2416	rBV	429498	599902	16.91%	3.045%
11	19.956	2845	2851	2859	rBV	3155107	3546893	100.00%	18.004%
12	21.515	3112	3116	3125	rBV	445230	585164	16.50%	2.970%
13	23.933	3521	3527	3536	rBV2	341291	665148	18.75%	3.376%




Sum of corrected areas: 19700209

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012323\
Data File : BM038507.D
Acq On : 23 Jan 2023 12:30
Operator : CG/JU
Sample : PB150201BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150201BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

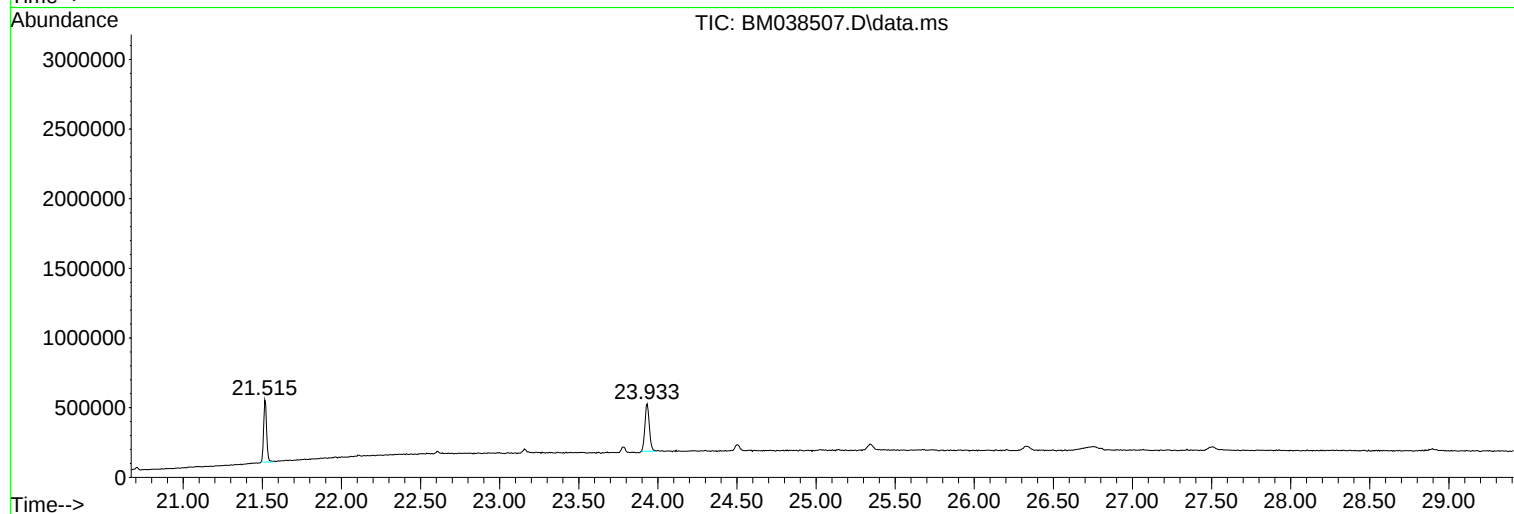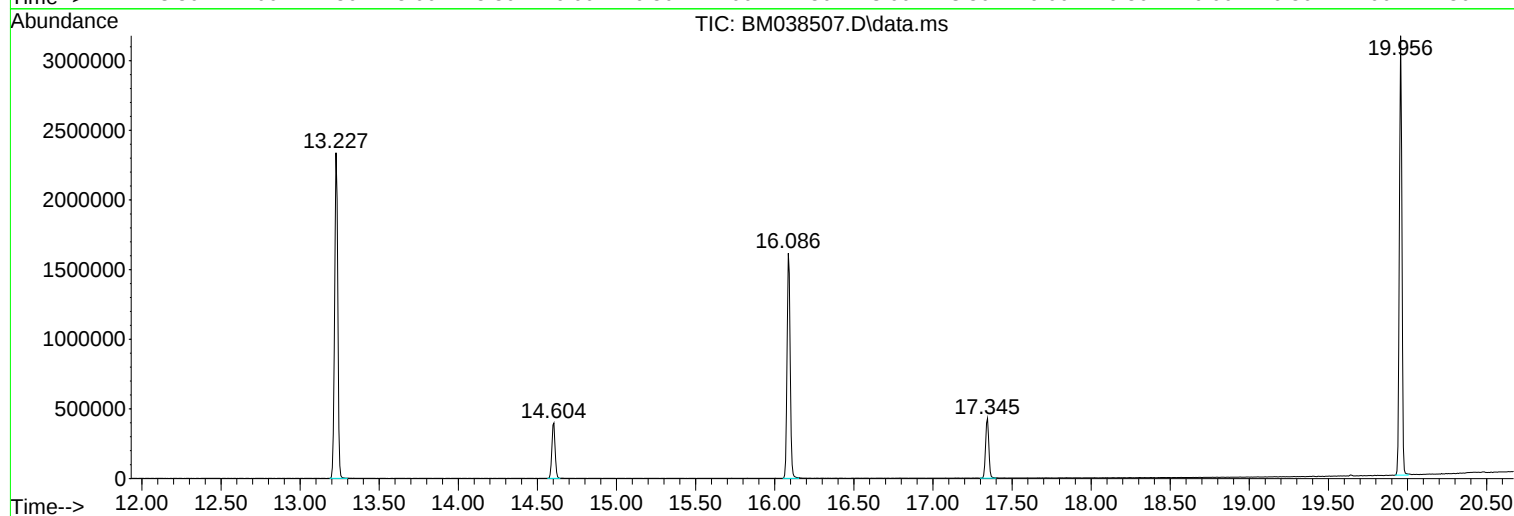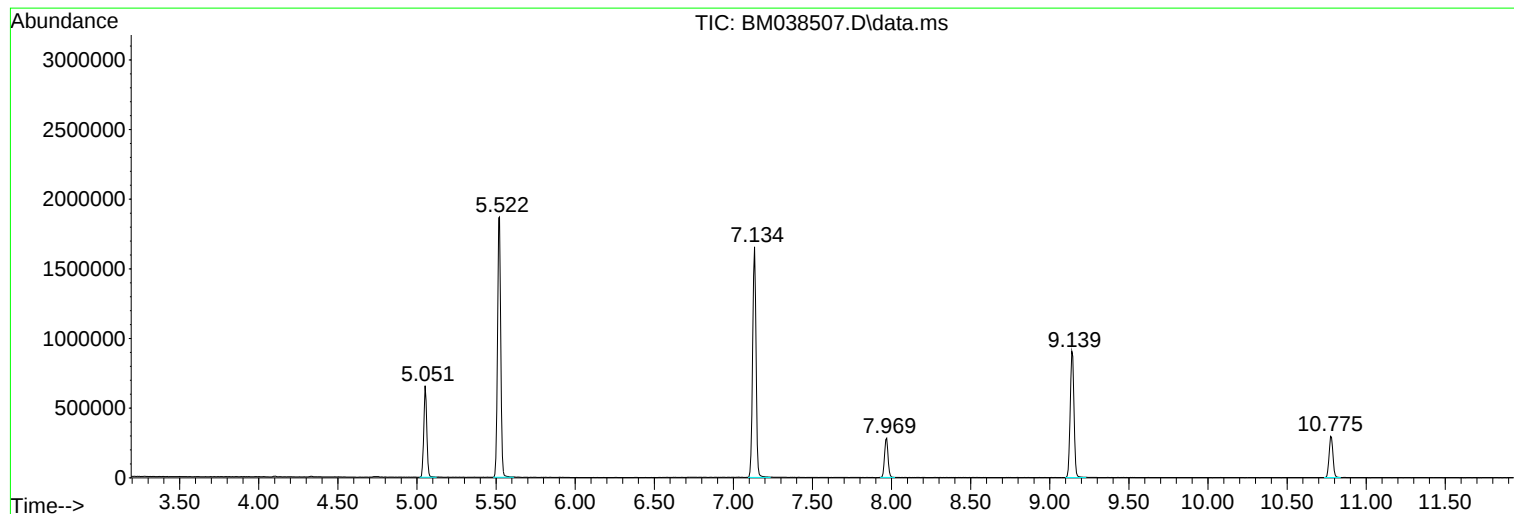

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012323\
Data File : BM038507.D
Acq On : 23 Jan 2023 12:30
Operator : CG/JU
Sample : PB150201BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150201BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.051	39.96 ng	866605	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Acetamide, N-(cyanomethyl)-	98	C4H6N2O	004814-80-6	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

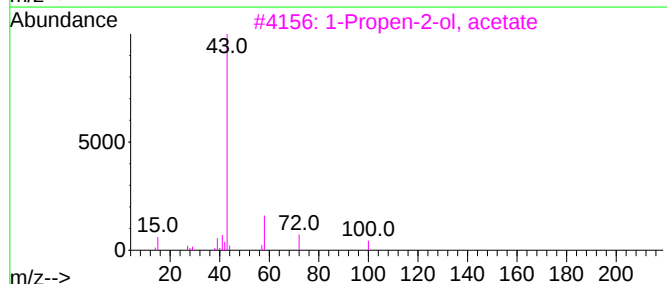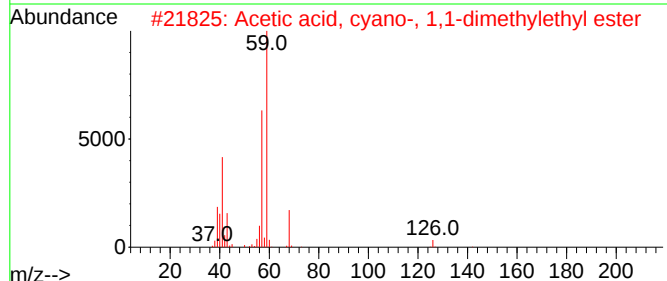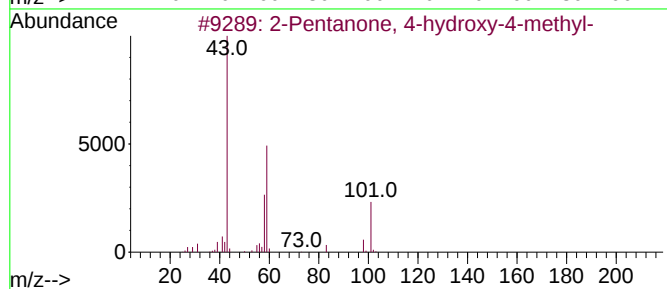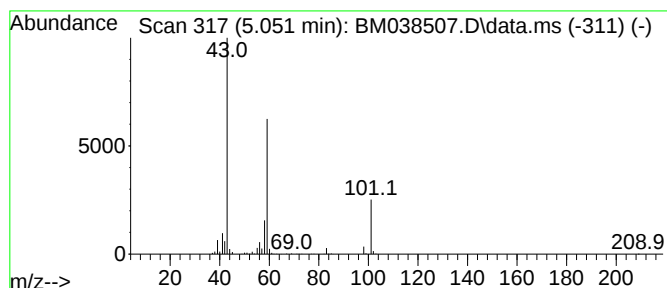

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012323\
Data File : BM038507.D
Acq On : 23 Jan 2023 12:30
Operator : CG/JU
Sample : PB150201BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150201BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.051	40.0	ng	866605	1	7.969	433716	20.0