

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033839.D
 Acq On : 24 Jan 2022 16:02
 Operator : CG/JU
 Sample : PB142204BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK204

Quant Time: Jan 24 16:55:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	1909	0.400	ng/ul	0.00
4) Naphthalene-d8	10.755	136	6753	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.579	164	4019	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.316	188	7718	0.400	ng/ul	0.00
17) Chrysene-d12	21.484	240	5834	0.400	ng/ul	# 0.00
23) Perylene-d12	23.882	264	6346	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	13794	6.912	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	3791	0.407	ng/ul	0.00
18) Fluoranthene-d10	19.337	212	7731	0.430	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.569	166	1251	0.076	ng/ul#	18
20) Pyrene	19.700	202	1317	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.729	252	2669	0.108	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033839.D
Acq On : 24 Jan 2022 16:02
Operator : CG/JU
Sample : PB142204BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK204

Quant Time: Jan 24 16:55:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration




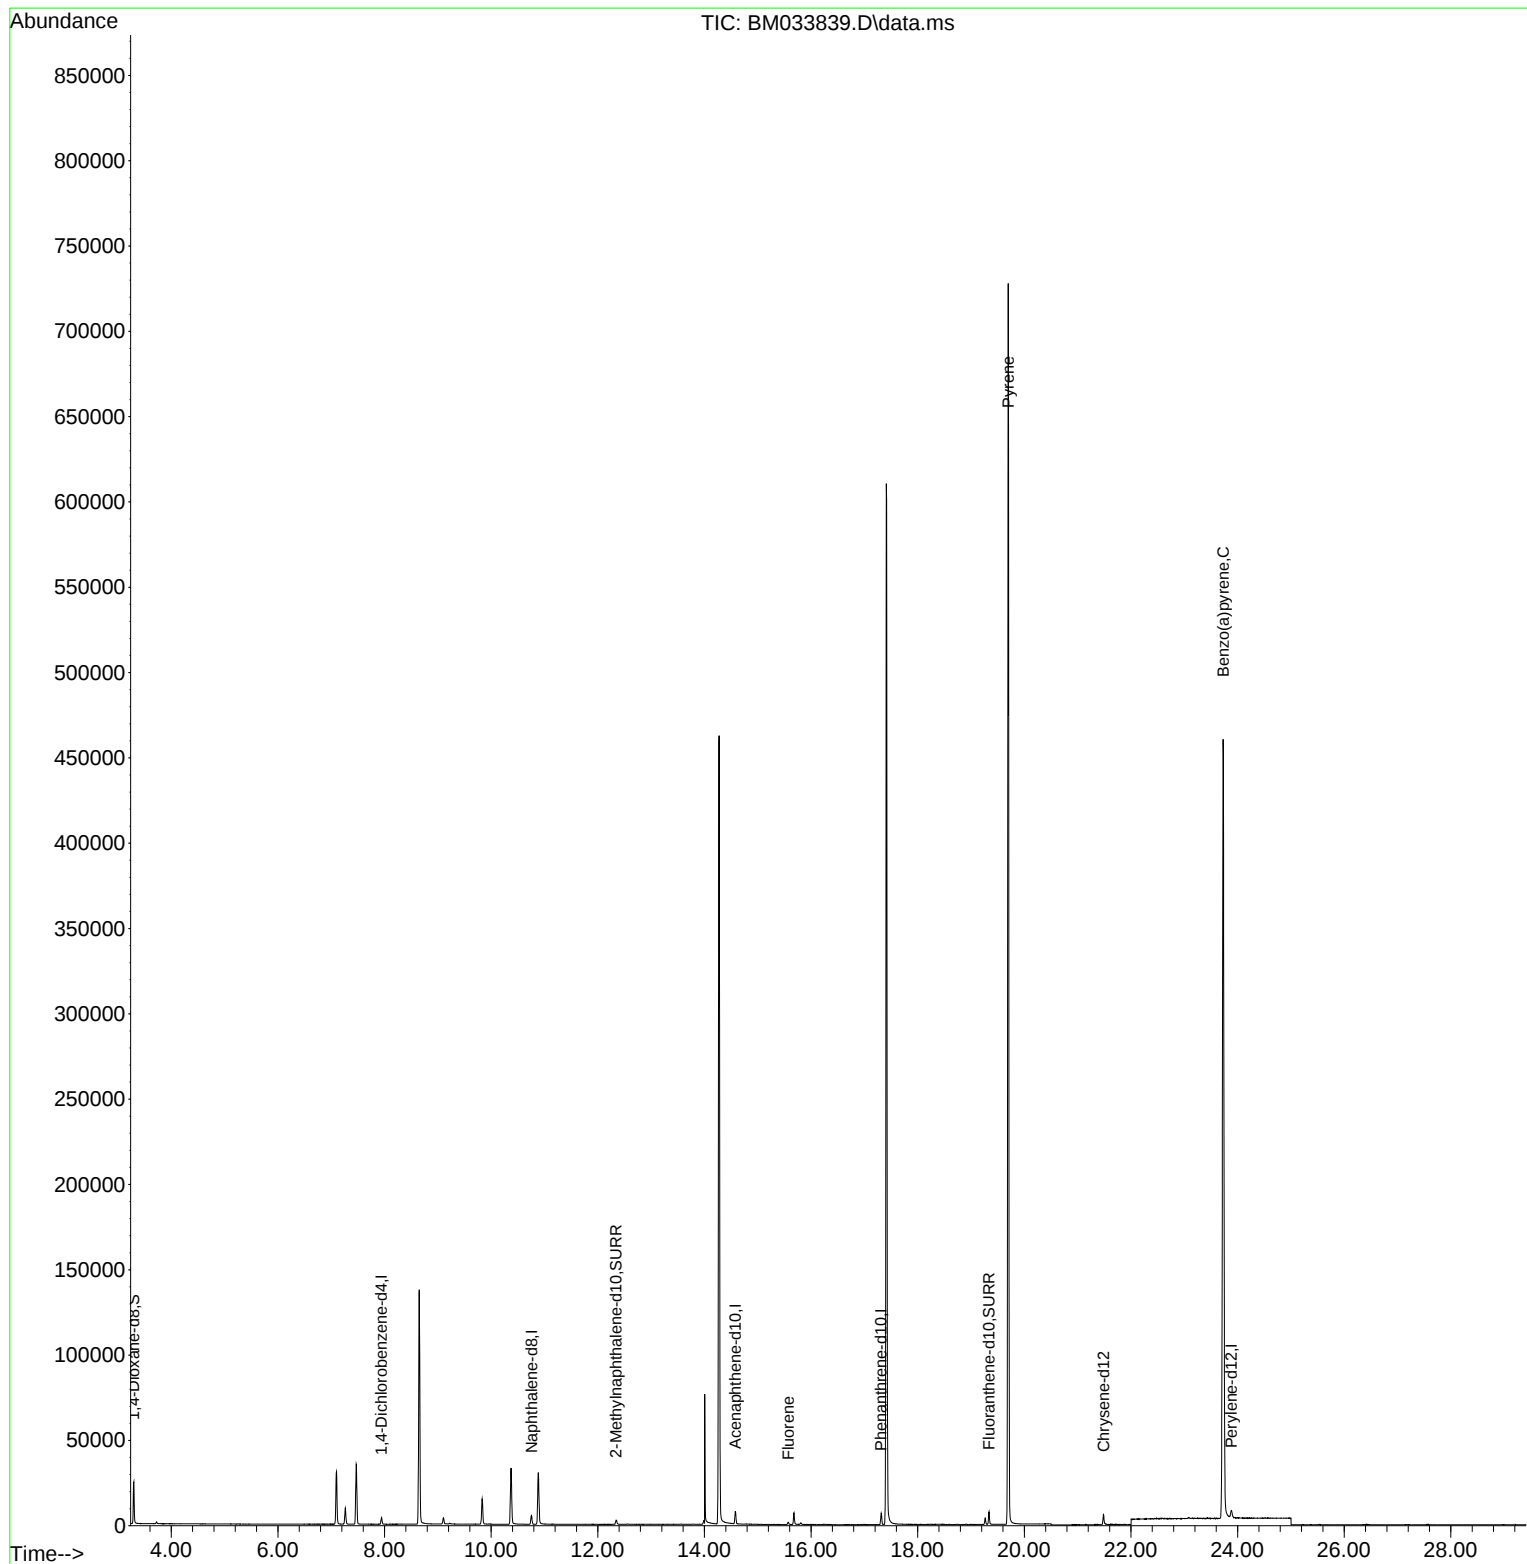


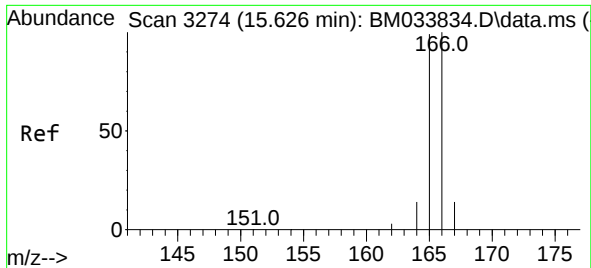

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.569 min Scan# 31
Delta R.T. -0.057 min
Lab File: BM033839.D
Acq: 24 Jan 2022 16:02




Instrument :
BNA_M
ClientSampleId :
SBLK204


Tgt Ion:166 Resp: 1251
Ion Ratio Lower Upper
166 100
165 11.0 81.1 121.7#
167 35.4 14.9 22.3#

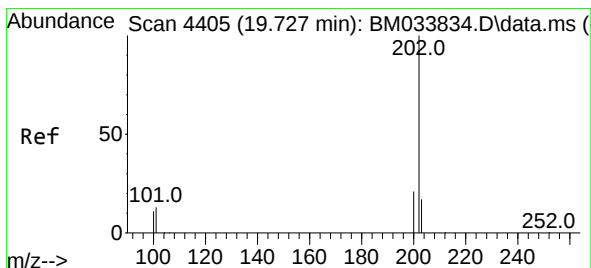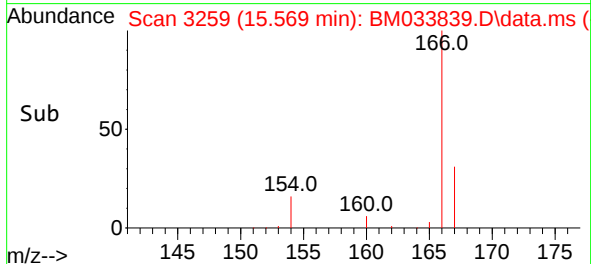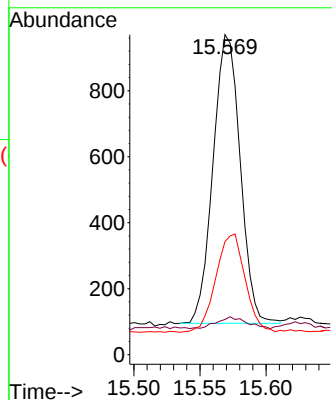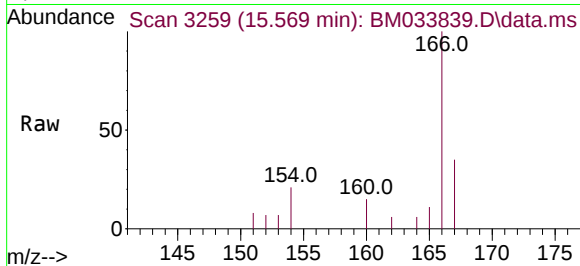

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.700 min Scan# 4398
Delta R.T. -0.027 min
Lab File: BM033839.D
Acq: 24 Jan 2022 16:02


Tgt Ion:202 Resp: 1317
Ion Ratio Lower Upper
202 100
101 175.5 9.3 13.9#
100 1279.6 7.8 11.6#

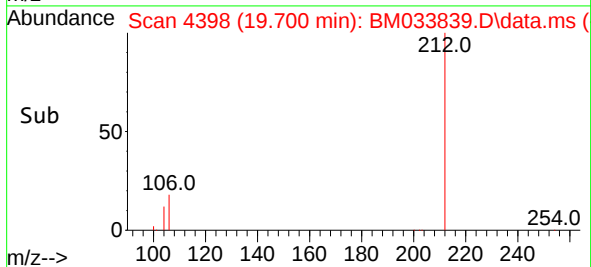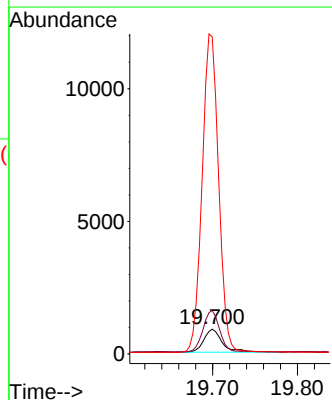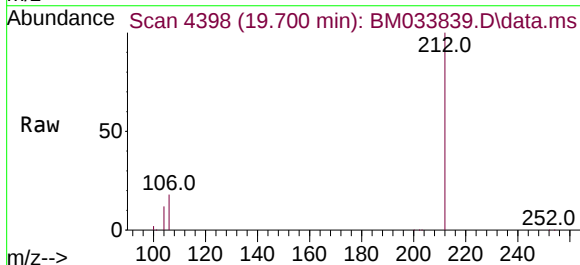

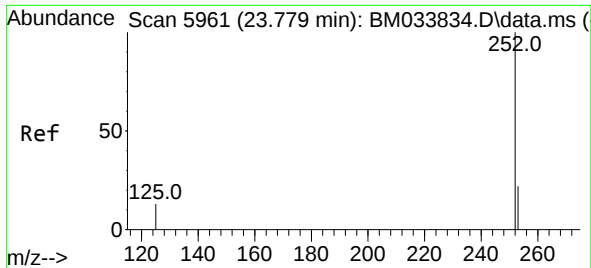

#26
 Benzo(a)pyrene
 Concen: 0.108 ng/ul
 RT: 23.729 min Scan# 5941
 Delta R.T. -0.049 min
 Lab File: BM033839.D
 Acq: 24 Jan 2022 16:02

Instrument :
 BNA_M
 ClientSampleId :
 SBLK204

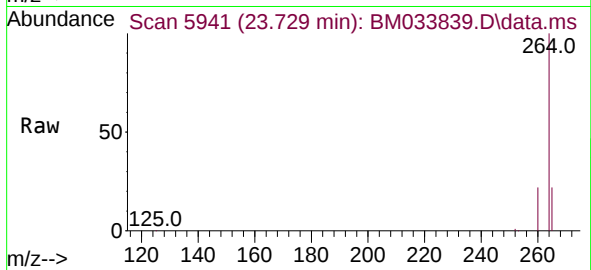

Tgt Ion:252 Resp: 2669
 Ion Ratio Lower Upper
 252 100
 253 53.9 32.0 48.0#
 125 49.7 14.5 21.7#

