




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033843.D
 Acq On : 24 Jan 2022 18:26
 Operator : CG/JU
 Sample : N1199-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q09

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:13:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :Yogesh Patel 02/01/2022

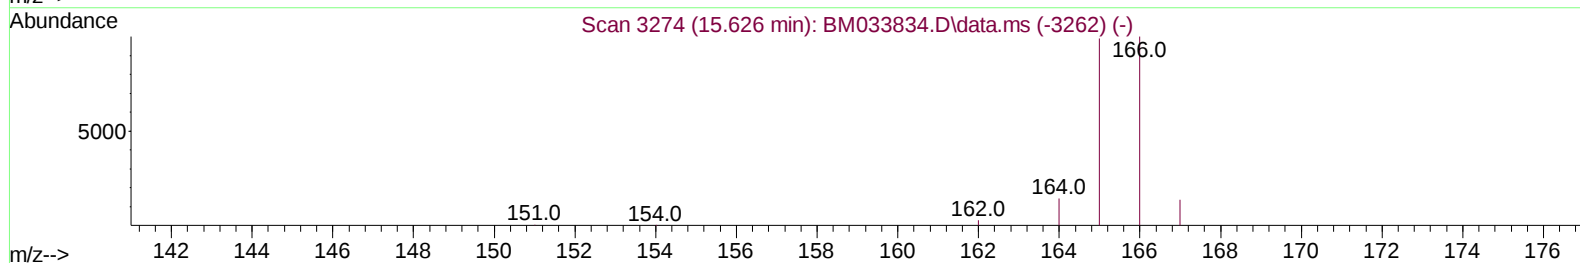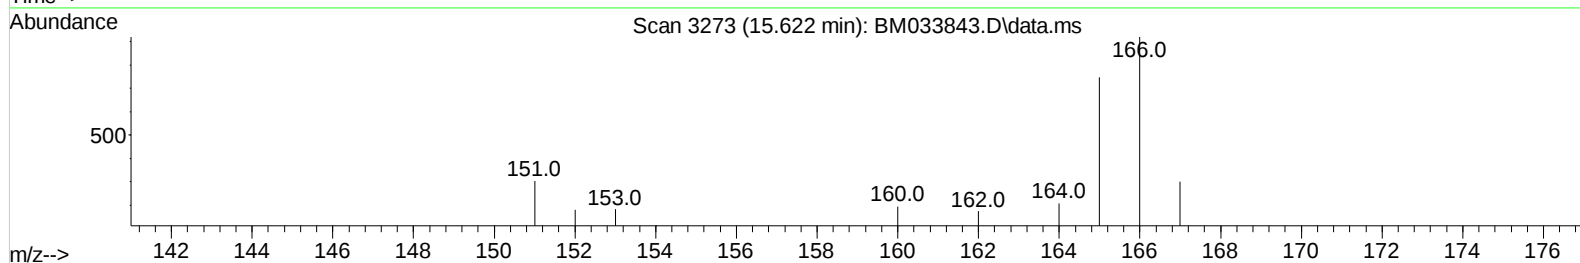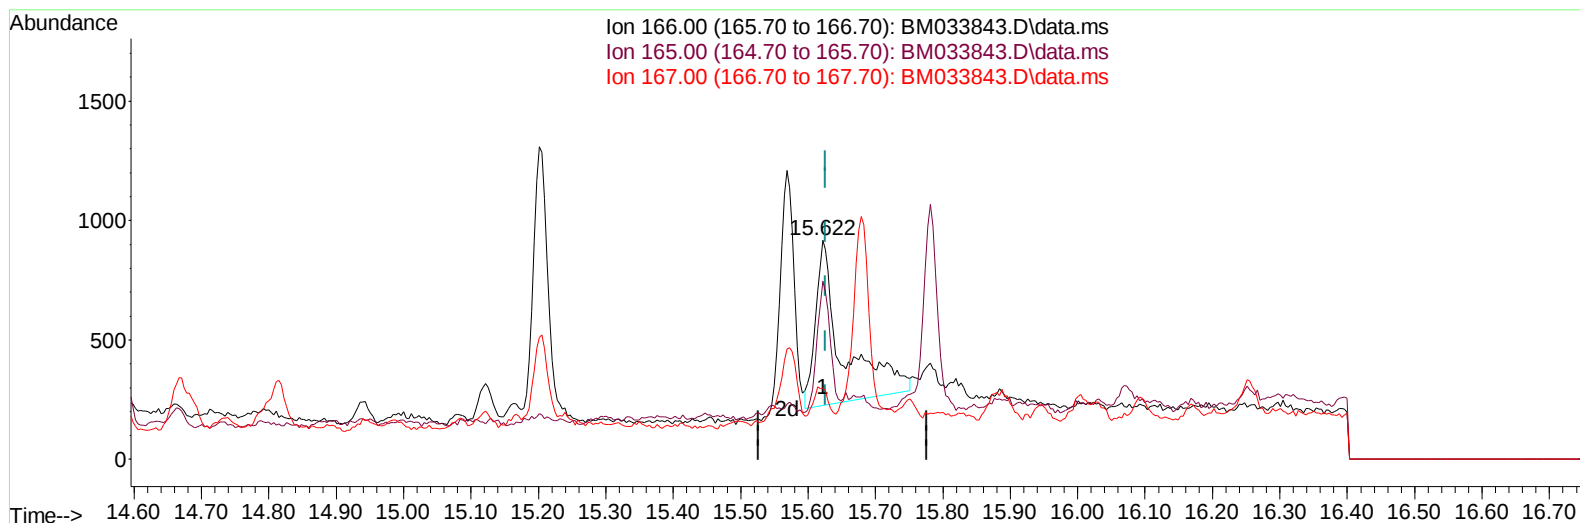

TIC: BM033843.D\data.ms

(12) Fluorene

15.622min (-0.004) 0.10 ng/u1

response 1925

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	101.40	81.18
167.00	18.60	32.64#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033843.D
Acq On : 24 Jan 2022 18:26
Operator : CG/JU
Sample : N1199-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q09

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:13:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :Yogesh Patel 02/01/2022

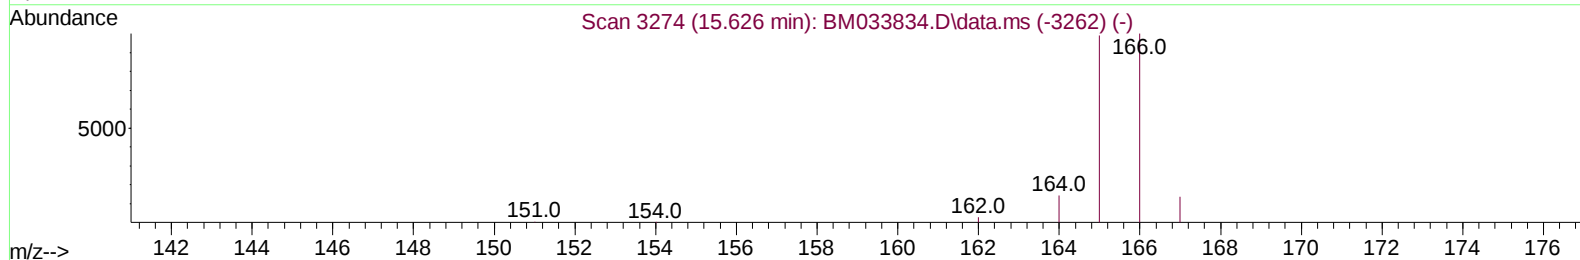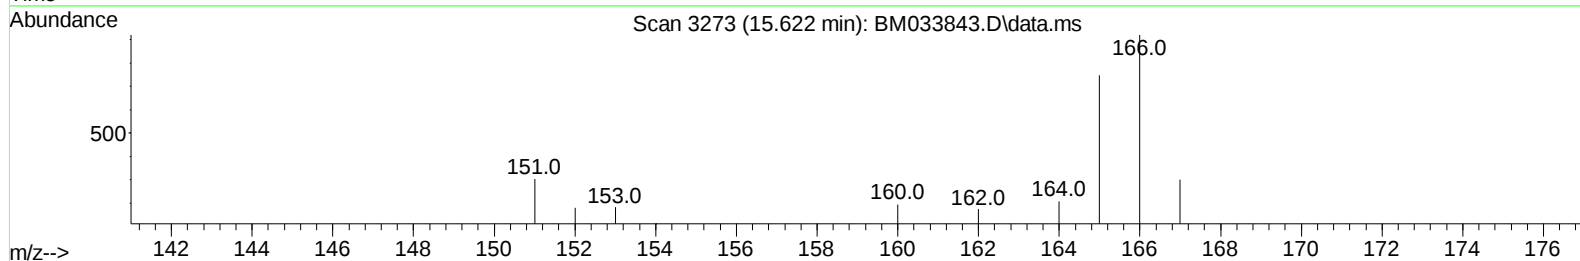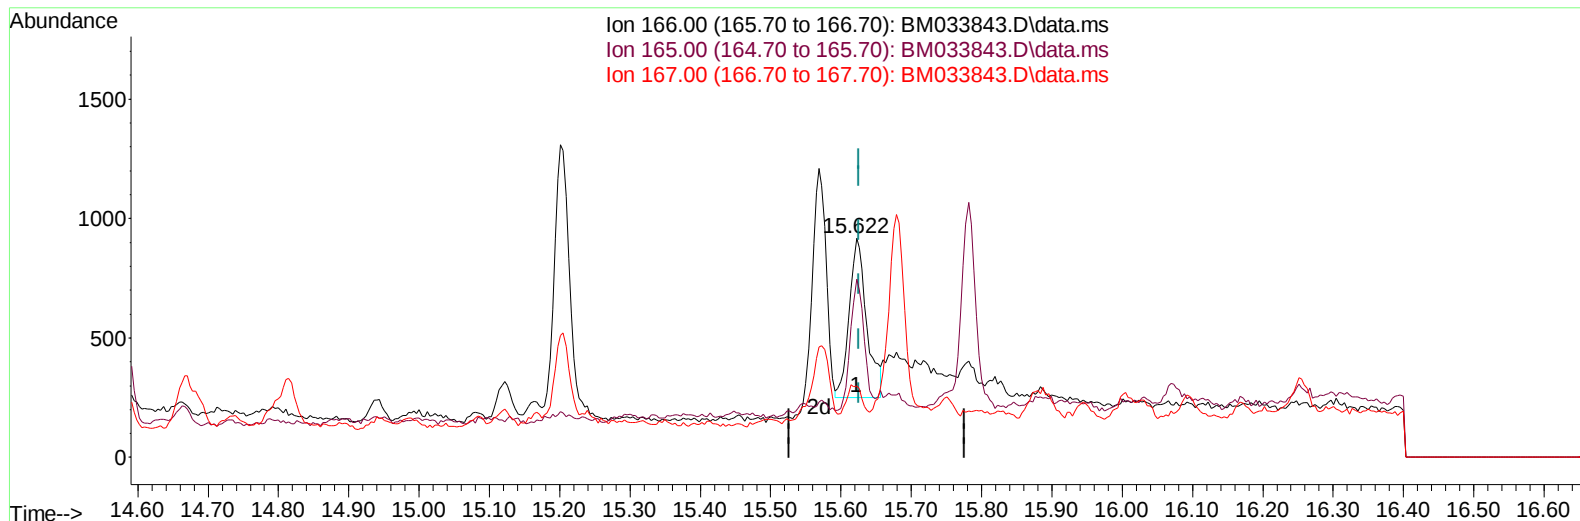

TIC: BM033843.D\data.ms

(12) Fluorene

15.622min (-0.004) 0.06 ng/ul m

response 1142

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	101.40	81.18
167.00	18.60	32.64#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033843.D
 Acq On : 24 Jan 2022 18:26
 Operator : CG/JU
 Sample : N1199-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q09

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:13:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :Yogesh Patel 02/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	1975	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	7186	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.579	164	4555	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.316	188	8681	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.482	240	6894	0.400	ng/ul	# 0.00
23) Perylene-d12	23.885	264	7503	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	8845	4.284	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	4558	0.460	ng/ul	0.00
18) Fluoranthene-d10	19.337	212	10036	0.473	ng/ul	0.00
Target Compounds				Qvalue		
12) Fluorene	15.622	166	1142m	0.061	ng/ul	
14) Pentachlorophenol	16.965	266	17928	4.495	ng/ul	97
15) Phenanthrene	17.358	178	758	0.027	ng/ul#	44
16) Anthracene	17.448	178	2067	0.080	ng/ul#	84
19) Fluoranthene	19.364	202	880	0.028	ng/ul#	31

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033843.D
Acq On : 24 Jan 2022 18:26
Operator : CG/JU
Sample : N1199-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q09

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:13:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :Yogesh Patel 02/01/2022

