




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033845.D
 Acq On : 24 Jan 2022 19:37
 Operator : CG/JU
 Sample : N1199-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q10

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:20:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :Yogesh Patel 02/01/2022

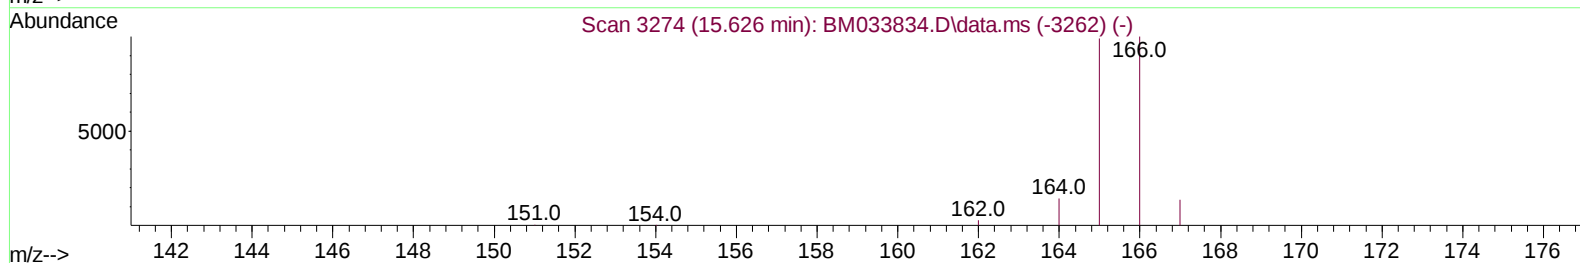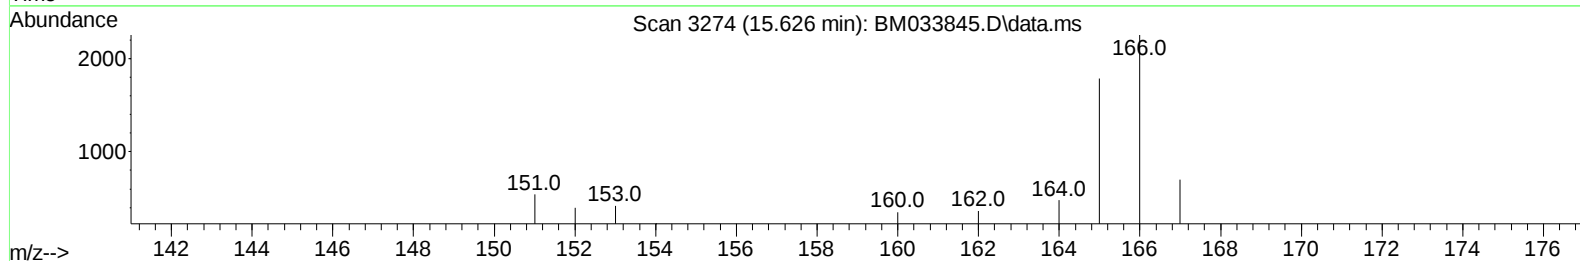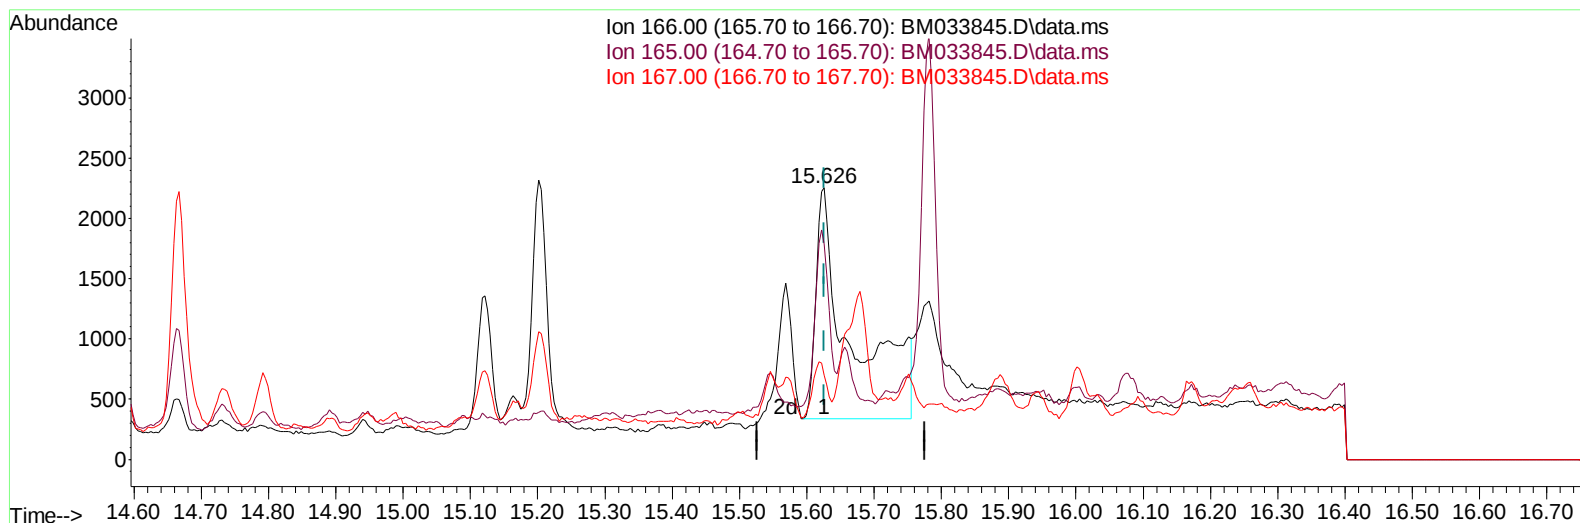

TIC: BM033845.D\data.ms

(12) Fluorene

15.626min (-0.000) 0.30 ng/u1

response 6901

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	101.40	79.26#
167.00	18.60	31.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033845.D
 Acq On : 24 Jan 2022 19:37
 Operator : CG/JU
 Sample : N1199-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q10

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:20:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :Yogesh Patel 02/01/2022

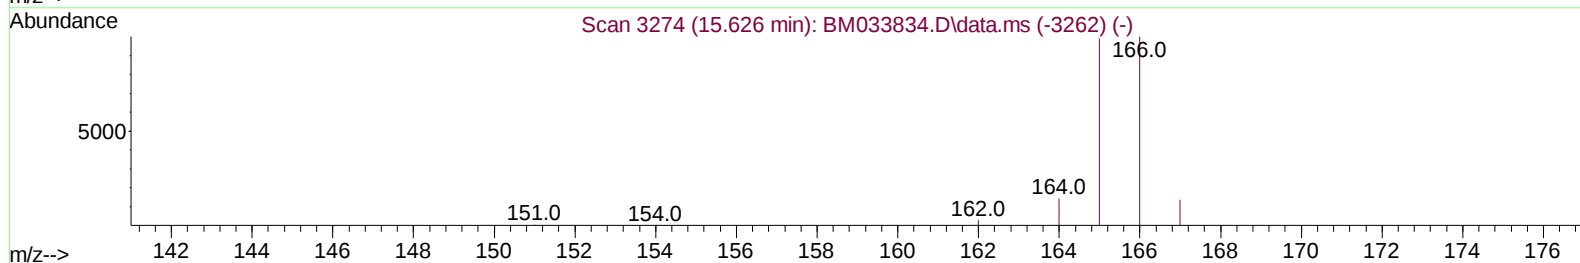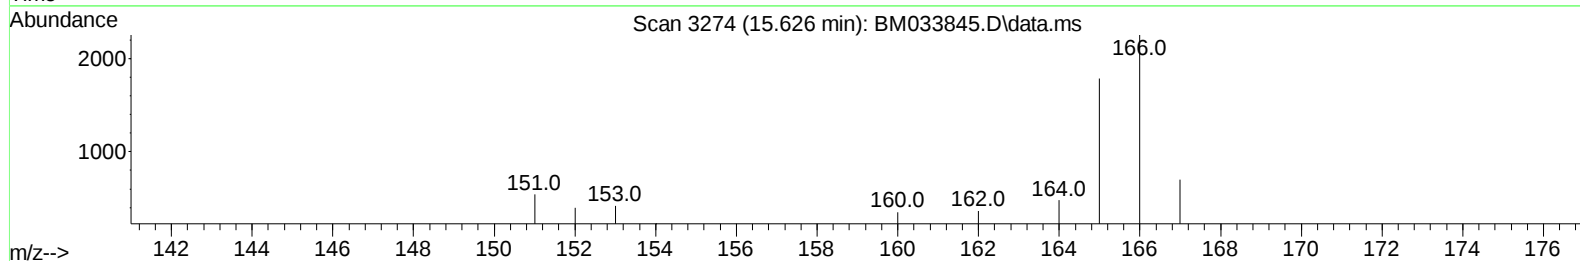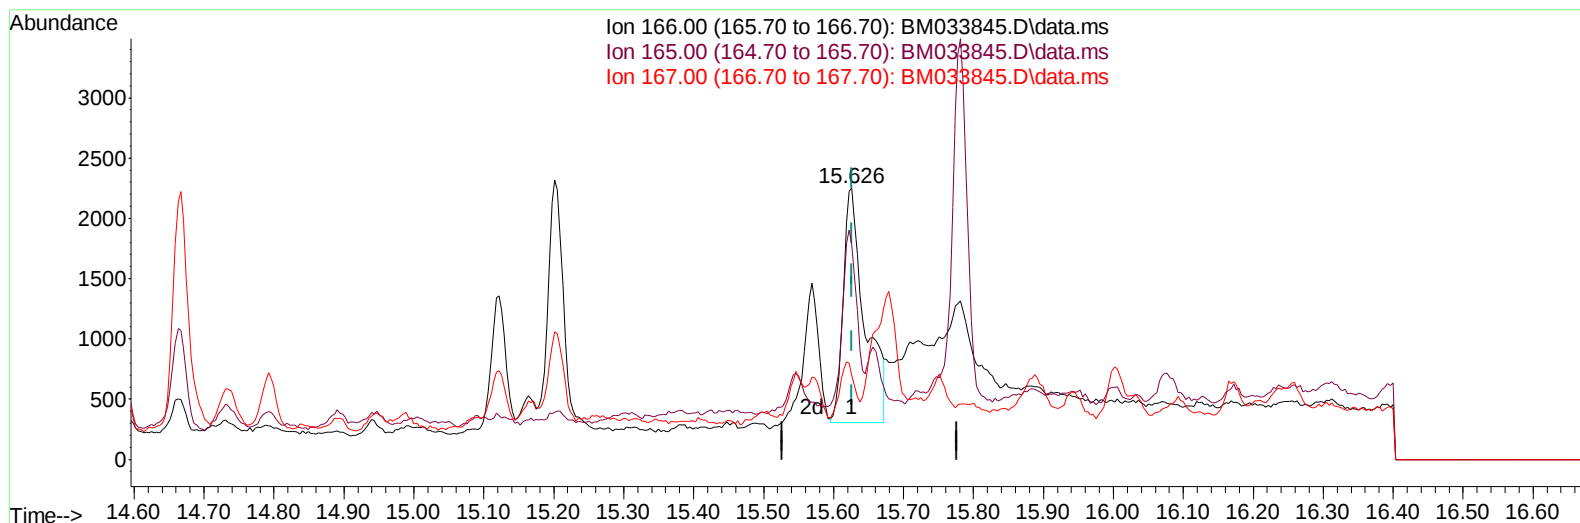

TIC: BM033845.D\data.ms

(12) Fluorene

15.626min (-0.000) 0.18 ng/ul m

response 4160

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	101.40	79.26#
167.00	18.60	31.04#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033845.D
 Acq On : 24 Jan 2022 19:37
 Operator : CG/JU
 Sample : N1199-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q10

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :Yogesh Patel 02/01/2022

Quant Time: Jan 25 02:20:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.943	152		2228	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136		8076	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.580	164		5622	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.316	188		9404	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.480	240		7373	0.400	ng/ul	# 0.00
23) Perylene-d12	23.883	264		8021	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.296	96		10276	4.412	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.344	152		4940	0.444	ng/ul	0.00
18) Fluoranthene-d10	19.334	212		10136	0.446	ng/ul	0.00
Target Compounds							Qvalue
12) Fluorene	15.626	166		4160m	0.181	ng/ul	
14) Pentachlorophenol	16.969	266		174859	40.468	ng/ul	97
15) Phenanthrene	17.358	178		981	0.033	ng/ul#	17
16) Anthracene	17.448	178		3768	0.134	ng/ul#	79
19) Fluoranthene	19.365	202		959	0.029	ng/ul#	19

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033845.D
Acq On : 24 Jan 2022 19:37
Operator : CG/JU
Sample : N1199-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q10

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:20:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :Yogesh Patel 02/01/2022

