




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033853.D
Acq On : 25 Jan 2022 00:57
Operator : CG/JU
Sample : N1199-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q13

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:22:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2022
Supervised By :Yogesh Patel 01/31/2022

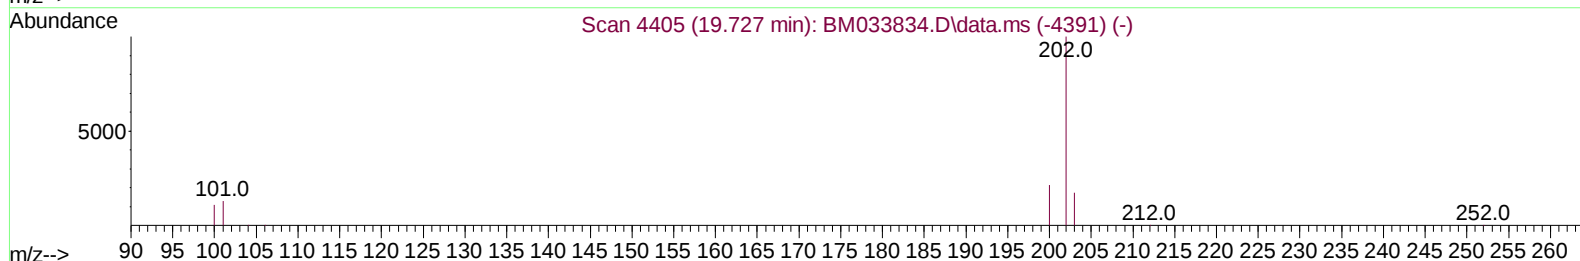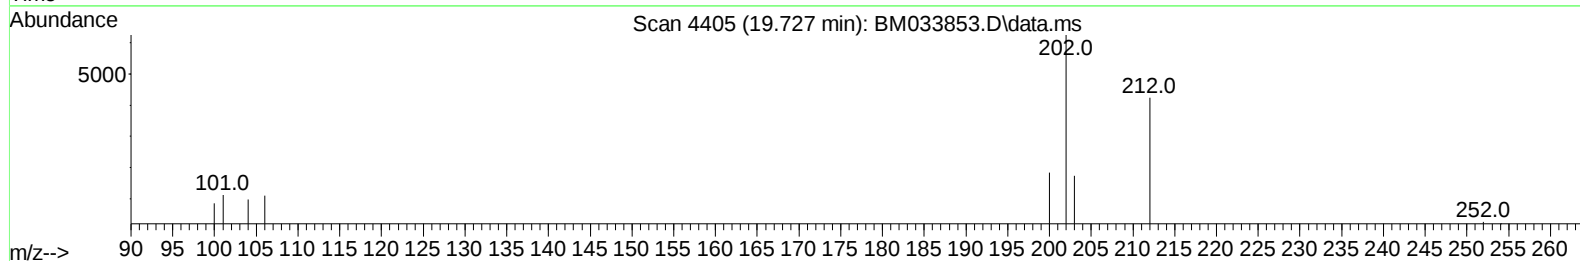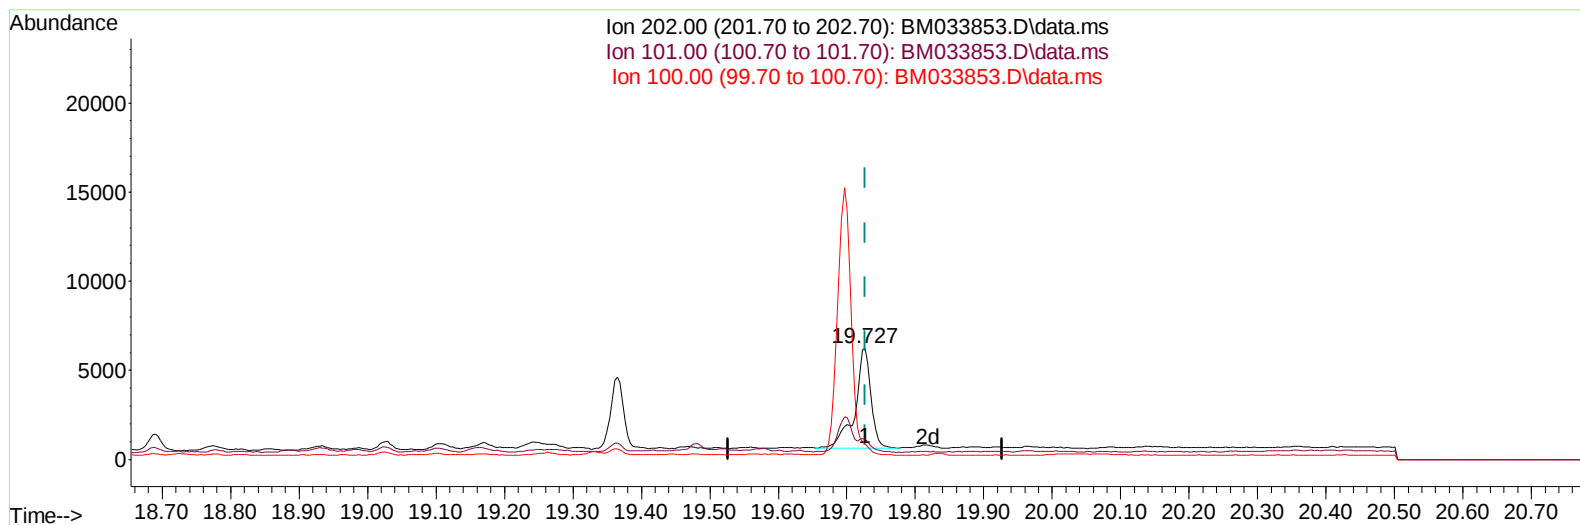

TIC: BM033853.D\data.ms

(20) Pyrene

19.727min (0.000) 0.25 ng/u1

response 9153

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	18.14#
100.00	9.70	13.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033853.D
 Acq On : 25 Jan 2022 00:57
 Operator : CG/JU
 Sample : N1199-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q13

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:22:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2022
 Supervised By :Yogesh Patel 01/31/2022

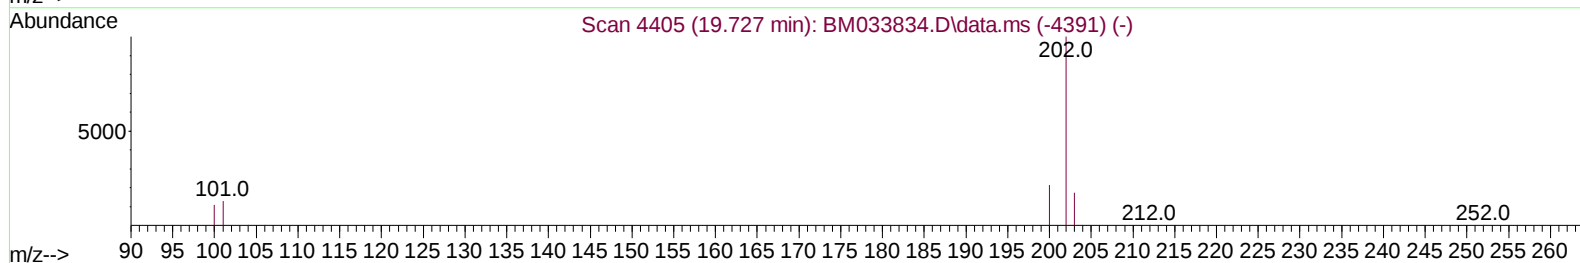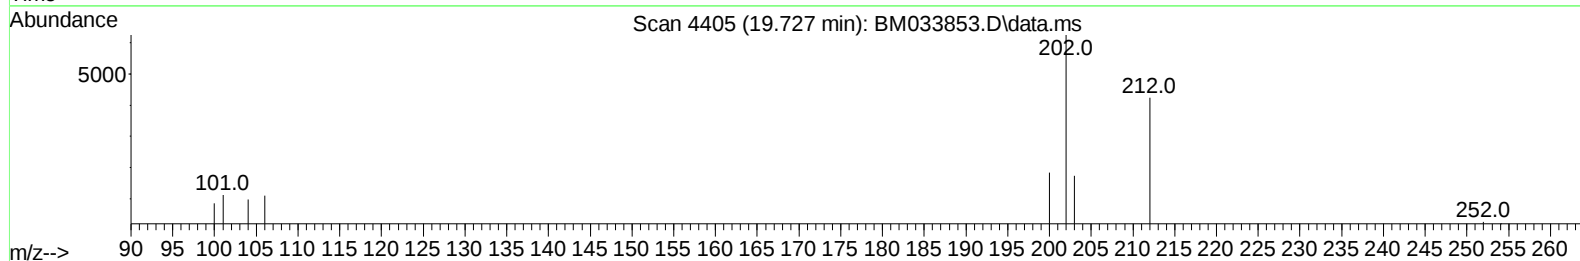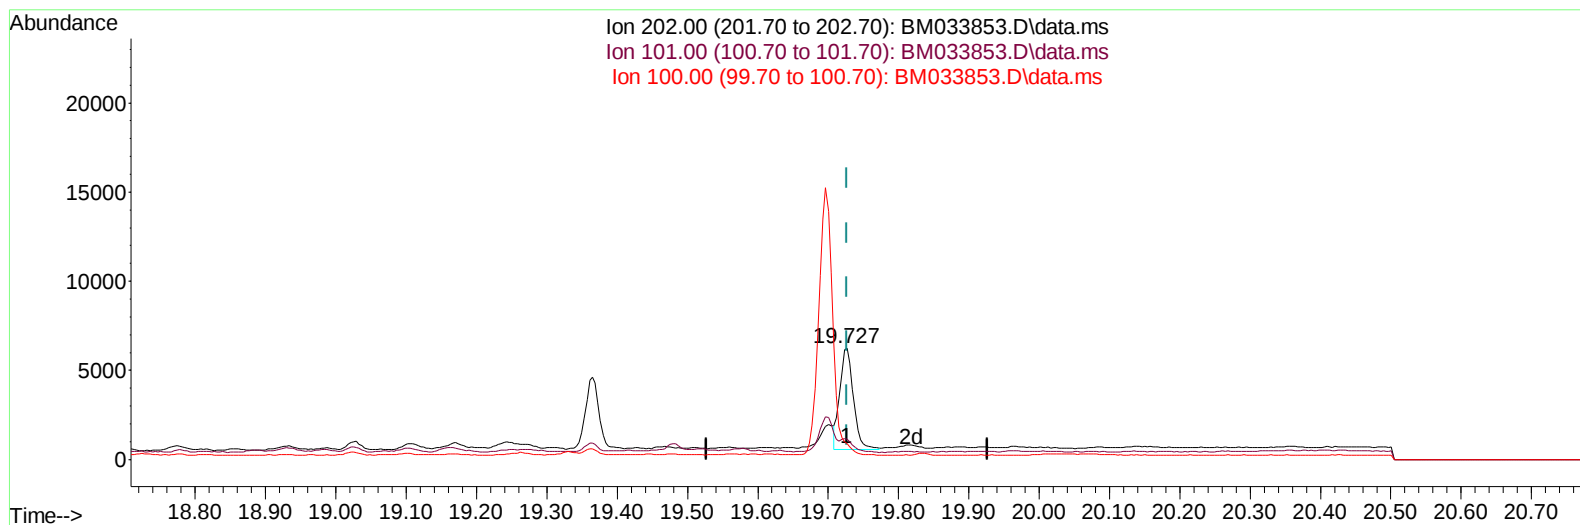

TIC: BM033853.D\data.ms

(20) Pyrene

19.727min (0.000) 0.21 ng/u1 m

response 7671

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	18.14#
100.00	9.70	13.91#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033853.D
 Acq On : 25 Jan 2022 00:57
 Operator : CG/JU
 Sample : N1199-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q13

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:22:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2022
 Supervised By :Yogesh Patel 01/31/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.943	152		2019	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136		7541	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164		6465	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.320	188		10573	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.477	240		7712	0.400	ng/ul	# 0.00
23) Perylene-d12	23.875	264		7993	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.296	96		9399	4.453	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152		4317	0.415	ng/ul	0.00
18) Fluoranthene-d10	19.334	212		11360	0.478	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.330	88		134	0.061	ng/ul#	48
5) Naphthalene	10.806	128		35709	1.723	ng/ul#	94
8) 1-Methylnaphthalene	12.632	142		111257	8.424	ng/ul	99
10) Acenaphthylene	14.299	152		11206	0.388	ng/ul#	60
11) Acenaphthene	14.640	153		28869	1.248	ng/ul	95
12) Fluorene	15.622	166		108095	4.096	ng/ul	96
14) Pentachlorophenol	17.000	266		9487369	1952.934	ng/ul	98
15) Phenanthrene	17.361	178		116679	3.464	ng/ul	95
16) Anthracene	17.448	178		27520	0.873	ng/ul	95
19) Fluoranthene	19.365	202		5428	0.154	ng/ul#	83
20) Pyrene	19.727	202		7671m	0.213	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033853.D
Acq On : 25 Jan 2022 00:57
Operator : CG/JU
Sample : N1199-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q13

Manual IntegrationsAPPROVED

Quant Time: Jan 25 02:22:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2022
Supervised By :Yogesh Patel 01/31/2022

