

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033856.D
 Acq On : 25 Jan 2022 02:44
 Operator : CG/JU
 Sample : N1199-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F09

Quant Time: Jan 25 03:17:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	2180	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	8018	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	4815	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	9645	0.400	ng/ul	0.00
17) Chrysene-d12	21.480	240	7631	0.400	ng/ul	# 0.00
23) Perylene-d12	23.875	264	8112	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	9946	4.364	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.344	152	3935	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.334	212	9637	0.410	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.969	266	933	0.211	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033856.D
Acq On : 25 Jan 2022 02:44
Operator : CG/JU
Sample : N1199-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F09


Quant Time: Jan 25 03:17:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

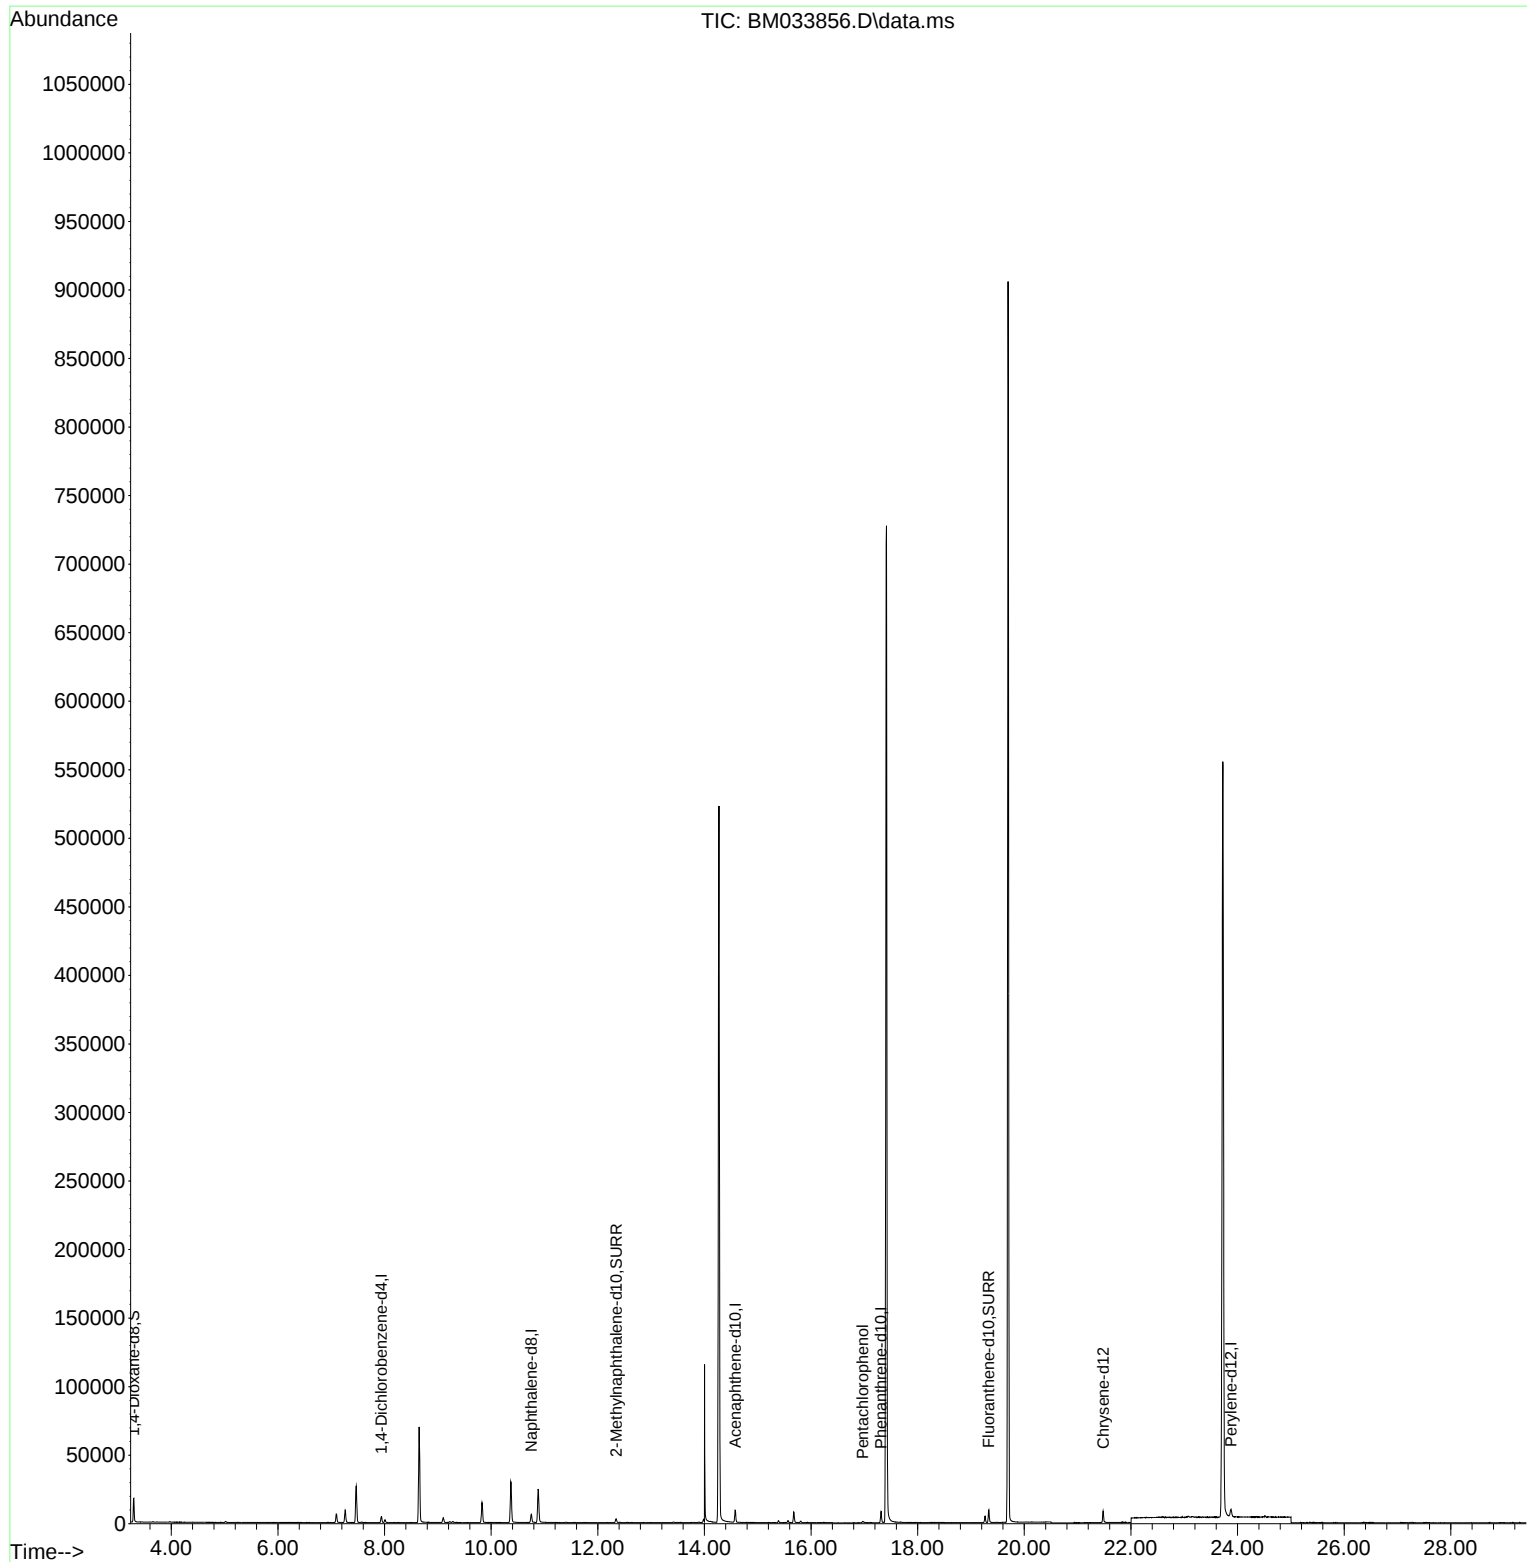

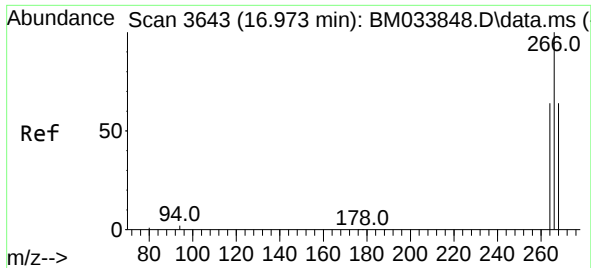

#14
Pentachlorophenol
Concen: 0.211 ng/ul
RT: 16.969 min Scan# 30
Delta R.T. -0.003 min
Lab File: BM033856.D
Acq: 25 Jan 2022 02:44

Instrument :
BNA_M
ClientSampleId :
C0F09

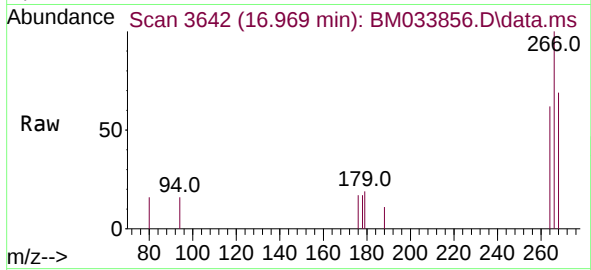

Tgt Ion:266 Resp: 933
Ion Ratio Lower Upper
266 100
264 63.3 51.4 77.0
268 63.7 53.1 79.7

