

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
 Data File : BM033860.D
 Acq On : 25 Jan 2022 10:11
 Operator : CG/JU
 Sample : N1199-15DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q09DL

Quant Time: Jan 25 23:20:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	1795	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	6392	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	3462	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.312	188	6875	0.400	ng/ul	0.00
17) Chrysene-d12	21.482	240	5443	0.400	ng/ul	# 0.00
23) Perylene-d12	23.880	264	5550	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	1043	0.556	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	847	0.096	ng/ul	0.00
18) Fluoranthene-d10	19.334	212	1881	0.112	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.965	266	2929	0.927	ng/ul	98
16) Anthracene	17.448	178	413	0.020	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012422\
Data File : BM033860.D
Acq On : 25 Jan 2022 10:11
Operator : CG/JU
Sample : N1199-15DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q09DL


Quant Time: Jan 25 23:20:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

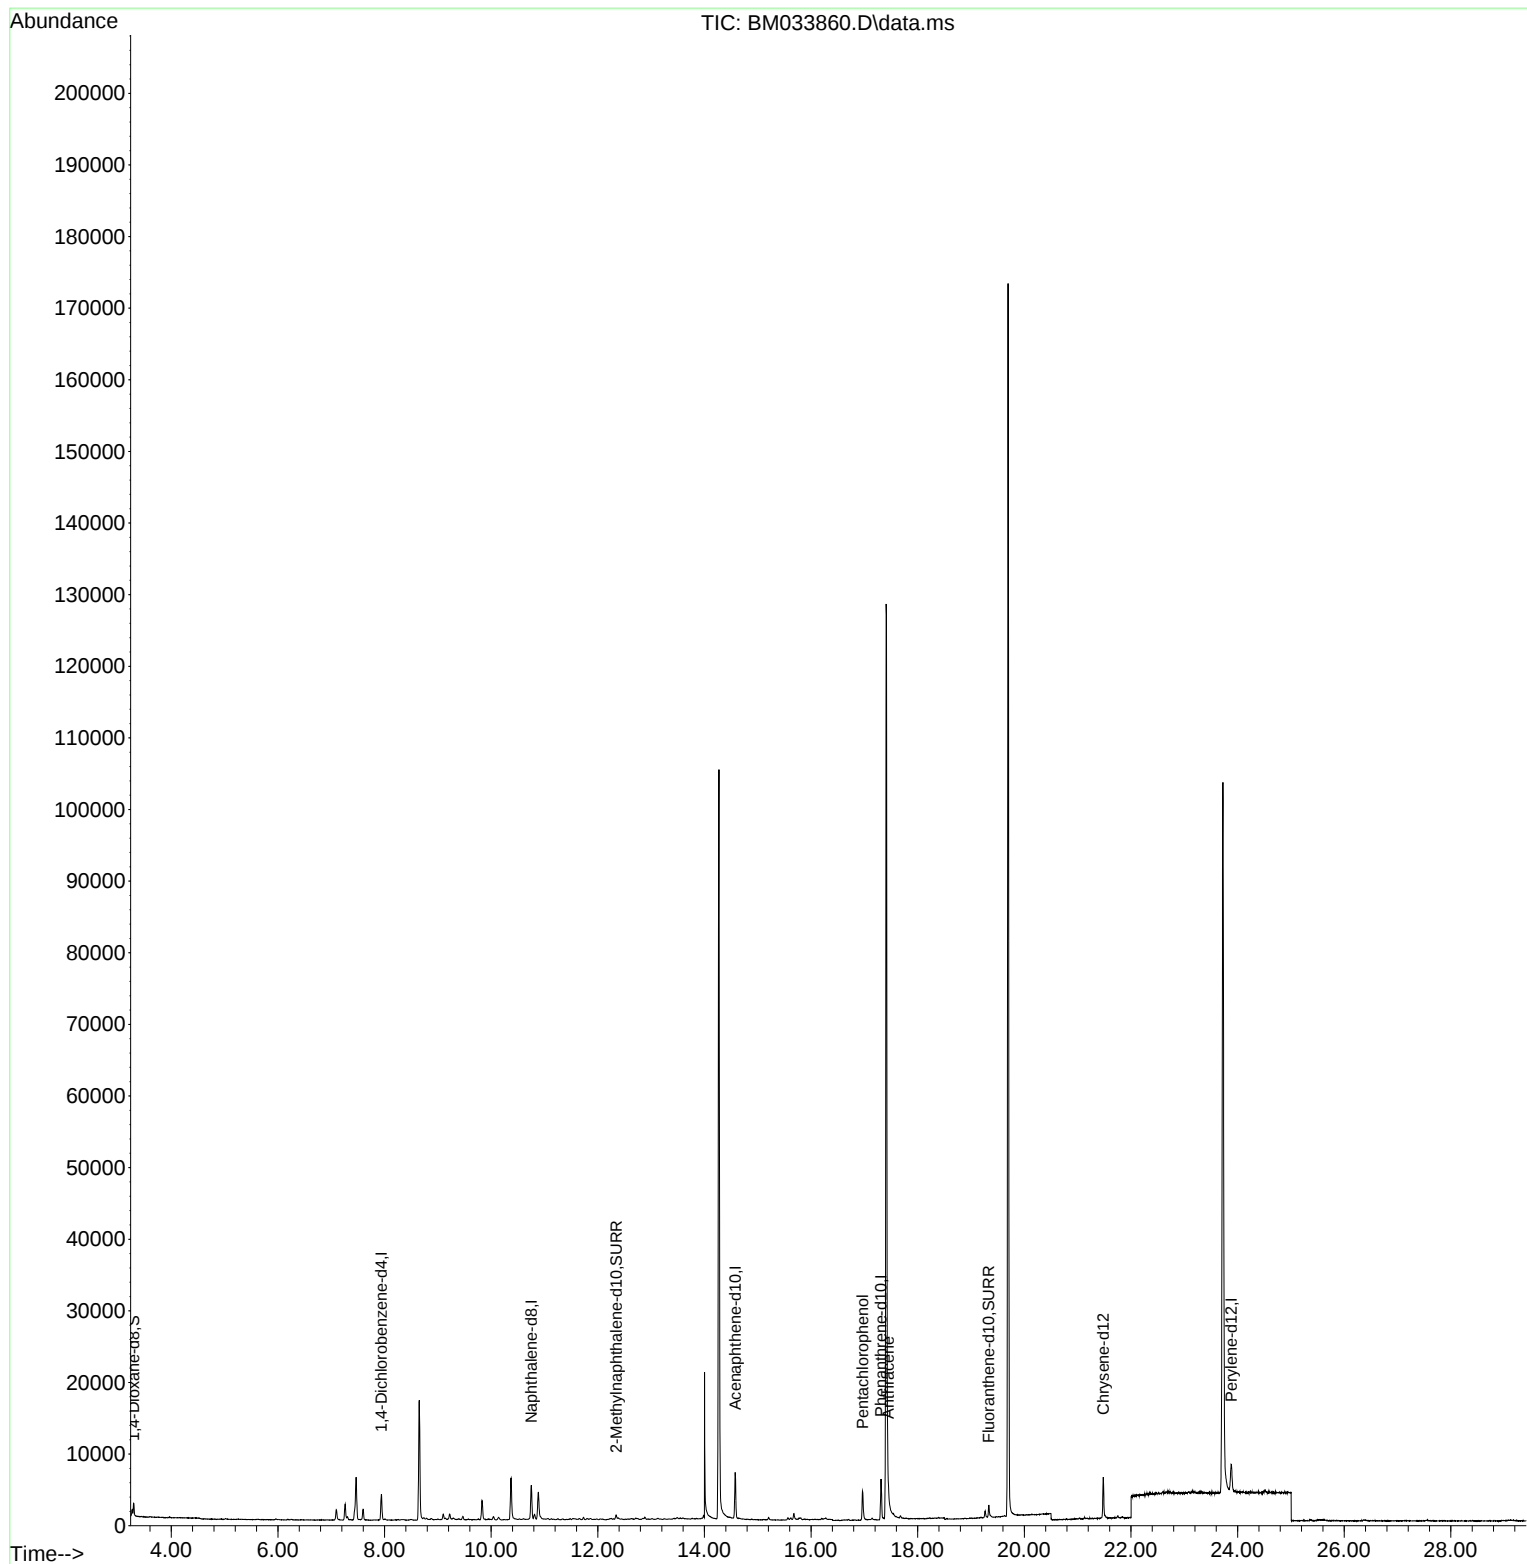



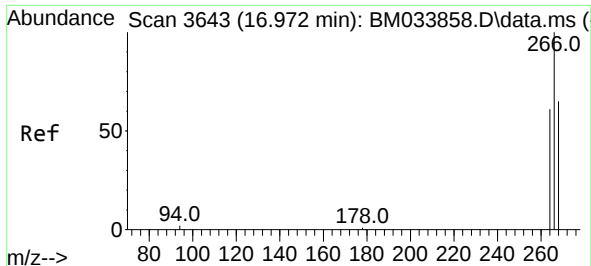


#14
Pentachlorophenol
Concen: 0.927 ng/ul
RT: 16.965 min Scan# 30
Delta R.T. -0.007 min
Lab File: BM033860.D
Acq: 25 Jan 2022 10:11

Instrument :
BNA_M
ClientSampleId :
C0Q09DL

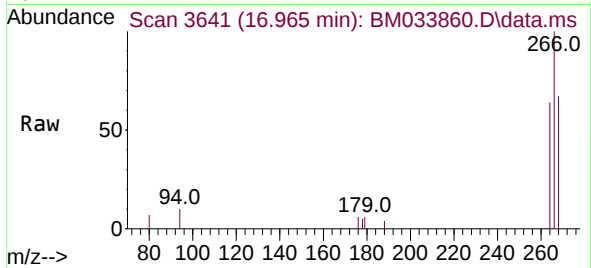

Tgt Ion:266 Resp: 2929
Ion Ratio Lower Upper
266 100
264 63.0 51.4 77.0
268 64.0 53.1 79.7

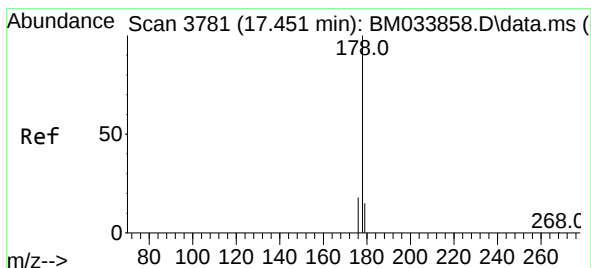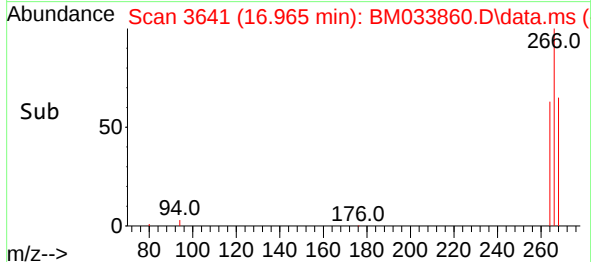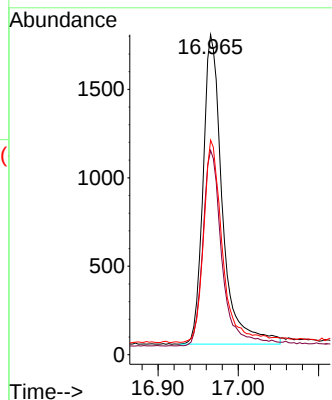

#16
Anthracene
Concen: 0.020 ng/ul
RT: 17.448 min Scan# 3780
Delta R.T. -0.004 min
Lab File: BM033860.D
Acq: 25 Jan 2022 10:11

Tgt Ion:178 Resp: 413
Ion Ratio Lower Upper
178 100
179 44.4 16.5 24.7#
176 37.5 18.3 27.5#

