


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012519\
 Data File : BM018649.D
 Acq On : 25 Jan 2019 11:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 22:01:30 2019

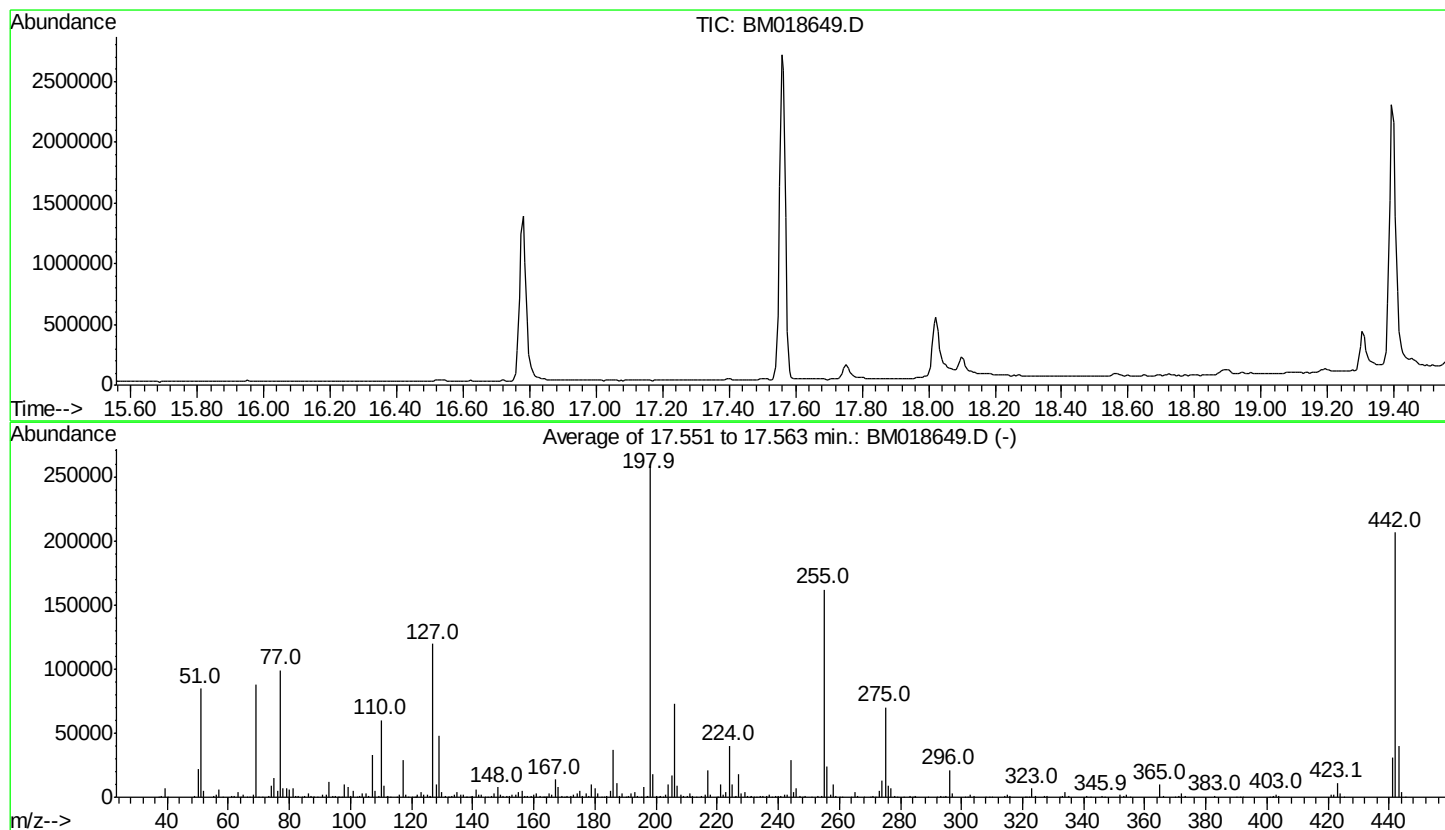

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	84740	PASS
68	69	0.00	2	1.9	1678	PASS
69	198	0.00	100	34.2	88314	PASS
70	69	0.00	2	0.1	129	PASS
127	198	10	80	46.2	119362	PASS
197	198	0.00	2	0.5	1370	PASS
198	198	100	100	100.0	258538	PASS
199	198	5	9	7.1	18452	PASS
275	198	10	60	27.0	69930	PASS
365	198	1	100	3.8	9781	PASS
441	198	0.01	100	11.9	30802	PASS
442	198	50	100	79.9	206525	PASS
443	442	15	24	19.3	39869	PASS