
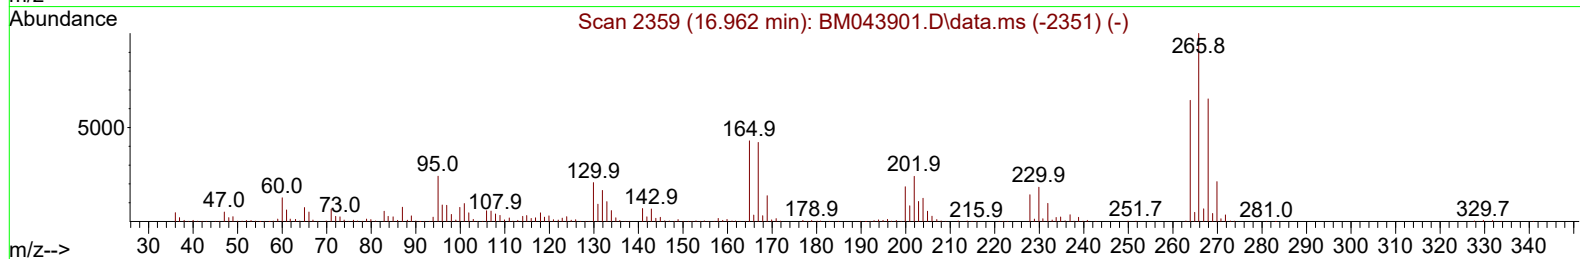
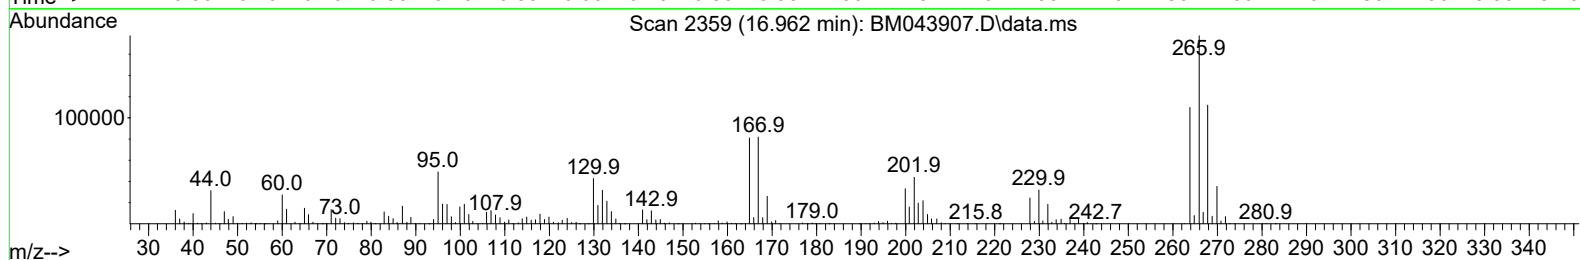


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012624\
Data File : BM043907.D
Acq On : 26 Jan 2024 10:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 14:32:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 00:26:01 2024
Response via : Initial Calibration

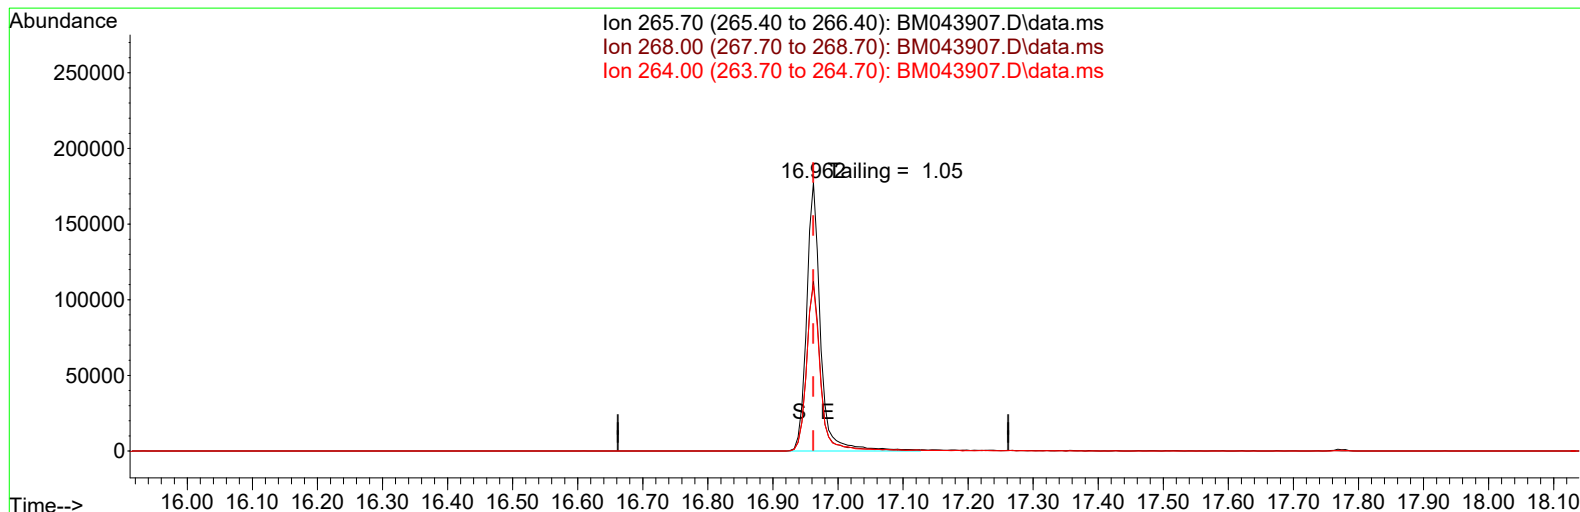

TIC: BM043907.D\data.ms

(70) Pentachlorophenol (C)




16.962min (+ 0.000) 534380.35 ng

response 263328

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	63.10
264.00	64.50	61.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012624\
Data File : BM043907.D
Acq On : 26 Jan 2024 10:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 14:32:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 00:26:01 2024
Response via : Initial Calibration

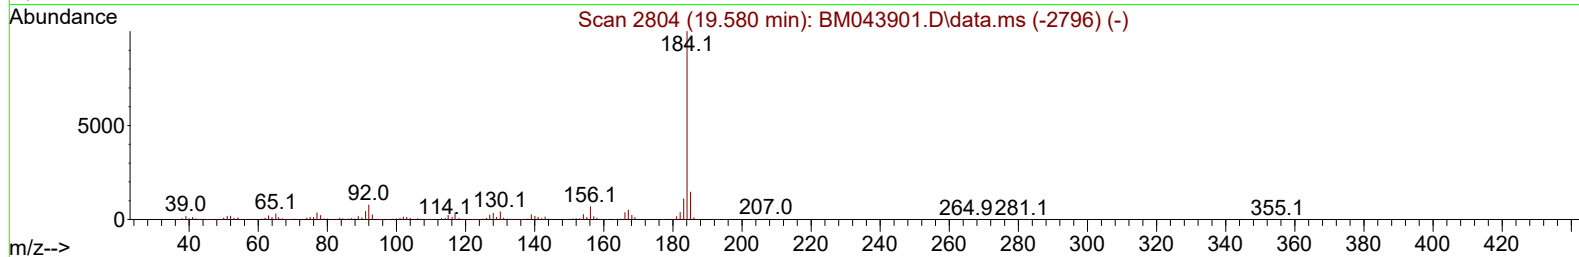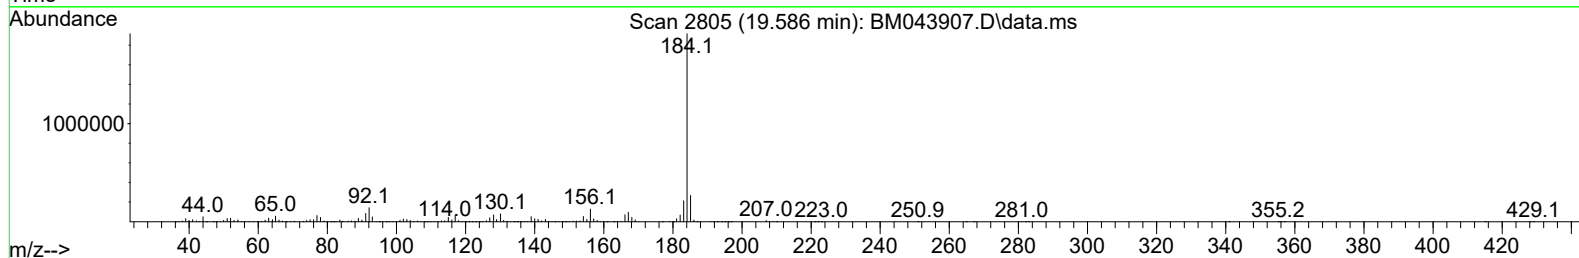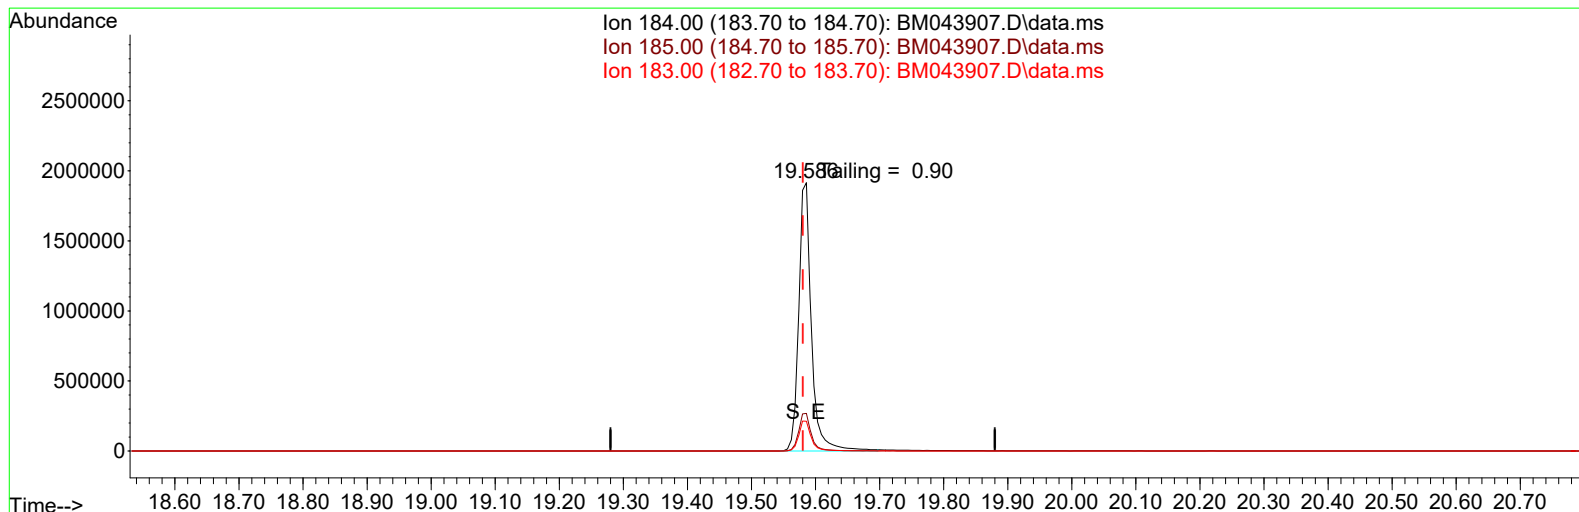

TIC: BM043907.D\data.ms

(77) Benzidine

19.586min (+ 0.006) 21335.52 ng

response 2670344

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.00
183.00	11.00	11.13
0.00	0.00	0.00