
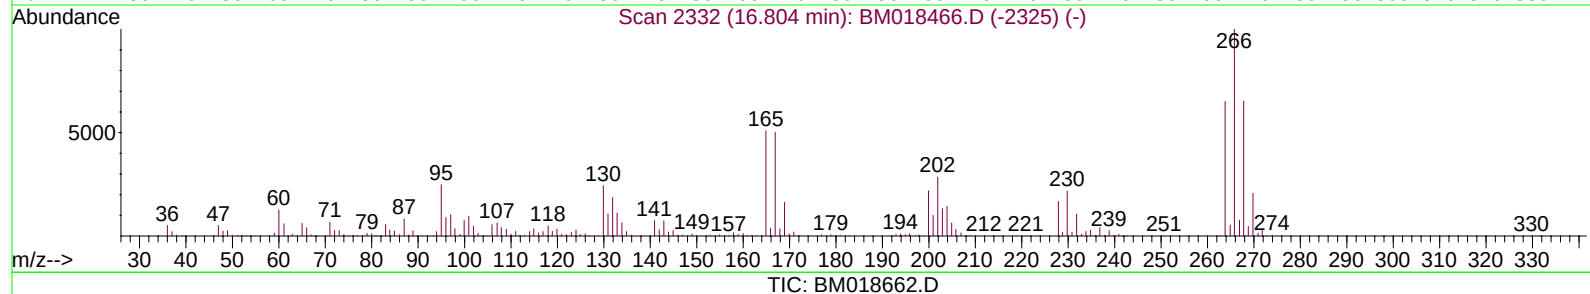
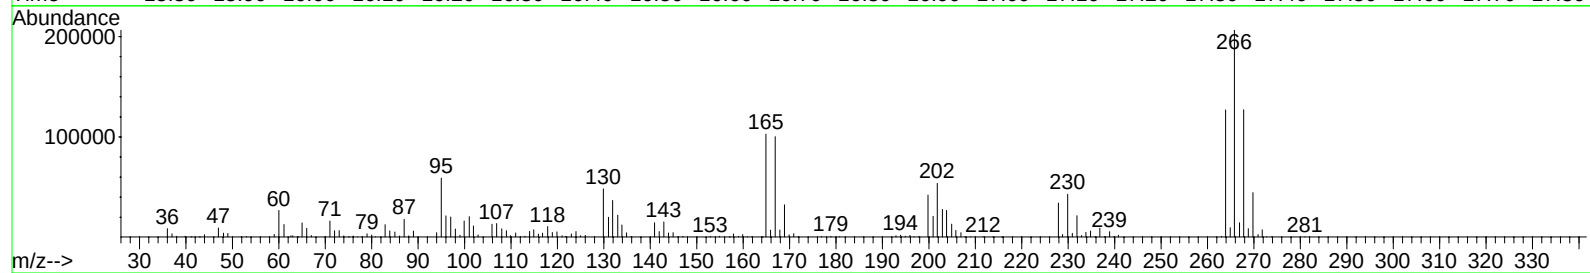


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012819\
Data File : BM018662.D
Acq On : 28 Jan 2019 13:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 17:19:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

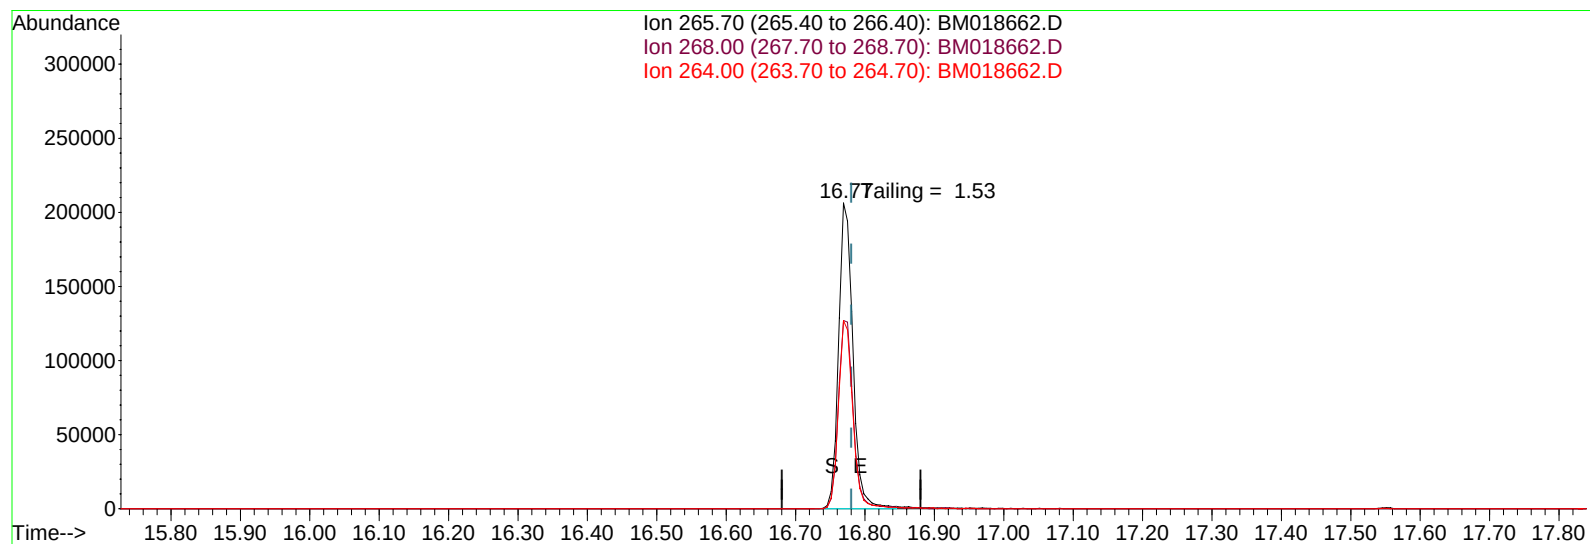

(70) Pentachlorophenol (C)




16.769min (-0.011) 23481.77ng

response 294192

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	61.57
264.00	62.60	61.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012819\
 Data File : BM018662.D
 Acq On : 28 Jan 2019 13:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 17:19:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 22:01:30 2019
 Response via : Initial Calibration

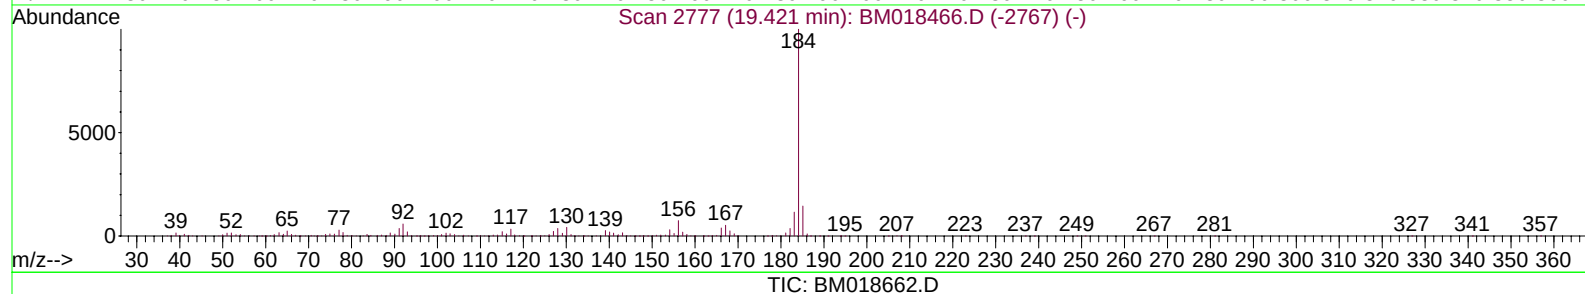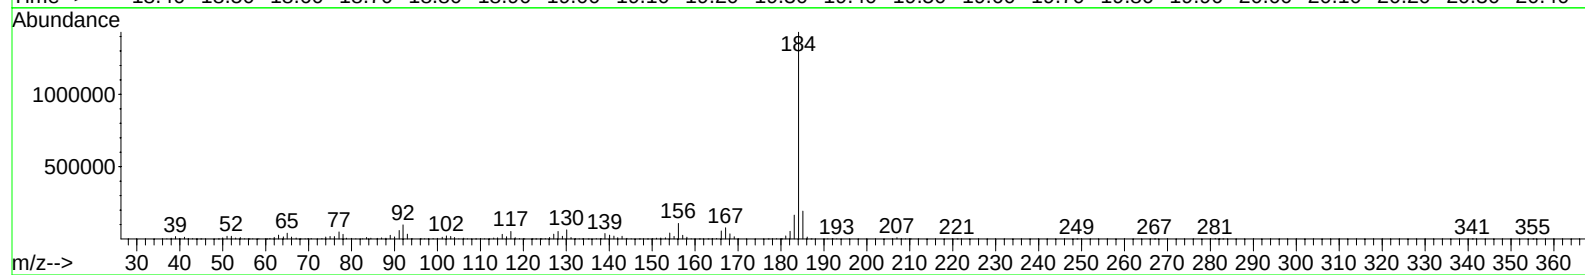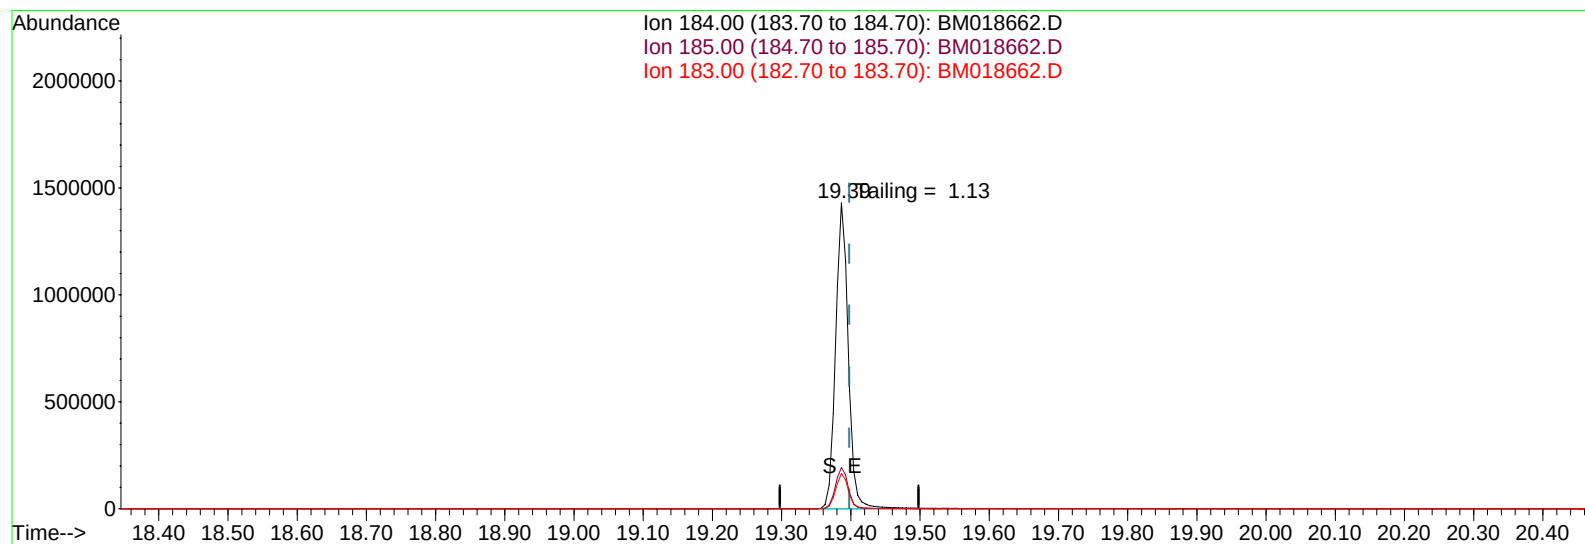

(77) Benzidine

19.386min (-0.011) 16628.83ng

response 1804954

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.45
183.00	11.90	11.59
0.00	0.00	0.00