


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012819\
 Data File : BM018662.D
 Acq On : 28 Jan 2019 13:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 22:01:30 2019

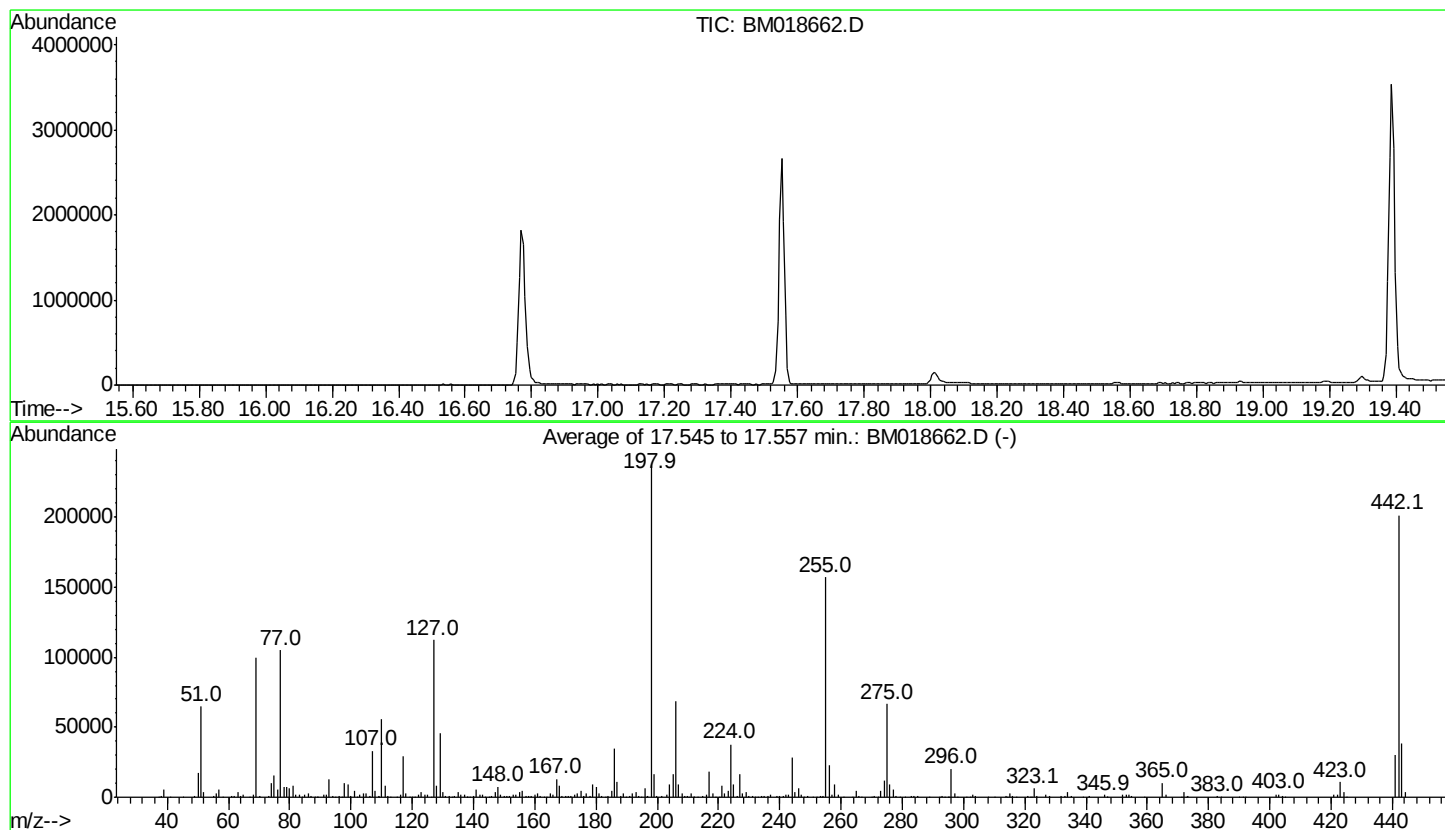

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	64893	PASS
68	69	0.00	2	2.0	2024	PASS
69	198	0.00	100	42.0	99432	PASS
70	69	0.00	2	0.6	642	PASS
127	198	10	80	47.4	112173	PASS
197	198	0.00	2	0.5	1267	PASS
198	198	100	100	100.0	236821	PASS
199	198	5	9	6.8	16087	PASS
275	198	10	60	28.0	66389	PASS
365	198	1	100	4.4	10452	PASS
441	198	0.01	100	12.8	30354	PASS
442	198	50	100	85.1	201562	PASS
443	442	15	24	19.3	38834	PASS