




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033913.D
Acq On : 28 Jan 2022 20:42
Operator : CG/JU
Sample : N1302-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F25

Manual IntegrationsAPPROVED

Quant Time: Jan 28 23:29:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 28 23:26:29 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :mohammad ahmed 02/01/2022

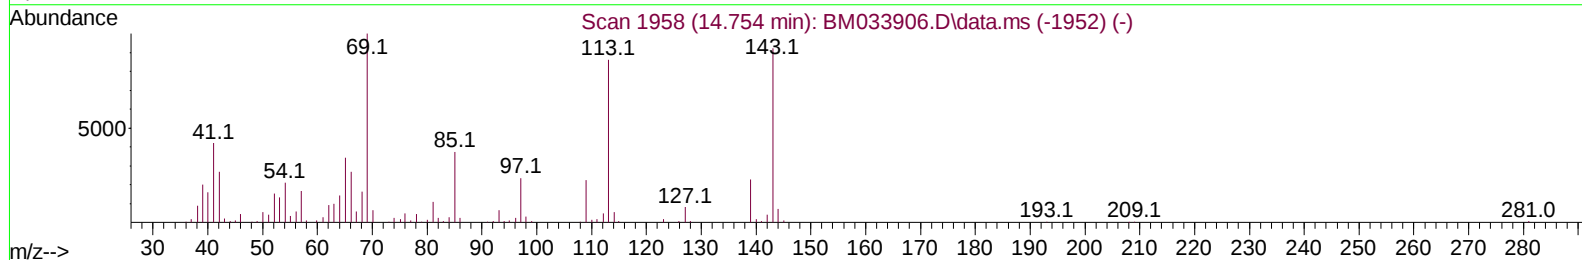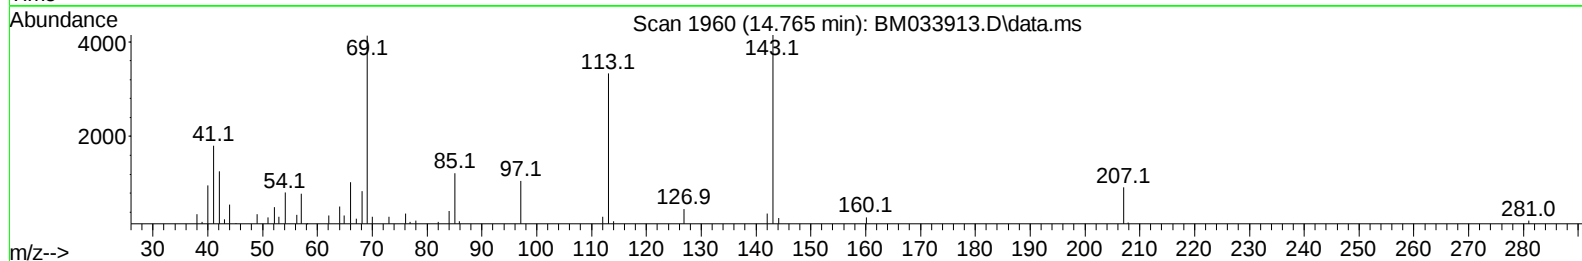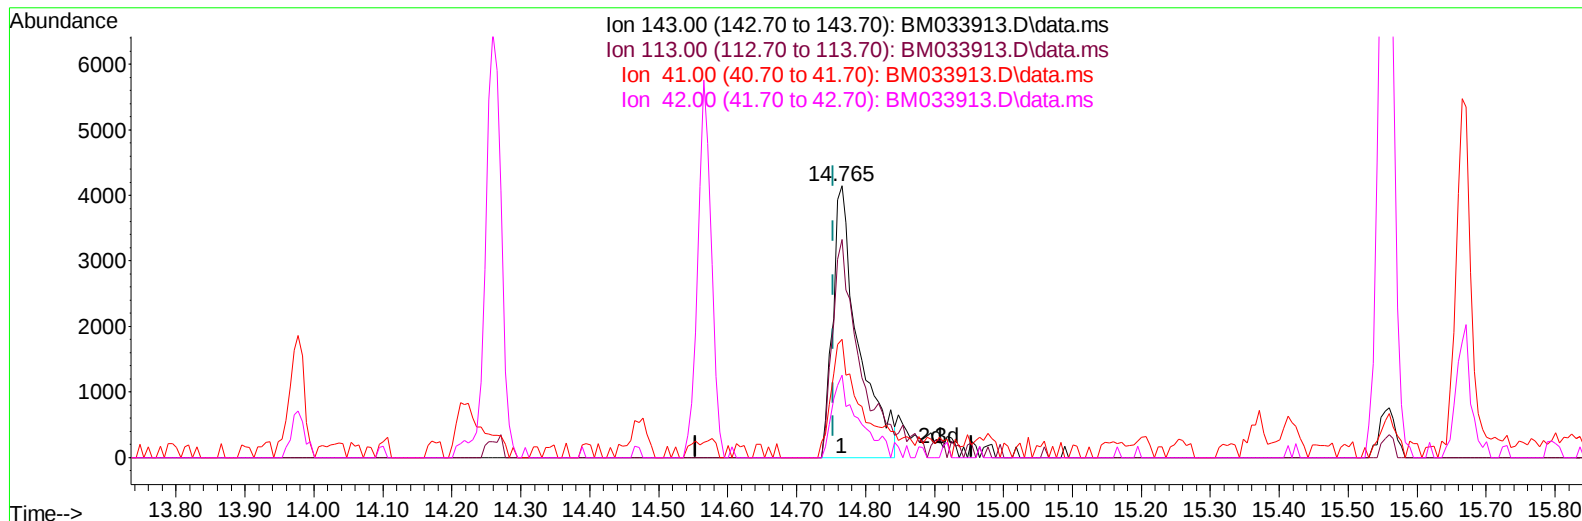

TIC: BM033913.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.765min (+ 0.012) 3.02 ng/ul m

response 10607

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	80.40#
41.00	57.20	43.54#
42.00	39.50	30.44#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033913.D
 Acq On : 28 Jan 2022 20:42
 Operator : CG/JU
 Sample : N1302-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F25

Manual IntegrationsAPPROVED

Quant Time: Jan 28 23:29:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 28 23:26:29 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :mohammad ahmed 02/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	88592	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	371032	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.565	164	232069	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188	478739	20.000	ng/ul	0.00
79) Chrysene-d12	21.465	240	473001	20.000	ng/ul	0.00
88) Perylene-d12	23.859	264	484556	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	9101	3.860	ng/uL	0.00
4) Pyridine-d5	3.719	84	48964	7.478	ng/ul	0.00
7) Phenol-d5	7.084	99	42857	5.386	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	157672	32.539	ng/ul	0.00
11) 2-Chlorophenol-d4	7.460	132	152644	25.091	ng/ul	0.00
15) 4-Methylphenol-d8	8.636	113	85427	12.970	ng/ul	0.00
21) Nitrobenzene-d5	9.089	128	98335	33.560	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	100241	32.279	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	163037	27.386	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	239579	27.072	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	649310	35.512	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	747028	34.632	ng/ul	0.00
54) 4-Nitrophenol-d4	14.765	143	10607m	3.023	ng/ul	0.01
60) Fluorene-d10	15.554	176	557004	36.720	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	83540	29.336	ng/ul	0.00
73) Anthracene-d10	17.401	188	949180	40.860	ng/ul	0.00
81) Pyrene-d10	19.689	212	1103021	43.182	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.706	264	1064828	42.235	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033913.D
Acq On : 28 Jan 2022 20:42
Operator : CG/JU
Sample : N1302-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F25

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :mohammad ahmed 02/01/2022

Quant Time: Jan 28 23:29:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 28 23:26:29 2022
Response via : Initial Calibration

