




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033915.D
Acq On : 28 Jan 2022 21:53
Operator : CG/JU
Sample : N1302-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F48

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :mohammad ahmed 02/01/2022

Quant Time: Jan 28 23:29:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 28 23:26:29 2022
Response via : Initial Calibration

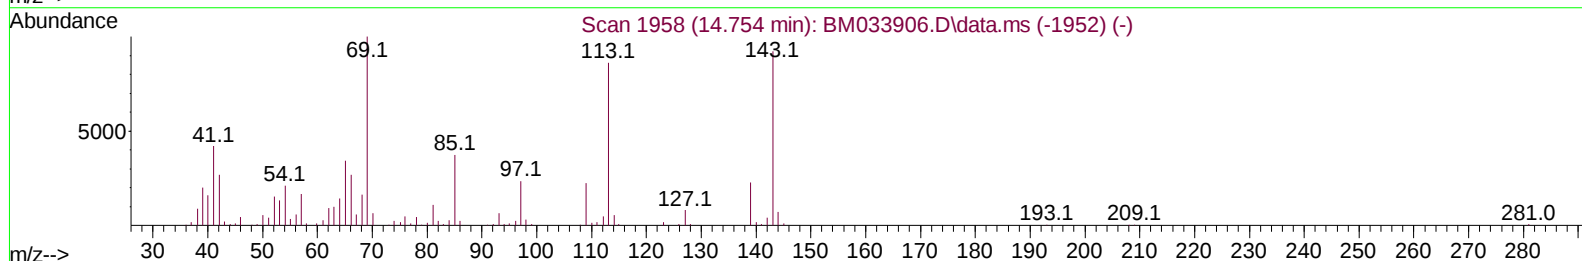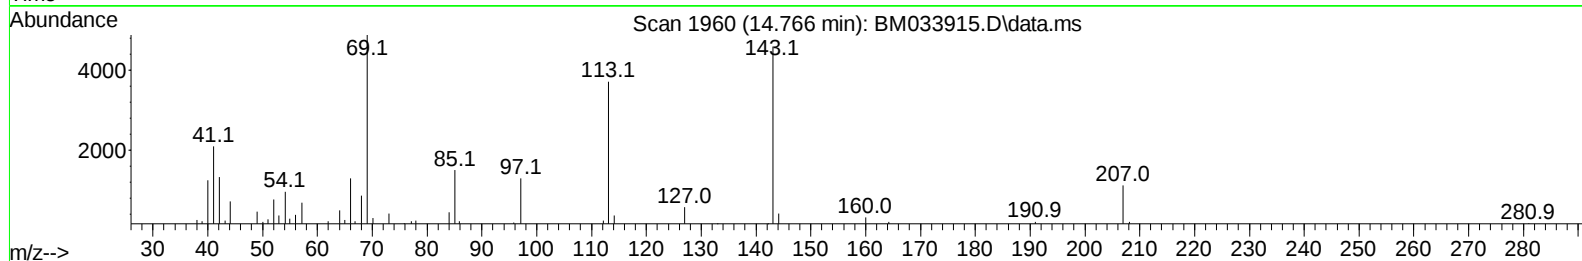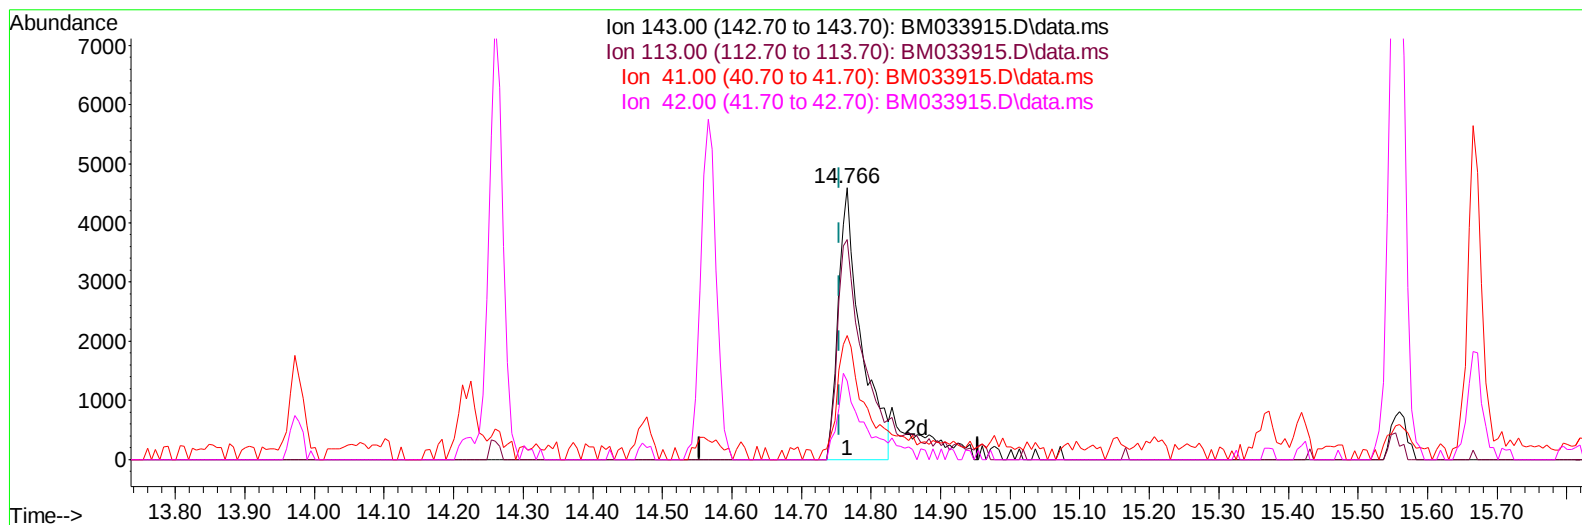

TIC: BM033915.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.766min (+ 0.012) 2.64 ng/u1

response 10447

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	80.88#
41.00	57.20	45.52#
42.00	39.50	28.88#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033915.D
 Acq On : 28 Jan 2022 21:53
 Operator : CG/JU
 Sample : N1302-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F48

Manual IntegrationsAPPROVED

Quant Time: Jan 28 23:29:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 28 23:26:29 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :mohammad ahmed 02/01/2022

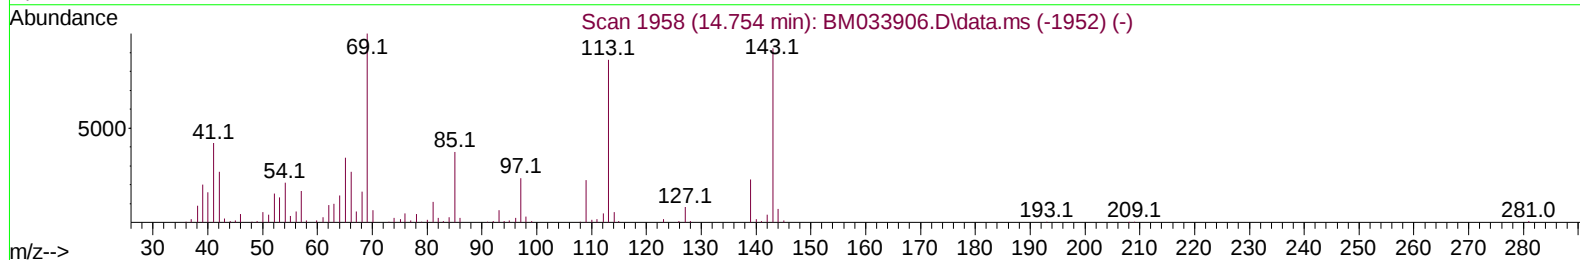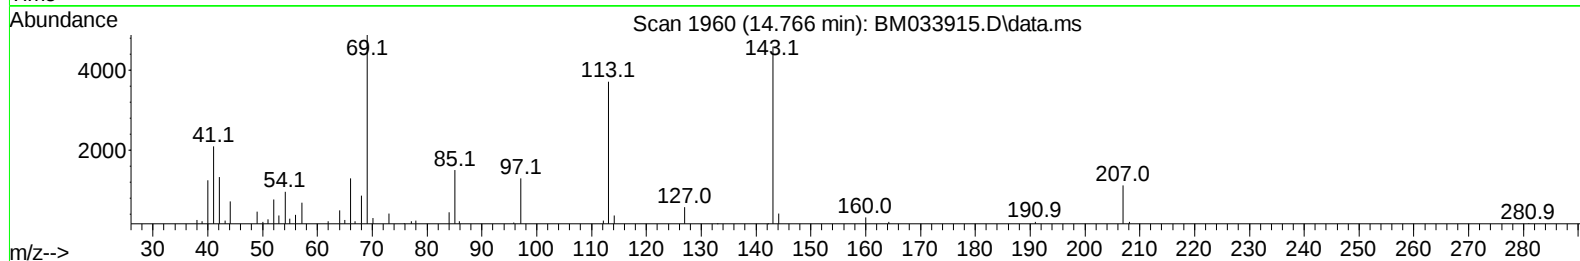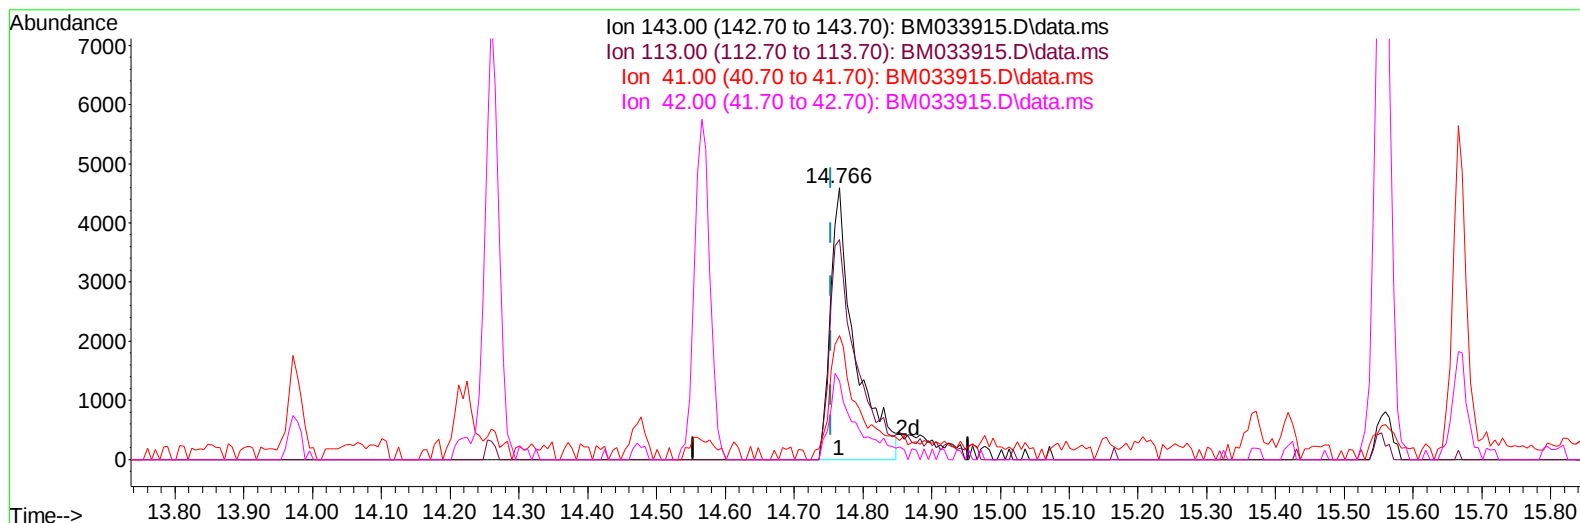

TIC: BM033915.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.766min (+ 0.012) 2.85 ng/ul m

response 11277

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	80.88#
41.00	57.20	45.52#
42.00	39.50	28.88#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033915.D
 Acq On : 28 Jan 2022 21:53
 Operator : CG/JU
 Sample : N1302-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F48

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/31/2022
 Supervised By :mohammad ahmed 02/01/2022

Quant Time: Jan 28 23:29:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 28 23:26:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	102214	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	420734	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164	261681	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.307	188	540454	20.000	ng/ul	0.00
79) Chrysene-d12	21.465	240	531547	20.000	ng/ul	0.00
88) Perylene-d12	23.859	264	542249	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	10363	3.809	ng/uL	0.00
4) Pyridine-d5	3.719	84	73307	9.703	ng/ul	0.00
7) Phenol-d5	7.084	99	48352	5.267	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	164247	29.379	ng/ul	0.00
11) 2-Chlorophenol-d4	7.460	132	160200	22.824	ng/ul	0.00
15) 4-Methylphenol-d8	8.637	113	94310	12.410	ng/ul	0.00
21) Nitrobenzene-d5	9.090	128	103146	31.043	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	105799	30.044	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	169707	25.138	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	251749	25.087	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	664514	32.231	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	767123	31.539	ng/ul	0.00
54) 4-Nitrophenol-d4	14.766	143	11277m	2.850	ng/ul	0.01
60) Fluorene-d10	15.560	176	563329	32.934	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.671	200	81288	25.285	ng/ul	0.00
73) Anthracene-d10	17.401	188	926645	35.335	ng/ul	0.00
81) Pyrene-d10	19.689	212	1076835	37.513	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.706	264	1035777	36.712	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033915.D
Acq On : 28 Jan 2022 21:53
Operator : CG/JU
Sample : N1302-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F48

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/31/2022
Supervised By :mohammad ahmed 02/01/2022

Quant Time: Jan 28 23:29:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 28 23:26:29 2022
Response via : Initial Calibration

