

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033907.D
 Acq On : 28 Jan 2022 17:08
 Operator : CG/JU
 Sample : PB142334BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK334

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	18	rVB	33495	44895	1.90%	0.177%
2	3.719	78	82	93	rBV	349259	536411	22.74%	2.111%
3	4.060	136	140	144	rVB3	7752	12204	0.52%	0.048%
4	4.096	144	146	150	rBV5	1979	3045	0.13%	0.012%
5	5.495	383	384	389	rVB5	2161	2478	0.11%	0.010%
6	7.089	648	655	668	rVB	409931	657322	27.86%	2.586%
7	7.254	677	683	692	rVB	334360	516535	21.89%	2.032%
8	7.460	711	718	728	rBV	442632	695466	29.48%	2.737%
9	7.607	740	743	747	rBV5	1762	2409	0.10%	0.009%
10	7.931	791	798	808	rBV	396671	628495	26.64%	2.473%
11	8.636	912	918	931	rBV	492488	806909	34.20%	3.175%
12	9.095	989	996	1006	rBV	400640	662325	28.07%	2.606%
13	9.819	1112	1119	1128	rBV	325487	534478	22.65%	2.103%
14	10.360	1204	1211	1230	rBV	461373	807494	34.23%	3.177%
15	10.742	1269	1276	1286	rBV	520236	886141	37.56%	3.487%
16	10.877	1289	1299	1315	rBV	444302	827103	35.06%	3.254%
17	12.336	1542	1547	1553	rBV3	6863	13312	0.56%	0.052%
18	13.548	1746	1753	1755	rBV5	1670	2949	0.12%	0.012%
19	13.977	1819	1826	1844	rBV	902997	1247324	52.87%	4.908%
20	14.265	1868	1875	1889	rVV	945173	1392760	59.03%	5.480%
21	14.571	1920	1927	1938	rBV	778085	1157389	49.06%	4.554%
22	14.754	1953	1958	1978	rBV	232045	509441	21.59%	2.005%
23	15.560	2088	2095	2108	rBV	1226376	1762725	74.72%	6.936%
24	15.671	2108	2114	2129	rVV	343746	507794	21.52%	1.998%
25	15.795	2131	2135	2139	rVB3	8861	12803	0.54%	0.050%
26	17.095	2350	2356	2359	rBV3	3809	7372	0.31%	0.029%
27	17.306	2385	2392	2402	rBV	995015	1396714	59.20%	5.496%
28	17.401	2402	2408	2424	rVV	1410030	2025909	85.87%	7.972%
29	17.683	2451	2456	2459	rBV6	2068	4031	0.17%	0.016%
30	18.895	2660	2662	2665	rBV4	2066	2381	0.10%	0.009%
31	19.259	2719	2724	2730	rBV3	14718	22129	0.94%	0.087%
32	19.330	2732	2736	2742	rVB	13089	19668	0.83%	0.077%
33	19.689	2791	2797	2807	rBV	1760723	2359252	100.00%	9.283%
34	21.471	3095	3100	3108	rBV	1182744	1531044	64.90%	6.024%
35	23.712	3474	3481	3488	rBV	1174379	2280372	96.66%	8.973%
36	23.865	3501	3507	3519	rVB2	739885	1535313	65.08%	6.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033907.D
Acq On : 28 Jan 2022 17:08
Operator : CG/JU
Sample : PB142334BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK334

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Title : SVOA CALIBRATION




Sum of corrected areas: 25414392

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033907.D
Acq On : 28 Jan 2022 17:08
Operator : CG/JU
Sample : PB142334BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK334

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

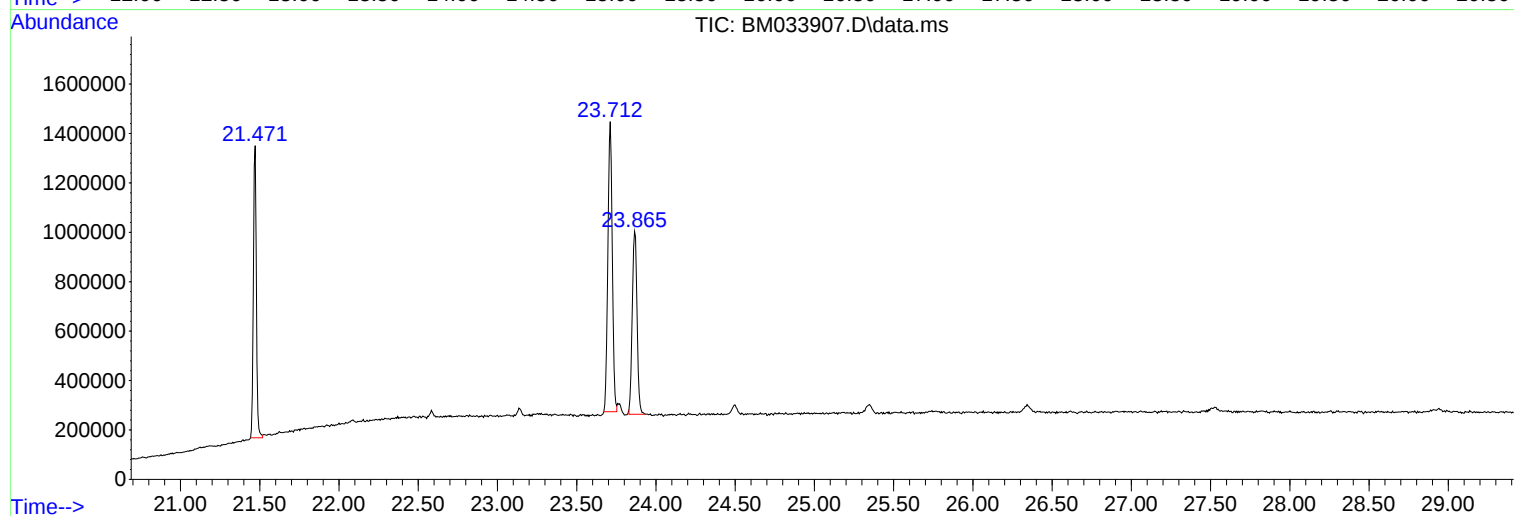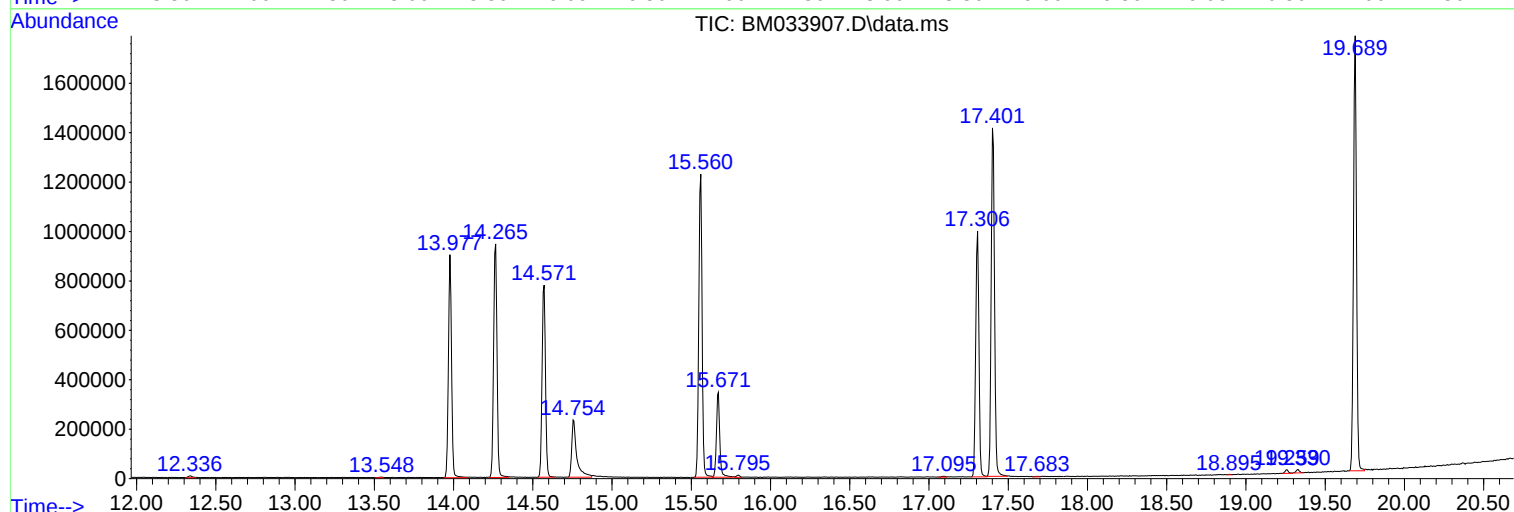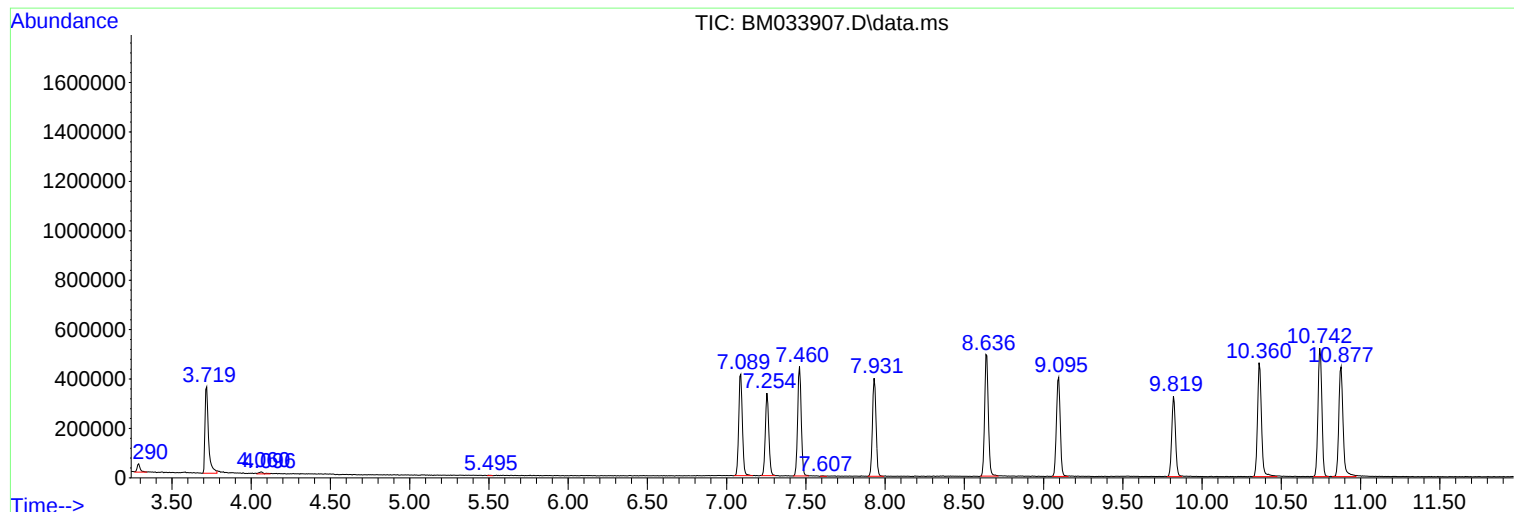

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033907.D
Acq On : 28 Jan 2022 17:08
Operator : CG/JU
Sample : PB142334BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK334

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033907.D
Acq On : 28 Jan 2022 17:08
Operator : CG/JU
Sample : PB142334BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK334

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc