

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033909.D
 Acq On : 28 Jan 2022 18:20
 Operator : CG/JU
 Sample : N1302-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	15	rBV	27598	33945	1.14%	0.117%
2	3.719	79	82	96	rBV	108444	167885	5.65%	0.577%
3	3.966	123	124	128	rVB3	5580	4135	0.14%	0.014%
4	4.060	136	140	146	rBV2	8236	11573	0.39%	0.040%
5	5.007	299	301	307	rVB3	5918	9030	0.30%	0.031%
6	6.931	624	628	631	rBV3	6789	9345	0.31%	0.032%
7	7.089	647	655	670	rVB2	109649	202600	6.82%	0.697%
8	7.254	676	683	695	rBV	439505	692618	23.30%	2.382%
9	7.460	711	718	727	rBV	452229	702770	23.64%	2.417%
10	7.566	731	736	740	rBV6	2939	4791	0.16%	0.016%
11	7.931	789	798	806	rVB	457780	720014	24.22%	2.476%
12	8.001	806	810	815	rBV5	4694	7947	0.27%	0.027%
13	8.166	837	838	845	rVB5	2723	3813	0.13%	0.013%
14	8.495	890	894	897	rBV4	2025	3339	0.11%	0.011%
15	8.636	912	918	930	rBV	310368	501515	16.87%	1.725%
16	9.095	989	996	1004	rBV	533358	887298	29.85%	3.051%
17	9.542	1067	1072	1079	rVB	21896	33351	1.12%	0.115%
18	9.819	1112	1119	1131	rBV	432489	709116	23.85%	2.439%
19	10.360	1204	1211	1224	rBV	583643	972387	32.71%	3.344%
20	10.536	1235	1241	1250	rBV6	6038	14942	0.50%	0.051%
21	10.742	1269	1276	1286	rVB	604998	991796	33.36%	3.411%
22	10.877	1291	1299	1315	rBV	555706	999541	33.62%	3.438%
23	11.783	1448	1453	1456	rVB6	2168	3427	0.12%	0.012%
24	12.177	1512	1520	1525	rBV2	8169	13872	0.47%	0.048%
25	12.336	1542	1547	1549	rBV	9834	15275	0.51%	0.053%
26	12.371	1549	1553	1557	rVB3	3712	7606	0.26%	0.026%
27	12.807	1620	1627	1631	rVB5	2783	4510	0.15%	0.016%
28	12.842	1631	1633	1636	rBV3	2963	3007	0.10%	0.010%
29	12.907	1641	1644	1647	rBV4	2526	3973	0.13%	0.014%
30	12.977	1654	1656	1662	rVB2	3740	5349	0.18%	0.018%
31	13.124	1678	1681	1686	rVB6	3207	4427	0.15%	0.015%
32	13.189	1688	1692	1696	rBV5	5372	7469	0.25%	0.026%
33	13.407	1724	1729	1738	rVB2	20519	31261	1.05%	0.108%
34	13.548	1749	1753	1757	rVB6	3000	4440	0.15%	0.015%
35	13.977	1818	1826	1832	rBV	1222908	1618945	54.46%	5.568%
36	14.224	1863	1868	1869	rBV3	14755	22377	0.75%	0.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033909.D
 Acq On : 28 Jan 2022 18:20
 Operator : CG/JU
 Sample : N1302-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	14.260	1869	1874	1886	rVB	1220877	1823701	61.35%	6.272%
38	14.471	1905	1910	1916	rVB2	8090	12301	0.41%	0.042%
39	14.565	1920	1926	1938	rBV	833931	1260967	42.42%	4.337%
40	14.760	1955	1959	1974	rBV2	31850	85174	2.87%	0.293%
41	14.912	1983	1985	1991	rVB6	2218	3048	0.10%	0.010%
42	14.971	1993	1995	2002	rVB4	2083	3599	0.12%	0.012%
43	15.101	2013	2017	2019	rBV5	2418	3770	0.13%	0.013%
44	15.160	2022	2027	2029	rBV4	3063	3727	0.13%	0.013%
45	15.201	2029	2034	2037	rBV4	6933	9988	0.34%	0.034%
46	15.371	2057	2063	2068	rBV3	13386	24942	0.84%	0.086%
47	15.424	2068	2072	2075	rVB5	8043	10532	0.35%	0.036%
48	15.554	2088	2094	2106	rBV	1607670	2350677	79.08%	8.084%
49	15.665	2107	2113	2128	rVV	475669	678161	22.81%	2.332%
50	15.801	2132	2136	2140	rVB3	10200	15038	0.51%	0.052%
51	15.924	2151	2157	2160	rVB7	4028	7010	0.24%	0.024%
52	15.971	2160	2165	2173	rBV8	5524	10319	0.35%	0.035%
53	16.101	2184	2187	2189	rBV3	3598	4156	0.14%	0.014%
54	16.189	2200	2202	2206	rBV5	3444	4300	0.14%	0.015%
55	16.236	2207	2210	2215	rVV5	6894	9227	0.31%	0.032%
56	16.277	2215	2217	2220	rVV2	7233	6682	0.22%	0.023%
57	16.342	2225	2228	2232	rVB6	4764	7044	0.24%	0.024%
58	16.448	2241	2246	2250	rBV4	7453	11542	0.39%	0.040%
59	16.548	2261	2263	2268	rVB6	3229	4940	0.17%	0.017%
60	16.795	2300	2305	2307	rBV5	4501	7179	0.24%	0.025%
61	16.848	2312	2314	2317	rBV4	3718	4098	0.14%	0.014%
62	17.071	2348	2352	2354	rVV	10732	14429	0.49%	0.050%
63	17.118	2358	2360	2367	rVB6	8267	11109	0.37%	0.038%
64	17.230	2374	2379	2383	rVB5	16832	20152	0.68%	0.069%
65	17.306	2385	2392	2401	rBV	963199	1430432	48.12%	4.919%
66	17.401	2401	2408	2421	rBV	1824504	2662318	89.56%	9.156%
67	17.612	2440	2444	2449	rVB7	4004	7837	0.26%	0.027%
68	17.689	2453	2457	2461	rBV7	5083	8458	0.28%	0.029%
69	17.806	2474	2477	2480	rBV5	3233	3801	0.13%	0.013%
70	17.918	2493	2496	2500	rBV6	3038	3651	0.12%	0.013%
71	17.983	2503	2507	2510	rVB4	9274	12474	0.42%	0.043%
72	18.101	2523	2527	2529	rBV5	3061	5025	0.17%	0.017%
73	18.195	2539	2543	2548	rBV2	36670	50882	1.71%	0.175%
74	18.500	2592	2595	2600	rBV6	5649	10770	0.36%	0.037%
75	18.630	2612	2617	2621	rBV5	14011	17961	0.60%	0.062%
76	18.748	2635	2637	2642	rVB5	4184	4350	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033909.D
 Acq On : 28 Jan 2022 18:20
 Operator : CG/JU
 Sample : N1302-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

77	18.865	2655	2657	2659	rVB3	4445	3457	0.12%	0.012%
78	18.971	2671	2675	2680	rBV7	5200	8805	0.30%	0.030%
79	19.059	2687	2690	2698	rVB7	10987	17559	0.59%	0.060%
80	19.124	2698	2701	2702	rBV3	7061	6935	0.23%	0.024%
81	19.253	2719	2723	2727	rBV2	24691	35701	1.20%	0.123%
82	19.295	2727	2730	2732	rVV4	6821	6979	0.23%	0.024%
83	19.324	2732	2735	2738	rVV	20269	23059	0.78%	0.079%
84	19.471	2756	2760	2765	rBV8	10537	18561	0.62%	0.064%
85	19.689	2791	2797	2808	rBV	2312596	2972705	100.00%	10.223%
86	21.183	3047	3051	3058	rBV4	62685	94758	3.19%	0.326%
87	21.471	3095	3100	3109	rBV	1097209	1460236	49.12%	5.022%
88	23.712	3473	3481	3488	rBV2	1427692	2873381	96.66%	9.882%
89	23.865	3500	3507	3518	rVB2	753296	1499871	50.45%	5.158%




Sum of corrected areas: 29077467

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033909.D
Acq On : 28 Jan 2022 18:20
Operator : CG/JU
Sample : N1302-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

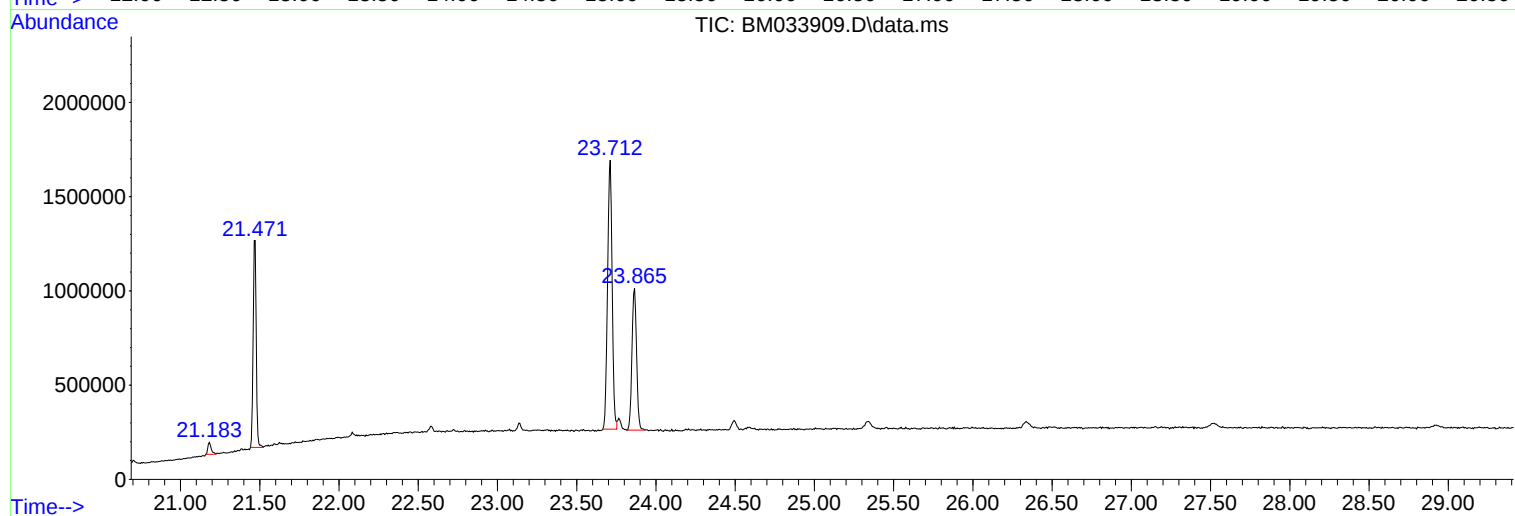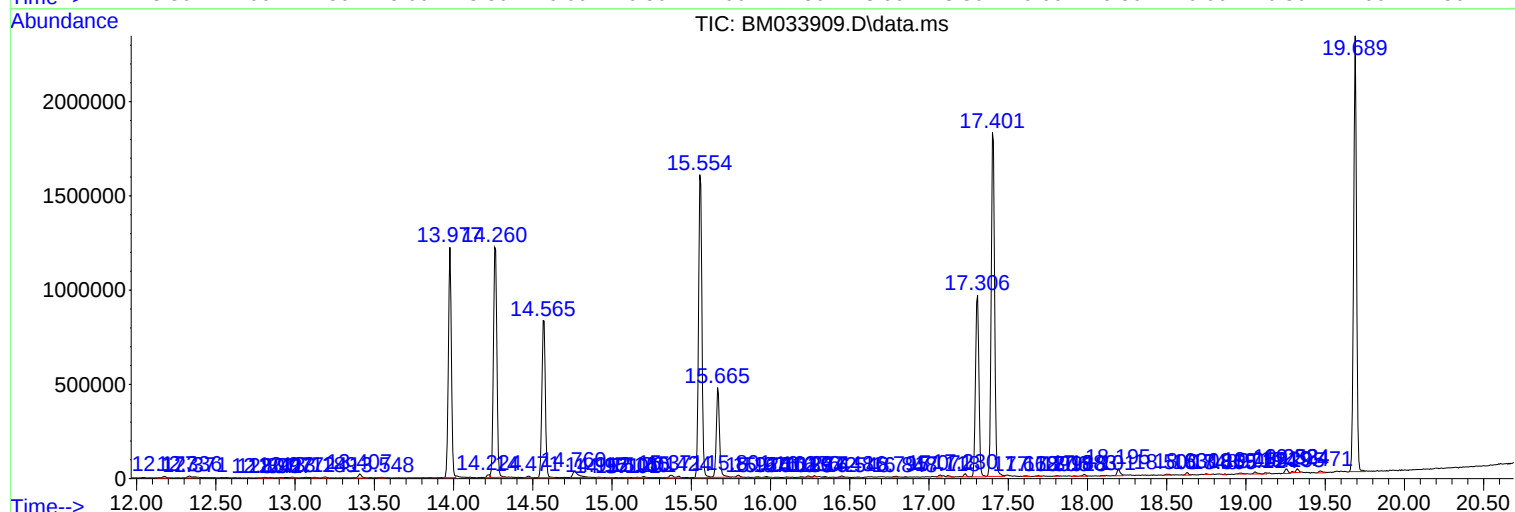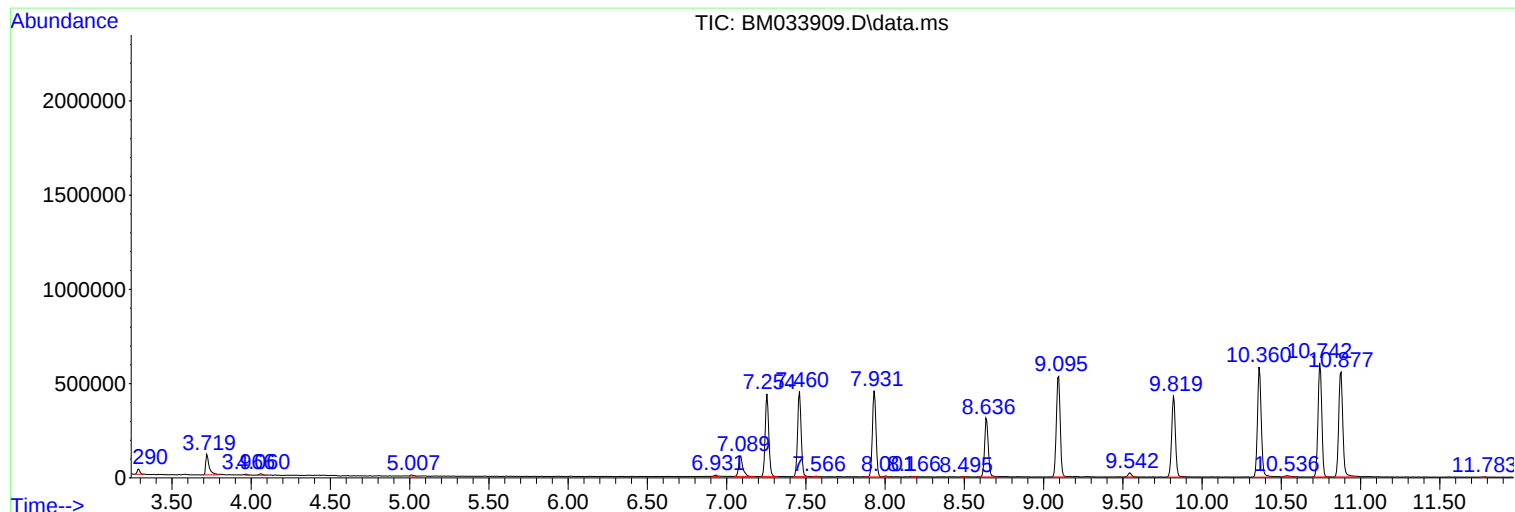

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033909.D
Acq On : 28 Jan 2022 18:20
Operator : CG/JU
Sample : N1302-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033909.D
Acq On : 28 Jan 2022 18:20
Operator : CG/JU
Sample : N1302-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F47

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------