

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033910.D
 Acq On : 28 Jan 2022 18:55
 Operator : CG/JU
 Sample : N1302-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	14	rVB	24195	30511	1.13%	0.116%
2	3.719	79	82	93	rBV	105206	164869	6.12%	0.628%
3	3.966	118	124	128	rVB8	5569	10859	0.40%	0.041%
4	4.061	137	140	144	rVB3	6969	10185	0.38%	0.039%
5	5.013	296	302	306	rBV4	4707	7618	0.28%	0.029%
6	5.608	400	403	405	rBV2	2620	2831	0.11%	0.011%
7	6.931	625	628	632	rVB4	3854	4735	0.18%	0.018%
8	7.084	649	654	665	rVB	118811	198609	7.37%	0.757%
9	7.255	675	683	697	rBV	389430	611440	22.68%	2.331%
10	7.460	709	718	729	rBV	396218	631628	23.43%	2.408%
11	7.931	791	798	806	rBV	396947	624527	23.17%	2.381%
12	8.002	806	810	814	rVB4	3577	4787	0.18%	0.018%
13	8.178	836	840	848	rVB9	2607	5364	0.20%	0.020%
14	8.637	911	918	928	rBV	292376	459737	17.06%	1.752%
15	9.090	988	995	1004	rBV	475228	777380	28.84%	2.963%
16	9.543	1065	1072	1080	rVB	161418	243828	9.05%	0.929%
17	9.819	1111	1119	1131	rBV	373139	621057	23.04%	2.367%
18	10.054	1155	1159	1163	rBV6	1438	2769	0.10%	0.011%
19	10.360	1204	1211	1224	rBV	506689	864937	32.09%	3.297%
20	10.537	1238	1241	1243	rBV3	2706	3926	0.15%	0.015%
21	10.690	1262	1267	1270	rBV2	7622	12639	0.47%	0.048%
22	10.743	1270	1276	1284	rVB	514835	861840	31.97%	3.285%
23	10.872	1291	1298	1312	rBV	455210	805898	29.90%	3.072%
24	12.042	1490	1497	1504	rVB	48778	72746	2.70%	0.277%
25	12.178	1514	1520	1525	rVB3	6792	11217	0.42%	0.043%
26	12.331	1541	1546	1551	rVB3	9212	13765	0.51%	0.052%
27	12.913	1639	1645	1647	rBV5	2540	3728	0.14%	0.014%
28	12.984	1653	1657	1661	rVB5	4439	6399	0.24%	0.024%
29	13.125	1677	1681	1686	rVB5	2602	3794	0.14%	0.014%
30	13.189	1686	1692	1696	rBV8	4009	6224	0.23%	0.024%
31	13.407	1725	1729	1736	rBV2	17210	24155	0.90%	0.092%
32	13.978	1819	1826	1832	rBV	1086245	1464590	54.33%	5.583%
33	14.113	1844	1849	1850	rVB4	1860	2886	0.11%	0.011%
34	14.219	1862	1867	1868	rBV4	11401	14079	0.52%	0.054%
35	14.260	1868	1874	1885	rVB	1134130	1646836	61.10%	6.277%
36	14.472	1907	1910	1918	rVB4	7469	12422	0.46%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033910.D
 Acq On : 28 Jan 2022 18:55
 Operator : CG/JU
 Sample : N1302-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	14.566	1920	1926	1937	rBV	744345	1087200	40.33%	4.144%
38	14.766	1954	1960	1974	rBV2	29741	82581	3.06%	0.315%
39	14.978	1992	1996	2002	rVB8	2569	4265	0.16%	0.016%
40	15.095	2009	2016	2021	rVB6	1933	4098	0.15%	0.016%
41	15.154	2023	2026	2029	rBV3	2458	3240	0.12%	0.012%
42	15.201	2031	2034	2037	rBV2	5851	7421	0.28%	0.028%
43	15.378	2058	2064	2068	rBV2	11605	20462	0.76%	0.078%
44	15.419	2068	2071	2077	rVB2	6996	9503	0.35%	0.036%
45	15.554	2087	2094	2107	rBV	1448980	2126093	78.88%	8.104%
46	15.666	2107	2113	2128	rVV	428990	603704	22.40%	2.301%
47	15.795	2131	2135	2139	rVV3	9588	12871	0.48%	0.049%
48	15.919	2153	2156	2158	rVV4	3274	3790	0.14%	0.014%
49	15.972	2162	2165	2171	rVB6	4482	6509	0.24%	0.025%
50	16.048	2176	2178	2183	rVB6	3237	4388	0.16%	0.017%
51	16.101	2183	2187	2188	rBV3	3159	4428	0.16%	0.017%
52	16.201	2199	2204	2206	rBV5	4716	7492	0.28%	0.029%
53	16.236	2206	2210	2214	rVB6	5300	5833	0.22%	0.022%
54	16.277	2214	2217	2219	rBV3	6748	7738	0.29%	0.029%
55	16.342	2225	2228	2232	rVB6	3245	4438	0.16%	0.017%
56	16.448	2242	2246	2249	rBV3	7175	9111	0.34%	0.035%
57	16.630	2272	2277	2278	rBV5	2347	3329	0.12%	0.013%
58	16.789	2299	2304	2311	rBV10	4611	9311	0.35%	0.035%
59	17.066	2347	2351	2354	rBV2	8126	12326	0.46%	0.047%
60	17.119	2358	2360	2366	rVB5	5347	7152	0.27%	0.027%
61	17.230	2375	2379	2382	rVB4	12414	14452	0.54%	0.055%
62	17.307	2385	2392	2399	rBV	863831	1254904	46.56%	4.783%
63	17.401	2401	2408	2424	rBV	1632157	2387973	88.59%	9.102%
64	17.613	2439	2444	2451	rBV10	3310	8558	0.32%	0.033%
65	17.689	2454	2457	2461	rVV6	2798	3514	0.13%	0.013%
66	17.801	2475	2476	2479	rBV3	3435	3816	0.14%	0.015%
67	17.977	2503	2506	2512	rVB5	7128	9070	0.34%	0.035%
68	18.195	2540	2543	2549	rBV2	25300	39459	1.46%	0.150%
69	18.395	2575	2577	2580	rBV4	2809	3079	0.11%	0.012%
70	18.501	2592	2595	2600	rVB6	5530	6921	0.26%	0.026%
71	18.630	2614	2617	2619	rBV4	8405	7281	0.27%	0.028%
72	19.060	2687	2690	2693	rBV4	8137	8385	0.31%	0.032%
73	19.260	2720	2724	2727	rVB	18822	22804	0.85%	0.087%
74	19.324	2732	2735	2741	rVB2	17655	22902	0.85%	0.087%
75	19.471	2757	2760	2765	rBV7	8211	11110	0.41%	0.042%
76	19.689	2791	2797	2804	rBV	2012524	2695485	100.00%	10.274%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033910.D
Acq On : 28 Jan 2022 18:55
Operator : CG/JU
Sample : N1302-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F53

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Title : SVOA CALIBRATION

77	21.183	3048	3051	3059	rVB4	56561	79800	2.96%	0.304%
78	21.471	3095	3100	3108	rBV	966856	1301171	48.27%	4.960%
79	23.136	3380	3383	3389	rVB2	87697	123386	4.58%	0.470%
80	23.706	3474	3480	3487	rBV	1347185	2575073	95.53%	9.815%
81	23.865	3500	3507	3517	rVB2	644689	1363822	50.60%	5.198%


Sum of corrected areas: 26235063

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033910.D
Acq On : 28 Jan 2022 18:55
Operator : CG/JU
Sample : N1302-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

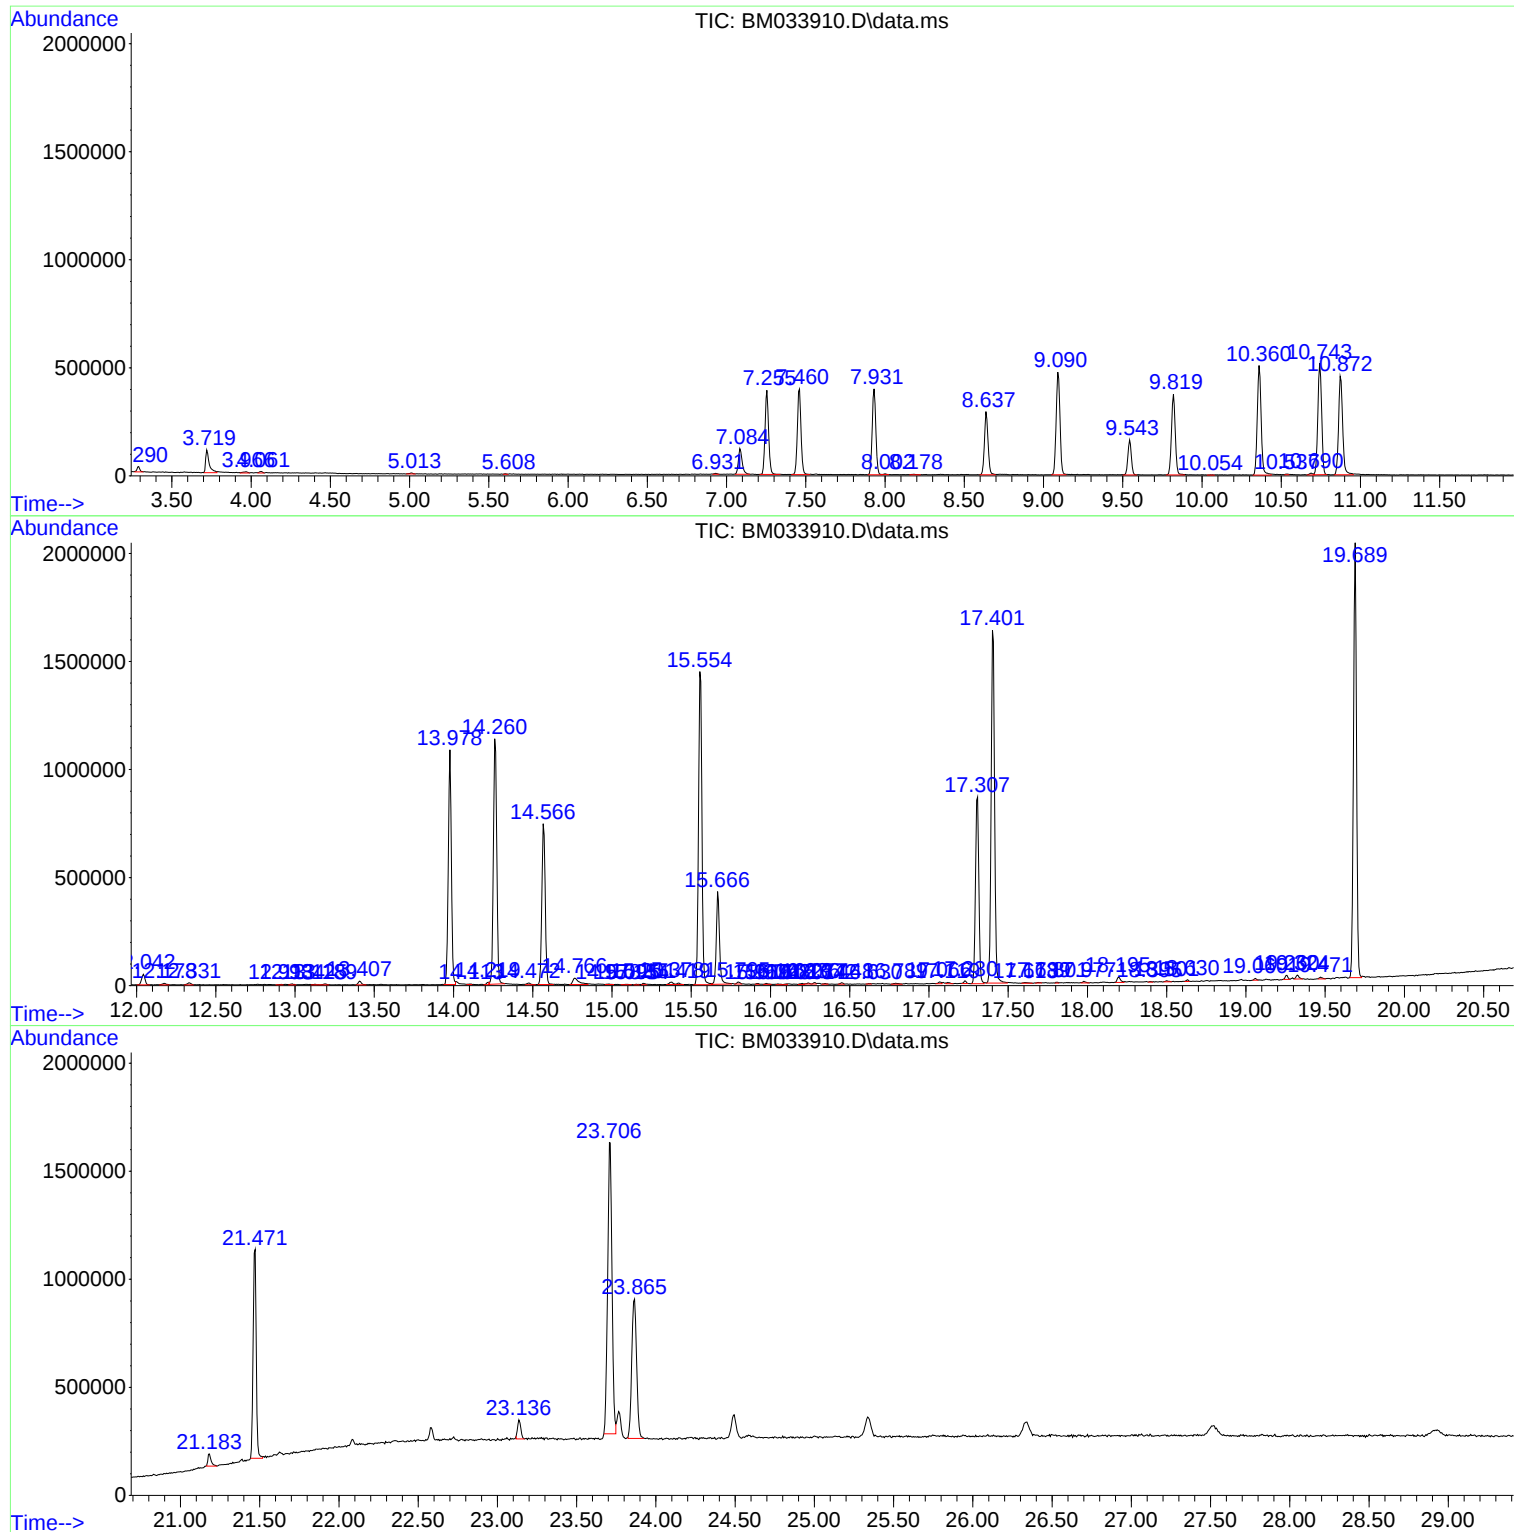

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033910.D
Acq On : 28 Jan 2022 18:55
Operator : CG/JU
Sample : N1302-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F53










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.543	5.66 ng/ul	243828	Naphthalene-d8	10.743

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	52
2			p-Trimethylsilyloxyphenyl-(trime...	398	C18H34O4Si3	1000079-05-1	47
3			4-Hydroxybenzoic acid, 2TMS deri...	282	C13H22O3Si2	002078-13-9	47
4			[(4-Hexylbenzene-1,3-diyl)bis(ox...	338	C18H34O2Si2	134273-01-1	47
5			Octopamine, 3TMS derivative	369	C17H35NO2Si3	068595-60-8	40

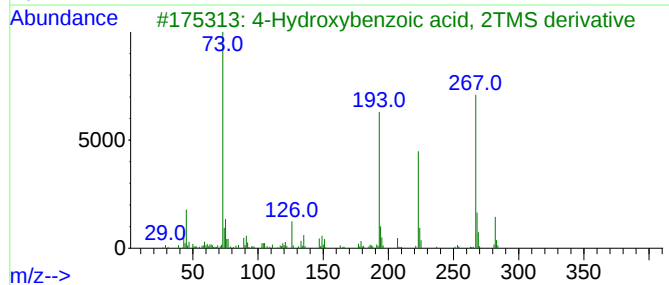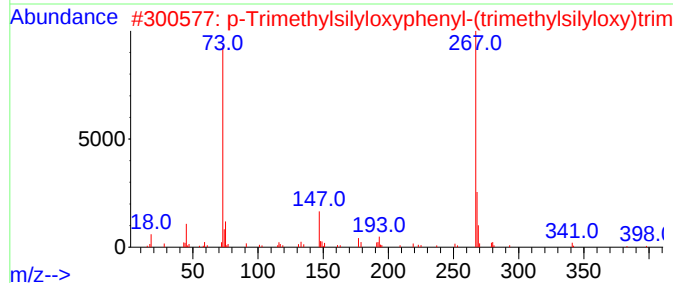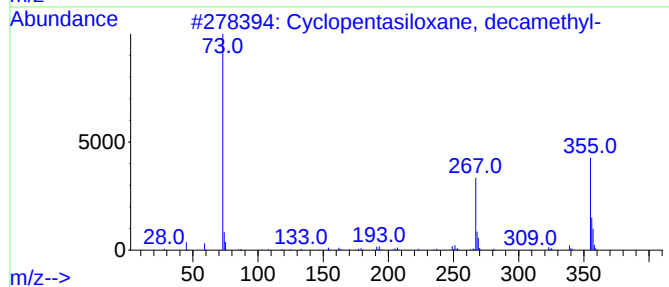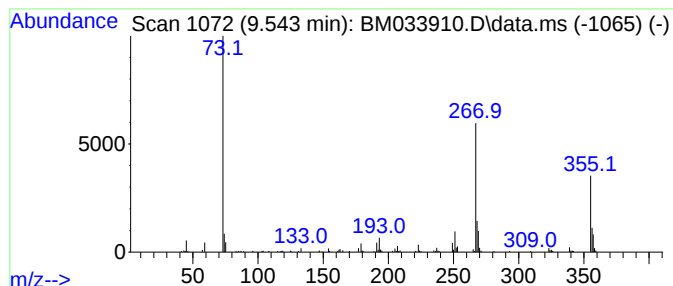

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033910.D
Acq On : 28 Jan 2022 18:55
Operator : CG/JU
Sample : N1302-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasilox...	9.543	5.7	ng/ul	243828	2	10.743	861840	20.0