

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033911.D
 Acq On : 28 Jan 2022 19:31
 Operator : CG/JU
 Sample : N1302-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	13	rBV	27267	32944	1.17%	0.123%
2	3.719	78	82	99	rBV	117386	194434	6.89%	0.727%
3	3.966	122	124	128	rVB3	5404	6580	0.23%	0.025%
4	4.060	136	140	147	rVB	8187	13959	0.49%	0.052%
5	5.013	298	302	307	rVB4	3737	5026	0.18%	0.019%
6	6.931	624	628	634	rVB7	4276	6472	0.23%	0.024%
7	7.084	649	654	665	rVB2	102923	181689	6.44%	0.680%
8	7.254	675	683	697	rBV	395003	627729	22.23%	2.348%
9	7.460	707	718	730	rBV	396718	634065	22.46%	2.372%
10	7.560	730	735	739	rBV4	2337	4468	0.16%	0.017%
11	7.931	791	798	807	rBV	390902	616935	21.85%	2.308%
12	8.001	807	810	814	rVB4	3184	4249	0.15%	0.016%
13	8.166	833	838	845	rBV8	3124	6799	0.24%	0.025%
14	8.495	888	894	897	rVB2	1943	3094	0.11%	0.012%
15	8.637	909	918	930	rBV	277101	461941	16.36%	1.728%
16	9.089	988	995	1005	rBV	478076	795440	28.17%	2.976%
17	9.542	1063	1072	1079	rVB	84663	130428	4.62%	0.488%
18	9.819	1112	1119	1129	rBV	384926	626909	22.21%	2.345%
19	10.360	1204	1211	1224	rBV	511919	868612	30.77%	3.250%
20	10.689	1260	1267	1269	rBV5	4144	5288	0.19%	0.020%
21	10.742	1269	1276	1286	rVB	511842	856252	30.33%	3.203%
22	10.872	1291	1298	1315	rBV	480329	873800	30.95%	3.269%
23	11.030	1323	1325	1330	rVB5	2200	2866	0.10%	0.011%
24	11.789	1450	1454	1457	rVB6	1779	3006	0.11%	0.011%
25	12.042	1491	1497	1502	rVB2	38892	56568	2.00%	0.212%
26	12.177	1512	1520	1525	rVB4	8696	15260	0.54%	0.057%
27	12.330	1540	1546	1553	rBV	9387	15462	0.55%	0.058%
28	12.848	1631	1634	1636	rVB3	2420	2866	0.10%	0.011%
29	12.907	1640	1644	1647	rBV4	2615	3514	0.12%	0.013%
30	12.983	1653	1657	1664	rVB6	4853	7853	0.28%	0.029%
31	13.072	1667	1672	1676	rVV7	3694	6037	0.21%	0.023%
32	13.124	1676	1681	1686	rVV8	3640	5594	0.20%	0.021%
33	13.195	1688	1693	1697	rVB6	3776	6559	0.23%	0.025%
34	13.407	1723	1729	1736	rVV4	18736	29470	1.04%	0.110%
35	13.495	1739	1744	1749	rBV7	1447	3030	0.11%	0.011%
36	13.542	1749	1752	1756	rBV3	2379	3484	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033911.D
 Acq On : 28 Jan 2022 19:31
 Operator : CG/JU
 Sample : N1302-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	13.977	1820	1826	1832	rBV	1084492	1469936	52.07%	5.499%
38	14.107	1846	1848	1854	rVB5	2924	3711	0.13%	0.014%
39	14.219	1862	1867	1868	rBV3	11978	13702	0.49%	0.051%
40	14.260	1868	1874	1888	rVB	1124080	1667988	59.08%	6.240%
41	14.477	1906	1911	1915	rVB	9373	12043	0.43%	0.045%
42	14.566	1920	1926	1937	rVV	710684	1076152	38.12%	4.026%
43	14.766	1954	1960	1975	rBV2	28528	82004	2.90%	0.307%
44	14.866	1975	1977	1981	rVB6	2205	2884	0.10%	0.011%
45	15.089	2011	2015	2020	rBV6	2113	3607	0.13%	0.013%
46	15.201	2029	2034	2038	rVB4	6277	7675	0.27%	0.029%
47	15.371	2056	2063	2067	rBV2	13192	24310	0.86%	0.091%
48	15.418	2067	2071	2077	rVB3	8799	12411	0.44%	0.046%
49	15.471	2077	2080	2084	rBV5	2269	3186	0.11%	0.012%
50	15.560	2088	2095	2106	rBV	1465193	2159650	76.50%	8.080%
51	15.665	2108	2113	2131	rVV	424508	618208	21.90%	2.313%
52	15.795	2131	2135	2139	rVV3	9044	12794	0.45%	0.048%
53	15.918	2154	2156	2161	rVB5	3521	4405	0.16%	0.016%
54	15.971	2161	2165	2169	rBV5	4841	6946	0.25%	0.026%
55	16.195	2199	2203	2205	rBV5	4793	5430	0.19%	0.020%
56	16.242	2206	2211	2214	rVV5	4621	6460	0.23%	0.024%
57	16.277	2214	2217	2220	rBV4	7137	8971	0.32%	0.034%
58	16.342	2225	2228	2233	rVB6	4294	6348	0.22%	0.024%
59	16.454	2241	2247	2251	rBV6	6626	9828	0.35%	0.037%
60	16.554	2261	2264	2267	rVB4	2294	3003	0.11%	0.011%
61	16.618	2269	2275	2278	rBV6	3766	7427	0.26%	0.028%
62	16.789	2300	2304	2308	rBV6	3115	4289	0.15%	0.016%
63	17.036	2340	2346	2347	rBV6	2217	4301	0.15%	0.016%
64	17.071	2348	2352	2354	rVV4	9969	13567	0.48%	0.051%
65	17.118	2358	2360	2364	rVB5	4883	6470	0.23%	0.024%
66	17.224	2373	2378	2383	rVB4	13904	18470	0.65%	0.069%
67	17.307	2386	2392	2401	rBV	852071	1249239	44.25%	4.674%
68	17.401	2402	2408	2420	rBV	1692427	2487626	88.11%	9.307%
69	17.542	2430	2432	2437	rVB5	3498	3834	0.14%	0.014%
70	17.612	2440	2444	2446	rBV5	3363	4872	0.17%	0.018%
71	17.677	2452	2455	2457	rBV3	4136	5967	0.21%	0.022%
72	17.812	2474	2478	2480	rBV5	4900	6017	0.21%	0.023%
73	17.977	2503	2506	2513	rVB5	7616	10990	0.39%	0.041%
74	18.195	2539	2543	2550	rBV2	31504	42900	1.52%	0.160%
75	18.501	2592	2595	2596	rBV2	5804	5428	0.19%	0.020%
76	18.630	2614	2617	2622	rVB6	7906	7843	0.28%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033911.D
 Acq On : 28 Jan 2022 19:31
 Operator : CG/JU
 Sample : N1302-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

77	18.754	2635	2638	2640	rBV3	3366	4070	0.14%	0.015%
78	18.971	2673	2675	2678	rVB4	5397	4394	0.16%	0.016%
79	19.059	2686	2690	2693	rBV4	8233	12284	0.44%	0.046%
80	19.124	2699	2701	2704	rBV4	8128	7114	0.25%	0.027%
81	19.253	2720	2723	2727	rBV2	20600	23625	0.84%	0.088%
82	19.289	2727	2729	2732	rBV3	5814	6766	0.24%	0.025%
83	19.324	2732	2735	2738	rVV2	16046	17354	0.61%	0.065%
84	19.465	2756	2759	2762	rBV5	9235	13010	0.46%	0.049%
85	19.689	2791	2797	2804	rBV	2128773	2823248	100.00%	10.562%
86	21.183	3047	3051	3058	rBV2	81088	116832	4.14%	0.437%
87	21.465	3094	3099	3106	rBV	1073401	1346848	47.71%	5.039%
88	23.706	3473	3480	3488	rBV2	1437113	2789420	98.80%	10.436%
89	23.859	3500	3506	3516	rVB2	659653	1344635	47.63%	5.031%



Sum of corrected areas: 26729174

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033911.D
Acq On : 28 Jan 2022 19:31
Operator : CG/JU
Sample : N1302-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F29

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

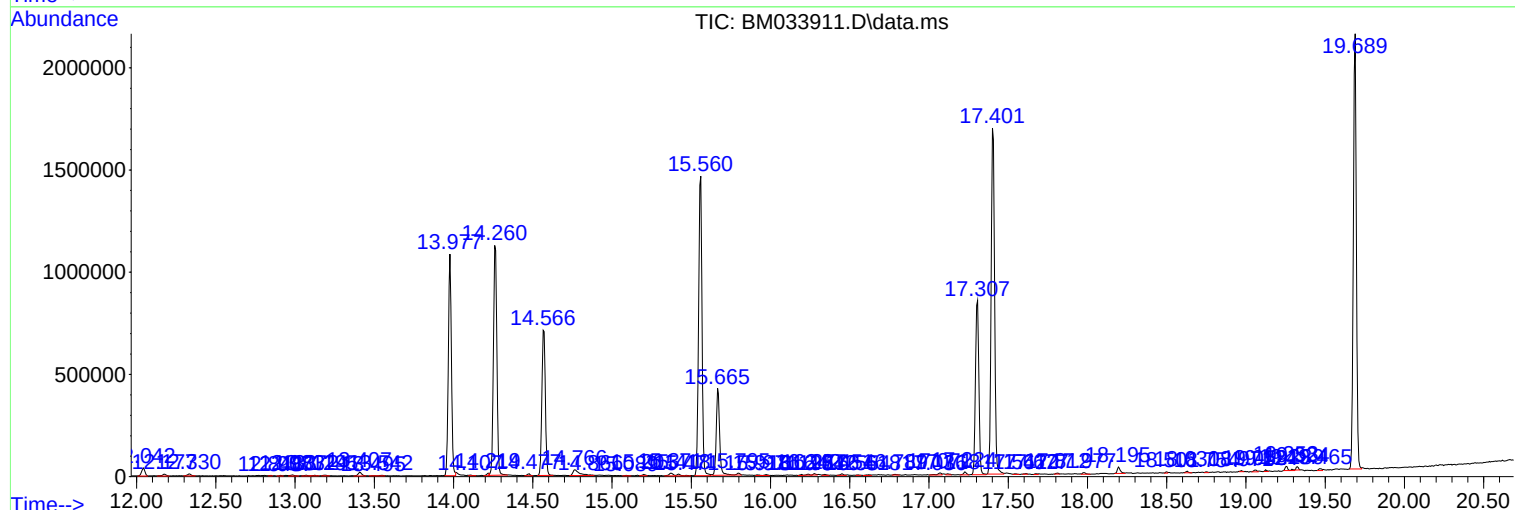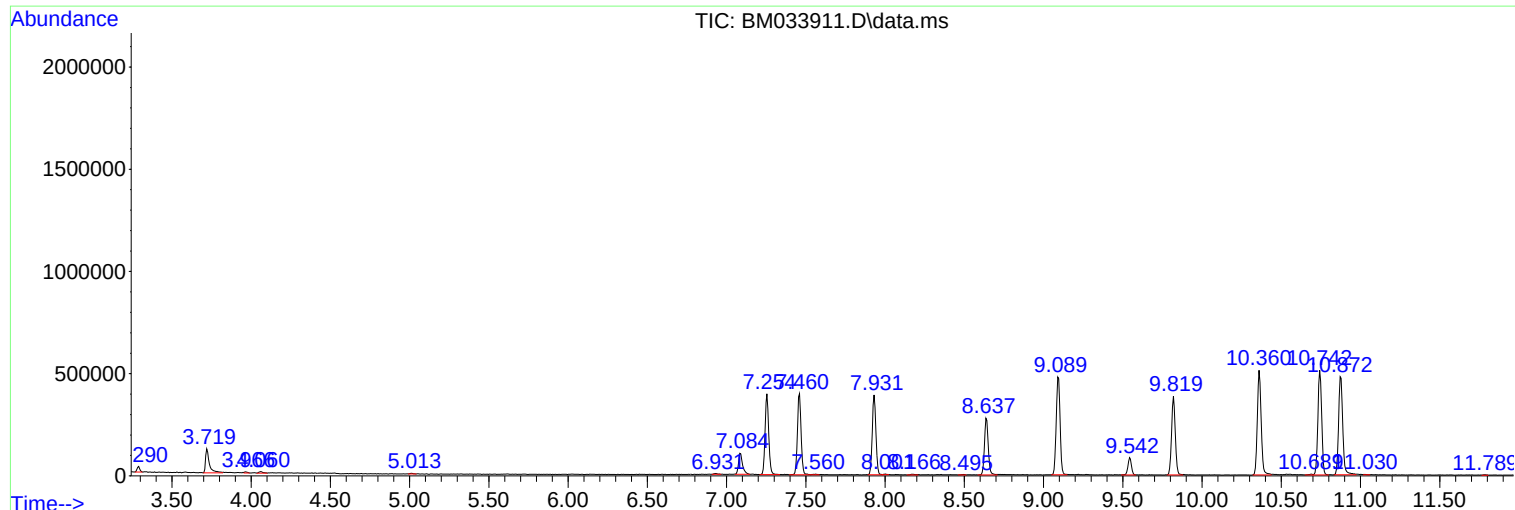

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033911.D
Acq On : 28 Jan 2022 19:31
Operator : CG/JU
Sample : N1302-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F29










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.542	3.05 ng/ul	130428	Naphthalene-d8	10.742

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	64
2			[(4-Hexylbenzene-1,3-diyl)bis(ox...	338	C18H34O2Si2	134273-01-1	43
3			Bamethan, 2TMS derivative	353	C18H35NO2Si2	040629-66-1	43
4			Octopamine, 3TMS derivative	369	C17H35NO2Si3	068595-60-8	43
5			1-(4-Hydroxyphenyl)propane-1,2-d...	384	C18H36O3Si3	1000495-85-7	43

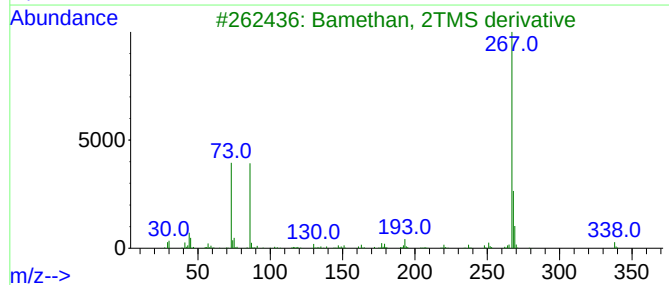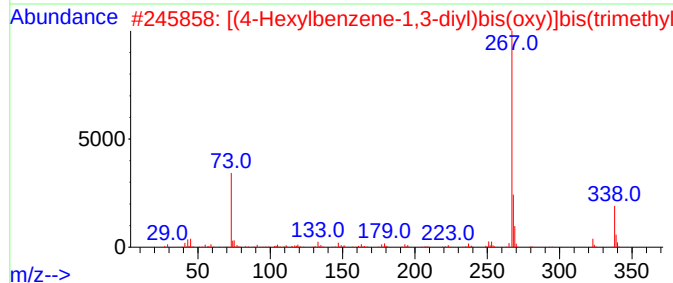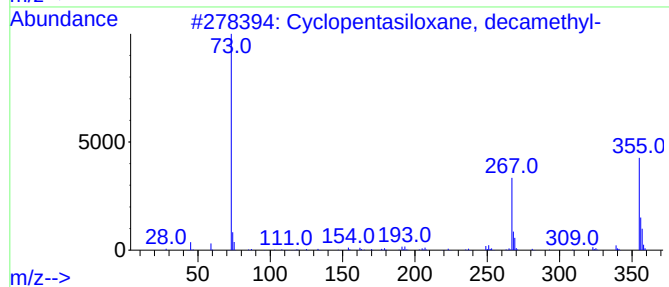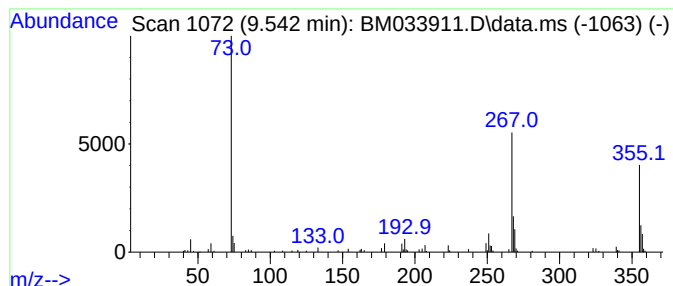

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033911.D
Acq On : 28 Jan 2022 19:31
Operator : CG/JU
Sample : N1302-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F29

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasilox...	9.542	3.0	ng/ul	130428	2	10.742	856252	20.0