

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033912.D
 Acq On : 28 Jan 2022 20:06
 Operator : CG/JU
 Sample : N1302-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	13	rBV	21520	27752	1.01%	0.111%
2	3.719	78	82	93	rBV	103760	166457	6.08%	0.667%
3	4.060	137	140	146	rVB3	6768	8890	0.32%	0.036%
4	5.007	298	301	308	rVB3	5098	7042	0.26%	0.028%
5	6.931	624	628	633	rVB4	4898	7256	0.27%	0.029%
6	7.084	649	654	665	rVB	82942	149226	5.45%	0.598%
7	7.254	676	683	692	rBV	370027	586825	21.45%	2.350%
8	7.460	711	718	731	rBV	357804	581080	21.24%	2.327%
9	7.931	791	798	806	rBV	336359	519914	19.00%	2.082%
10	7.995	807	809	814	rVB4	3628	5480	0.20%	0.022%
11	8.178	836	840	844	rBV5	2497	3047	0.11%	0.012%
12	8.637	912	918	927	rBV	256233	407104	14.88%	1.630%
13	9.090	987	995	1005	rBV	456060	754731	27.58%	3.022%
14	9.272	1022	1026	1030	rVB7	2742	3553	0.13%	0.014%
15	9.542	1066	1072	1077	rBV	21616	33047	1.21%	0.132%
16	9.819	1111	1119	1127	rBV	357224	587725	21.48%	2.354%
17	9.872	1127	1128	1135	rVB5	2754	3290	0.12%	0.013%
18	10.360	1204	1211	1221	rBV	492914	805206	29.43%	3.225%
19	10.525	1237	1239	1244	rBV4	2272	4055	0.15%	0.016%
20	10.742	1267	1276	1283	rBV	434960	735029	26.86%	2.943%
21	10.872	1290	1298	1310	rBV	450379	809800	29.60%	3.243%
22	12.042	1491	1497	1501	rBV6	1659	3310	0.12%	0.013%
23	12.172	1509	1519	1523	rBV4	7560	11460	0.42%	0.046%
24	12.330	1540	1546	1550	rBV2	8863	13789	0.50%	0.055%
25	12.807	1623	1627	1631	rBV4	1961	2801	0.10%	0.011%
26	12.977	1654	1656	1661	rVB2	4651	5993	0.22%	0.024%
27	13.054	1666	1669	1671	rBV4	2897	3023	0.11%	0.012%
28	13.125	1677	1681	1686	rBV6	3219	3805	0.14%	0.015%
29	13.189	1688	1692	1697	rVB6	3774	6352	0.23%	0.025%
30	13.407	1725	1729	1734	rBV2	17955	22817	0.83%	0.091%
31	13.977	1820	1826	1839	rVV	1025697	1413881	51.67%	5.662%
32	14.101	1843	1847	1850	rBV5	2622	3546	0.13%	0.014%
33	14.260	1868	1874	1887	rVB	1092099	1580973	57.78%	6.331%
34	14.472	1907	1910	1914	rVB3	7580	9889	0.36%	0.040%
35	14.566	1920	1926	1937	rBV	647544	956294	34.95%	3.830%
36	14.766	1955	1960	1973	rBV3	25440	72466	2.65%	0.290%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033912.D
 Acq On : 28 Jan 2022 20:06
 Operator : CG/JU
 Sample : N1302-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	15.095	2012	2016	2022	rVB7	2479	3901	0.14%	0.016%
38	15.160	2022	2027	2029	rBV6	1817	3236	0.12%	0.013%
39	15.201	2031	2034	2040	rVB7	4882	7793	0.28%	0.031%
40	15.371	2057	2063	2068	rBV3	12732	24228	0.89%	0.097%
41	15.419	2068	2071	2076	rVV4	7053	9178	0.34%	0.037%
42	15.554	2088	2094	2107	rBV	1439802	2065214	75.48%	8.270%
43	15.666	2107	2113	2130	rVV	420654	606412	22.16%	2.428%
44	15.795	2131	2135	2141	rVB7	9988	15987	0.58%	0.064%
45	15.918	2153	2156	2159	rVB5	5085	4404	0.16%	0.018%
46	15.971	2162	2165	2169	rVB5	4020	5212	0.19%	0.021%
47	16.195	2199	2203	2207	rVB6	4078	5830	0.21%	0.023%
48	16.236	2207	2210	2213	rBV4	7050	9814	0.36%	0.039%
49	16.277	2213	2217	2220	rBV4	6615	7542	0.28%	0.030%
50	16.454	2241	2247	2252	rBV6	6926	11737	0.43%	0.047%
51	16.624	2272	2276	2283	rBV8	3541	8767	0.32%	0.035%
52	16.677	2283	2285	2289	rBV4	2354	3544	0.13%	0.014%
53	16.789	2300	2304	2305	rBV3	5199	5459	0.20%	0.022%
54	16.913	2321	2325	2328	rVV6	2160	3029	0.11%	0.012%
55	17.030	2340	2345	2346	rBV4	3011	4111	0.15%	0.016%
56	17.071	2346	2352	2355	rVV4	9645	15016	0.55%	0.060%
57	17.118	2358	2360	2363	rVB3	4130	4588	0.17%	0.018%
58	17.230	2375	2379	2382	rVB3	12866	16145	0.59%	0.065%
59	17.301	2385	2391	2401	rVV	771526	1140053	41.67%	4.565%
60	17.401	2401	2408	2421	rVV	1660104	2401213	87.76%	9.616%
61	17.495	2421	2424	2428	rVB5	8109	11378	0.42%	0.046%
62	17.812	2475	2478	2480	rBV4	4569	5182	0.19%	0.021%
63	17.977	2503	2506	2511	rVB6	8659	10117	0.37%	0.041%
64	18.095	2523	2526	2527	rBV3	3591	3699	0.14%	0.015%
65	18.195	2539	2543	2549	rVV6	22455	33607	1.23%	0.135%
66	18.312	2562	2563	2566	rBV3	3632	3974	0.15%	0.016%
67	18.507	2592	2596	2598	rBV5	5662	6006	0.22%	0.024%
68	18.630	2613	2617	2620	rBV5	6735	8566	0.31%	0.034%
69	18.748	2635	2637	2641	rBV5	3831	3602	0.13%	0.014%
70	19.054	2687	2689	2695	rBV5	8321	11716	0.43%	0.047%
71	19.254	2719	2723	2727	rBV	22530	28105	1.03%	0.113%
72	19.295	2727	2730	2732	rVV3	7071	7580	0.28%	0.030%
73	19.324	2732	2735	2740	rVB2	20495	25087	0.92%	0.100%
74	19.471	2756	2760	2766	rBV9	8217	16388	0.60%	0.066%
75	19.571	2774	2777	2778	rBV3	5705	6099	0.22%	0.024%
76	19.689	2791	2797	2803	rBV	2129462	2736167	100.00%	10.957%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033912.D
Acq On : 28 Jan 2022 20:06
Operator : CG/JU
Sample : N1302-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F28

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Title : SVOA CALIBRATION

77	21.183	3047	3051	3056	rBV4	59563	94707	3.46%	0.379%
78	21.465	3094	3099	3108	rBV	986734	1287876	47.07%	5.157%
79	23.706	3473	3480	3487	rBV2	1331887	2705770	98.89%	10.836%
80	23.859	3500	3506	3516	rVB2	613418	1266315	46.28%	5.071%




Sum of corrected areas: 24971262

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033912.D
Acq On : 28 Jan 2022 20:06
Operator : CG/JU
Sample : N1302-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

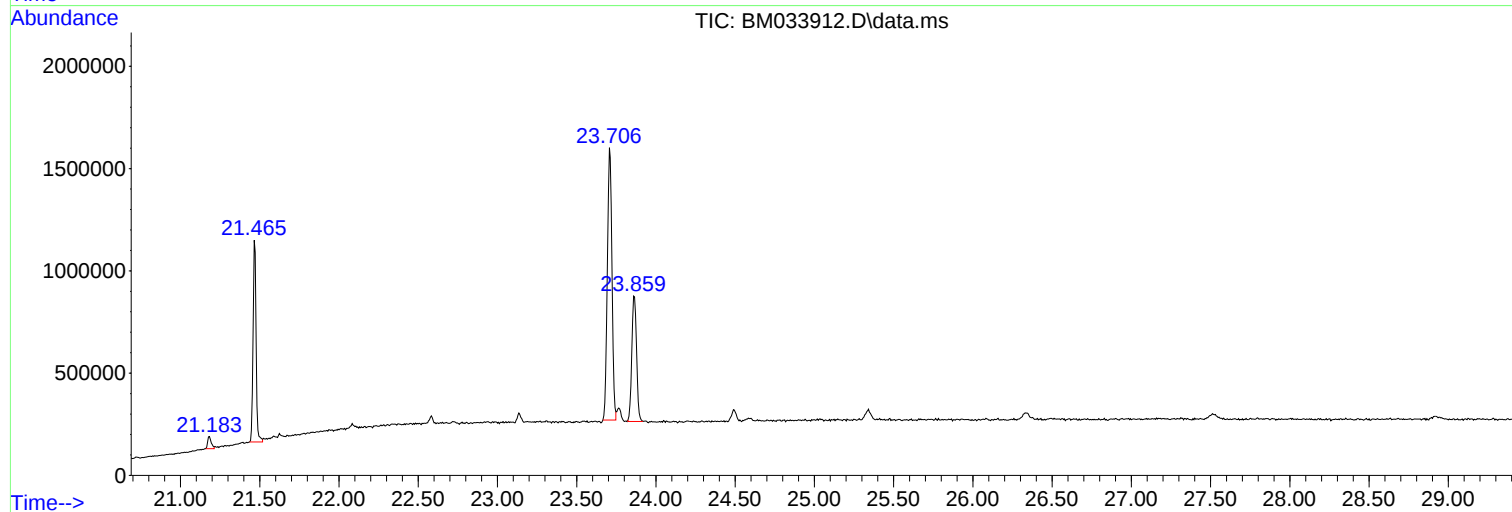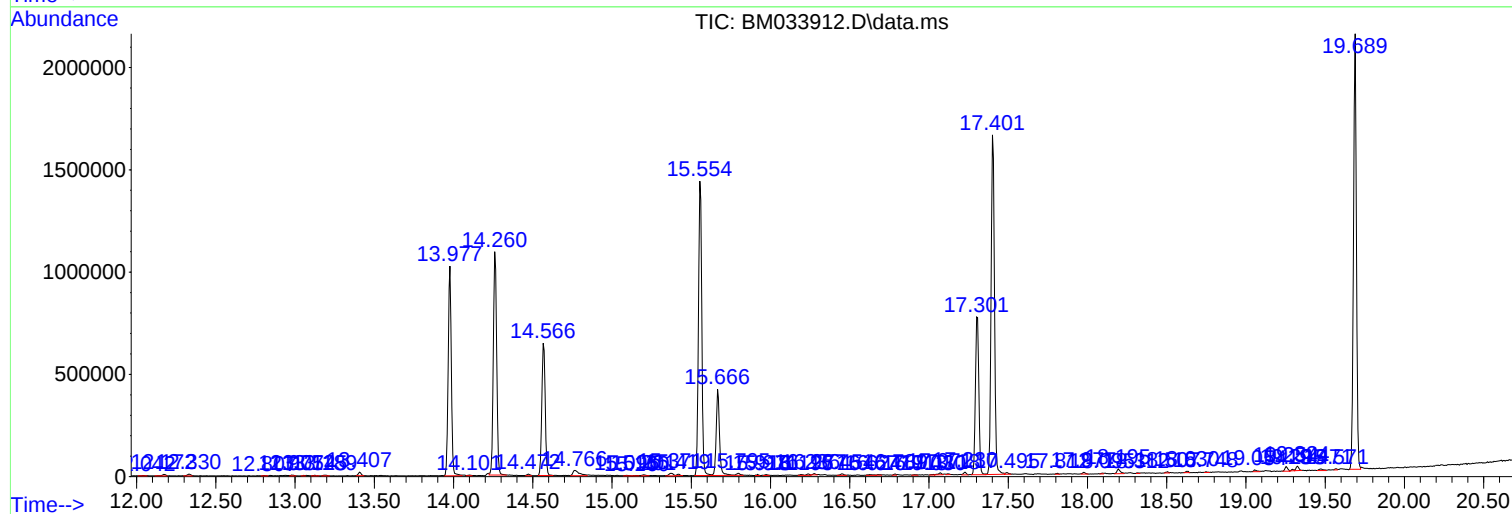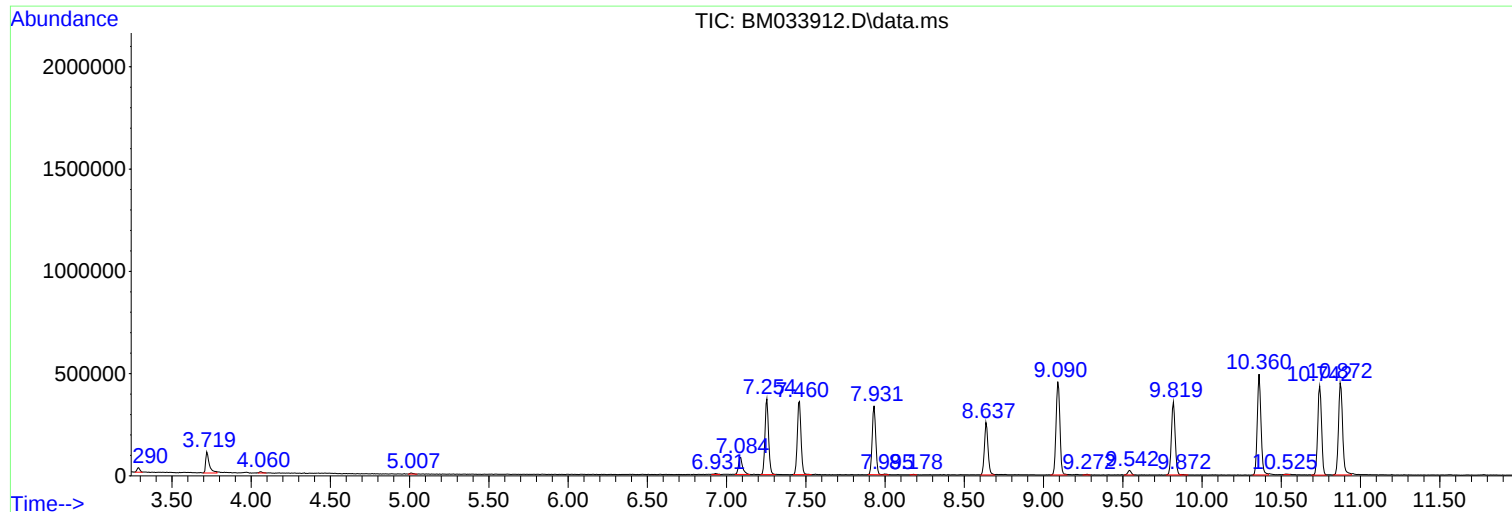

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033912.D
Acq On : 28 Jan 2022 20:06
Operator : CG/JU
Sample : N1302-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033912.D
Acq On : 28 Jan 2022 20:06
Operator : CG/JU
Sample : N1302-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc