

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033915.D
 Acq On : 28 Jan 2022 21:53
 Operator : CG/JU
 Sample : N1302-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	17	rVB	23602	33815	1.18%	0.124%
2	3.719	78	82	96	rBV	143696	219506	7.69%	0.804%
3	3.960	121	123	129	rVB3	5066	6455	0.23%	0.024%
4	4.060	136	140	146	rVB3	6989	9761	0.34%	0.036%
5	5.007	298	301	306	rVB4	4306	7621	0.27%	0.028%
6	6.925	624	627	633	rVB4	4288	7233	0.25%	0.027%
7	7.084	648	654	666	rVB2	92845	170217	5.96%	0.624%
8	7.254	675	683	693	rBV	376773	603547	21.14%	2.212%
9	7.454	710	717	727	rBV	377456	605293	21.20%	2.218%
10	7.931	791	798	805	rBV	423410	643624	22.54%	2.359%
11	8.001	808	810	815	rVB4	3932	4635	0.16%	0.017%
12	8.178	835	840	843	rBV6	2002	3273	0.11%	0.012%
13	8.637	910	918	931	rBV	274463	442633	15.50%	1.622%
14	8.760	936	939	945	rVB8	2194	3349	0.12%	0.012%
15	9.090	987	995	1004	rBV	464652	775812	27.17%	2.843%
16	9.213	1012	1016	1019	rVB4	1966	2962	0.10%	0.011%
17	9.542	1067	1072	1077	rVB	18449	28815	1.01%	0.106%
18	9.819	1112	1119	1126	rBV	373340	607161	21.26%	2.225%
19	10.360	1203	1211	1220	rBV	503012	844012	29.56%	3.093%
20	10.531	1234	1240	1250	rBV4	10481	25964	0.91%	0.095%
21	10.742	1269	1276	1283	rBV	547359	893683	31.30%	3.275%
22	10.872	1291	1298	1313	rBV	487157	874007	30.61%	3.203%
23	12.178	1514	1520	1524	rVB4	5526	8628	0.30%	0.032%
24	12.331	1540	1546	1552	rBV2	8894	15879	0.56%	0.058%
25	12.978	1654	1656	1660	rVB4	3521	3837	0.13%	0.014%
26	13.060	1664	1670	1674	rBV5	2738	5572	0.20%	0.020%
27	13.125	1677	1681	1685	rVV5	2426	3846	0.13%	0.014%
28	13.189	1685	1692	1697	rVB8	5130	8580	0.30%	0.031%
29	13.407	1724	1729	1734	rBV2	15558	22183	0.78%	0.081%
30	13.478	1736	1741	1749	rVV3	9972	15171	0.53%	0.056%
31	13.542	1749	1752	1755	rVB5	2458	3048	0.11%	0.011%
32	13.848	1800	1804	1807	rBV5	2175	3088	0.11%	0.011%
33	13.977	1819	1826	1838	rBV	1059379	1488786	52.14%	5.456%
34	14.260	1868	1874	1883	rVB	1125578	1648810	57.74%	6.043%
35	14.472	1907	1910	1915	rBV2	7143	9287	0.33%	0.034%
36	14.566	1920	1926	1940	rVB	768690	1158427	40.57%	4.245%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033915.D
 Acq On : 28 Jan 2022 21:53
 Operator : CG/JU
 Sample : N1302-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	14.766	1952	1960	1968	rBV	30961	74343	2.60%	0.272%
38	15.154	2022	2026	2029	rBV6	2206	3046	0.11%	0.011%
39	15.207	2029	2035	2041	rVB5	4827	9400	0.33%	0.034%
40	15.372	2057	2063	2068	rBV2	12484	21667	0.76%	0.079%
41	15.419	2068	2071	2076	rVB3	6907	7971	0.28%	0.029%
42	15.560	2088	2095	2107	rBV	1469529	2170152	76.00%	7.953%
43	15.666	2107	2113	2127	rVV	436395	643628	22.54%	2.359%
44	15.795	2131	2135	2143	rVV5	10784	22502	0.79%	0.082%
45	15.854	2143	2145	2149	rVB4	2273	2872	0.10%	0.011%
46	15.913	2154	2155	2159	rVB4	3871	4574	0.16%	0.017%
47	15.971	2159	2165	2167	rBV5	5005	7223	0.25%	0.026%
48	16.042	2174	2177	2181	rVB4	2108	2871	0.10%	0.011%
49	16.195	2201	2203	2206	rBV4	3709	4082	0.14%	0.015%
50	16.236	2206	2210	2214	rVV4	6763	10220	0.36%	0.037%
51	16.277	2214	2217	2220	rVV2	8699	12048	0.42%	0.044%
52	16.301	2220	2221	2225	rVV3	5237	5235	0.18%	0.019%
53	16.342	2225	2228	2231	rVV5	4364	5381	0.19%	0.020%
54	16.401	2234	2238	2240	rVB5	2365	3130	0.11%	0.011%
55	16.448	2240	2246	2252	rBV4	7230	14974	0.52%	0.055%
56	16.554	2260	2264	2266	rBV4	2645	3469	0.12%	0.013%
57	16.618	2271	2275	2277	rBV5	3806	4995	0.17%	0.018%
58	16.689	2283	2287	2288	rBV4	2745	3373	0.12%	0.012%
59	16.789	2301	2304	2306	rBV4	3896	4432	0.16%	0.016%
60	16.854	2312	2315	2318	rBV5	3275	3879	0.14%	0.014%
61	17.071	2347	2352	2359	rBV4	10159	19410	0.68%	0.071%
62	17.124	2359	2361	2365	rVB3	4560	5055	0.18%	0.019%
63	17.224	2373	2378	2382	rBV3	15741	20729	0.73%	0.076%
64	17.307	2385	2392	2401	rBV	955545	1385705	48.53%	5.078%
65	17.401	2401	2408	2421	rVV	1701488	2477129	86.75%	9.078%
66	17.495	2421	2424	2427	rVB4	6843	8214	0.29%	0.030%
67	17.613	2440	2444	2447	rVB6	3064	4800	0.17%	0.018%
68	17.683	2451	2456	2462	rBV8	6682	14446	0.51%	0.053%
69	17.807	2474	2477	2480	rVB5	3409	3956	0.14%	0.014%
70	17.977	2502	2506	2510	rBV3	11142	14098	0.49%	0.052%
71	18.101	2523	2527	2529	rBV5	2589	3759	0.13%	0.014%
72	18.195	2539	2543	2551	rBV3	33228	50977	1.79%	0.187%
73	18.507	2592	2596	2599	rVB6	5824	8932	0.31%	0.033%
74	18.536	2599	2601	2604	rBV4	2589	3403	0.12%	0.012%
75	18.630	2613	2617	2623	rVB	31952	39528	1.38%	0.145%
76	18.960	2671	2673	2681	rVB7	7092	11651	0.41%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033915.D
 Acq On : 28 Jan 2022 21:53
 Operator : CG/JU
 Sample : N1302-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

77	19.054	2687	2689	2697	rVB5	11949	15740	0.55%	0.058%
78	19.254	2719	2723	2727	rBV3	22331	31403	1.10%	0.115%
79	19.295	2727	2730	2731	rVV3	7447	6987	0.24%	0.026%
80	19.324	2732	2735	2743	rVB2	18992	30457	1.07%	0.112%
81	19.465	2756	2759	2763	rBV6	10256	16794	0.59%	0.062%
82	19.689	2791	2797	2804	rBV	2167616	2855618	100.00%	10.465%
83	21.177	3047	3050	3057	rBV2	82026	118067	4.13%	0.433%
84	21.465	3094	3099	3107	rBV	1203494	1529854	53.57%	5.607%
85	23.706	3473	3480	3487	rBV2	1412127	2814009	98.54%	10.313%
86	23.859	3500	3506	3517	rVB2	744634	1542053	54.00%	5.651%




Sum of corrected areas: 27286761

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033915.D
Acq On : 28 Jan 2022 21:53
Operator : CG/JU
Sample : N1302-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

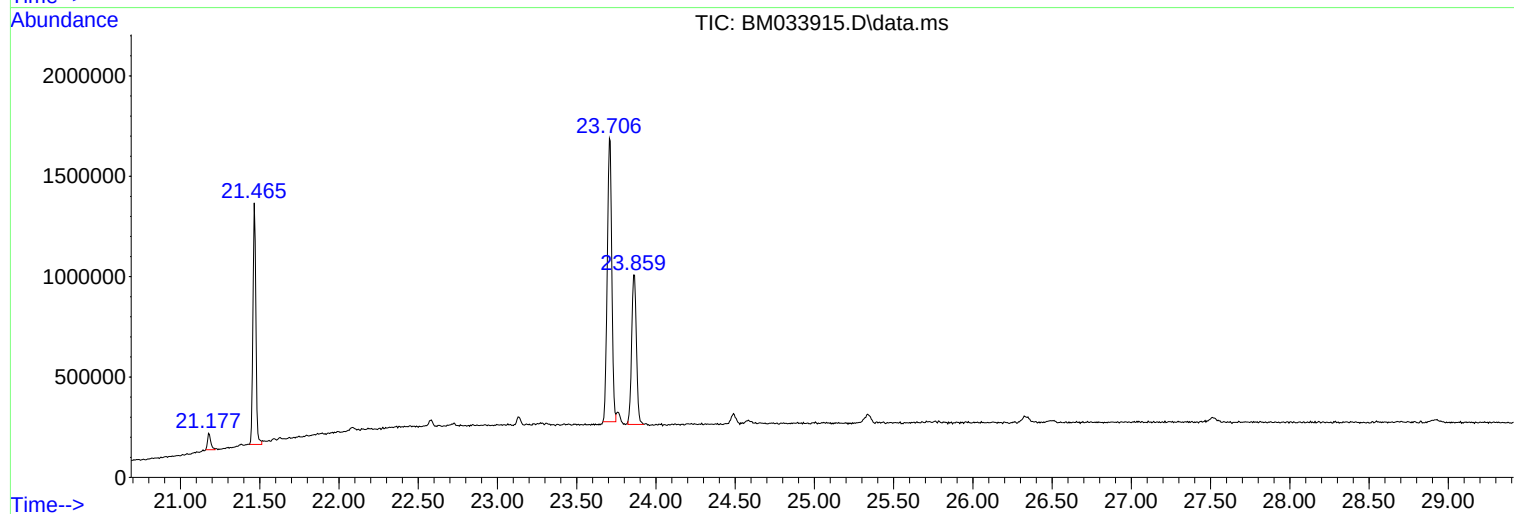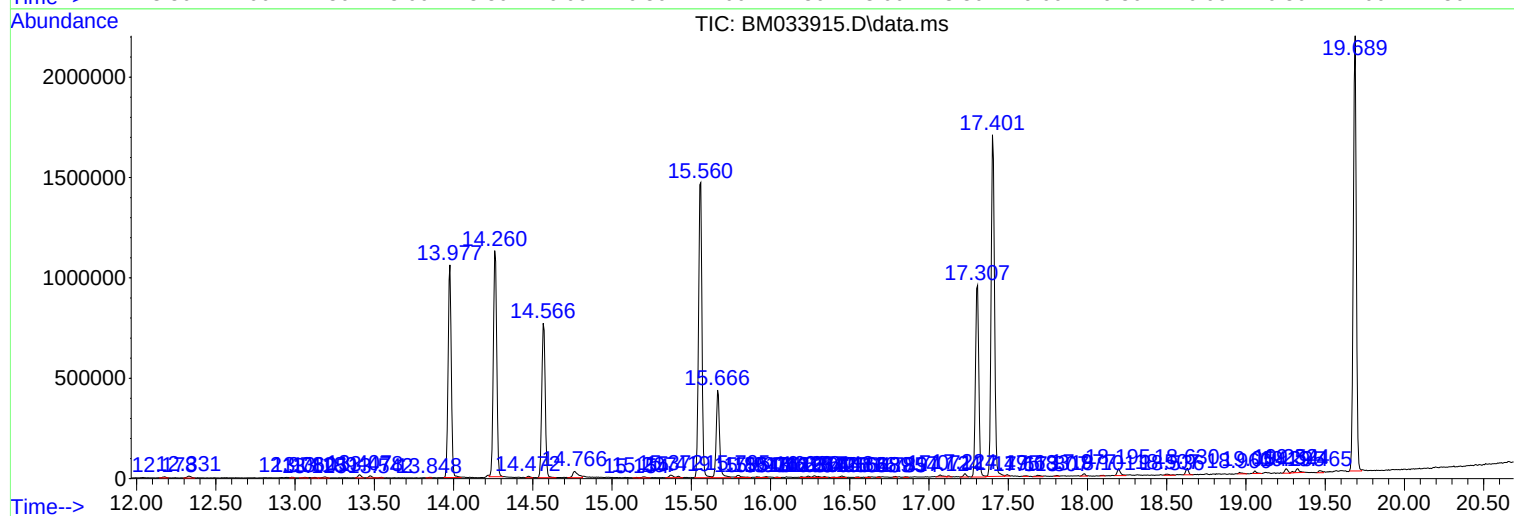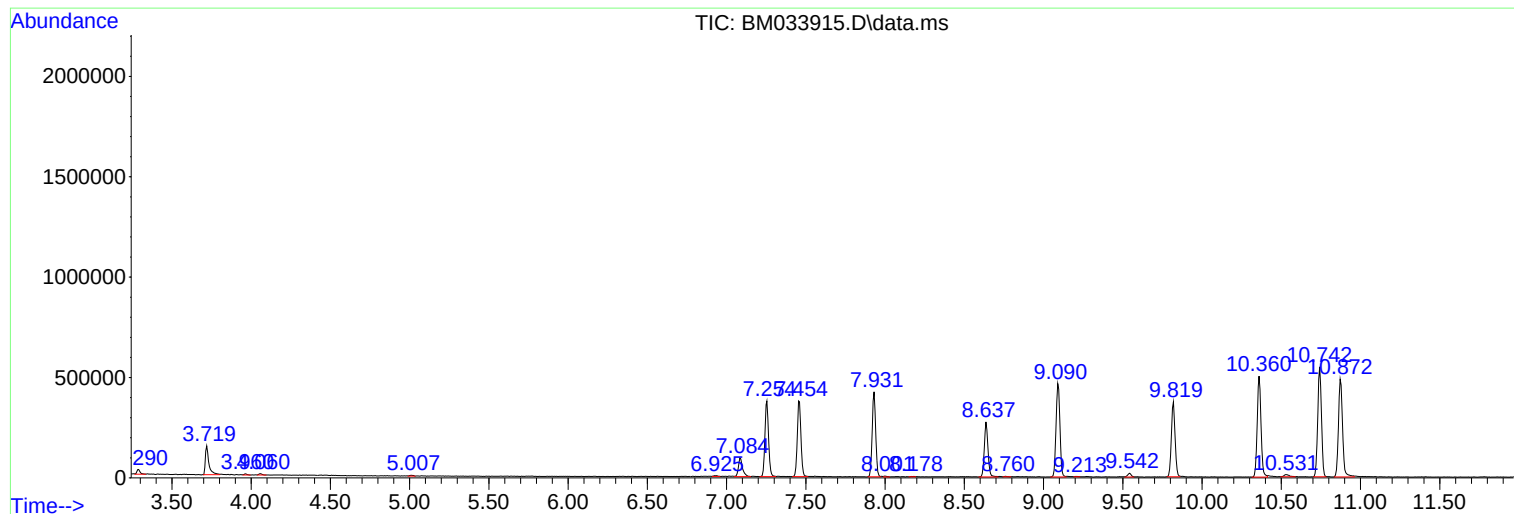

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033915.D
Acq On : 28 Jan 2022 21:53
Operator : CG/JU
Sample : N1302-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033915.D
Acq On : 28 Jan 2022 21:53
Operator : CG/JU
Sample : N1302-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc