

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033916.D
 Acq On : 28 Jan 2022 22:29
 Operator : CG/JU
 Sample : N1302-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	16	rVB2	21639	31174	1.10%	0.118%
2	3.719	79	82	97	rBV	105651	166396	5.89%	0.632%
3	3.896	110	112	115	rBV4	2728	3435	0.12%	0.013%
4	4.060	137	140	146	rVB2	7175	8792	0.31%	0.033%
5	5.013	299	302	306	rVB5	3534	4280	0.15%	0.016%
6	6.931	619	628	631	rBV7	4844	7220	0.26%	0.027%
7	7.084	649	654	664	rVB	101026	170762	6.04%	0.649%
8	7.254	674	683	693	rBV	371255	592698	20.97%	2.251%
9	7.454	710	717	729	rBV	374840	607688	21.50%	2.308%
10	7.931	791	798	805	rBV	368744	576154	20.38%	2.188%
11	7.995	808	809	815	rVB5	3040	3863	0.14%	0.015%
12	8.354	866	870	875	rBV5	1451	3002	0.11%	0.011%
13	8.636	910	918	932	rBV	284858	457045	16.17%	1.736%
14	8.766	937	940	944	rVB5	2208	3007	0.11%	0.011%
15	9.089	988	995	1008	rBV	462207	756356	26.76%	2.872%
16	9.542	1067	1072	1077	rVB	79647	115291	4.08%	0.438%
17	9.819	1109	1119	1130	rBV	377891	609353	21.56%	2.314%
18	10.360	1204	1211	1225	rBV	504852	848063	30.00%	3.221%
19	10.530	1236	1240	1242	rBV4	1972	3219	0.11%	0.012%
20	10.742	1269	1276	1284	rVV	489217	809113	28.62%	3.073%
21	10.872	1291	1298	1311	rBV	457657	811601	28.71%	3.082%
22	12.042	1490	1497	1504	rVB	46489	66552	2.35%	0.253%
23	12.177	1515	1520	1524	rVB5	4346	6691	0.24%	0.025%
24	12.336	1540	1547	1555	rVB2	8799	14498	0.51%	0.055%
25	12.530	1579	1580	1586	rVB3	2113	3090	0.11%	0.012%
26	12.777	1616	1622	1623	rBV5	2047	3543	0.13%	0.013%
27	13.189	1688	1692	1700	rVB9	2977	4834	0.17%	0.018%
28	13.407	1722	1729	1736	rBV3	11371	18112	0.64%	0.069%
29	13.542	1747	1752	1757	rVB9	2697	4717	0.17%	0.018%
30	13.854	1801	1805	1809	rVB4	2357	3913	0.14%	0.015%
31	13.977	1819	1826	1832	rBV	1069062	1482464	52.44%	5.630%
32	14.101	1844	1847	1851	rVB5	2480	3504	0.12%	0.013%
33	14.218	1863	1867	1868	rBV2	8172	8946	0.32%	0.034%
34	14.260	1868	1874	1885	rVB	1119798	1652455	58.45%	6.276%
35	14.477	1905	1911	1915	rBV4	4658	7062	0.25%	0.027%
36	14.565	1920	1926	1939	rBV	745809	1062290	37.58%	4.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033916.D
 Acq On : 28 Jan 2022 22:29
 Operator : CG/JU
 Sample : N1302-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	14.760	1953	1959	1978	rBV3	32650	95762	3.39%	0.364%
38	15.201	2031	2034	2037	rVV5	2946	4381	0.15%	0.017%
39	15.371	2059	2063	2067	rBV3	8626	13765	0.49%	0.052%
40	15.418	2067	2071	2074	rVB4	5166	6869	0.24%	0.026%
41	15.554	2088	2094	2107	rBV	1492884	2166668	76.64%	8.229%
42	15.665	2107	2113	2128	rVV	446172	638750	22.60%	2.426%
43	15.795	2131	2135	2140	rVB5	8648	12628	0.45%	0.048%
44	15.918	2148	2156	2160	rBV7	2887	6410	0.23%	0.024%
45	15.971	2162	2165	2170	rVB6	2790	3993	0.14%	0.015%
46	16.195	2199	2203	2206	rBV6	2365	3539	0.13%	0.013%
47	16.236	2206	2210	2213	rBV5	4856	5743	0.20%	0.022%
48	16.277	2213	2217	2220	rBV6	4645	6579	0.23%	0.025%
49	16.454	2241	2247	2250	rBV4	4863	7724	0.27%	0.029%
50	16.630	2271	2277	2278	rBV5	1824	3100	0.11%	0.012%
51	16.783	2298	2303	2306	rBV6	3466	4886	0.17%	0.019%
52	17.071	2349	2352	2357	rBV6	5387	8946	0.32%	0.034%
53	17.124	2359	2361	2366	rVB6	3851	3712	0.13%	0.014%
54	17.224	2375	2378	2383	rVB4	9817	12620	0.45%	0.048%
55	17.301	2385	2391	2401	rVV	878153	1263667	44.70%	4.799%
56	17.401	2401	2408	2426	rVV	1719255	2472918	87.48%	9.392%
57	17.689	2453	2457	2462	rBV7	4692	7665	0.27%	0.029%
58	17.801	2473	2476	2480	rBV6	3192	4791	0.17%	0.018%
59	17.912	2494	2495	2499	rBV4	2778	3008	0.11%	0.011%
60	17.983	2503	2507	2512	rBV7	4965	7580	0.27%	0.029%
61	18.101	2523	2527	2530	rBV6	2190	3096	0.11%	0.012%
62	18.195	2539	2543	2550	rBV4	22699	32450	1.15%	0.123%
63	18.271	2554	2556	2559	rVB4	4424	4108	0.15%	0.016%
64	18.495	2592	2594	2597	rBV4	3052	3263	0.12%	0.012%
65	18.630	2613	2617	2621	rBV3	18752	23108	0.82%	0.088%
66	19.059	2686	2690	2695	rBV7	9237	15754	0.56%	0.060%
67	19.253	2719	2723	2728	rBV2	22752	35529	1.26%	0.135%
68	19.324	2732	2735	2738	rVB	18220	22225	0.79%	0.084%
69	19.689	2791	2797	2803	rBV	2091817	2826934	100.00%	10.736%
70	21.177	3047	3050	3056	rBV4	53390	83319	2.95%	0.316%
71	21.465	3094	3099	3107	rBV	1098240	1399125	49.49%	5.314%
72	23.706	3473	3480	3487	rBV2	1403620	2798437	98.99%	10.628%
73	23.859	3500	3506	3516	rVB2	687029	1386976	49.06%	5.267%




Sum of corrected areas: 26331211

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033916.D
Acq On : 28 Jan 2022 22:29
Operator : CG/JU
Sample : N1302-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

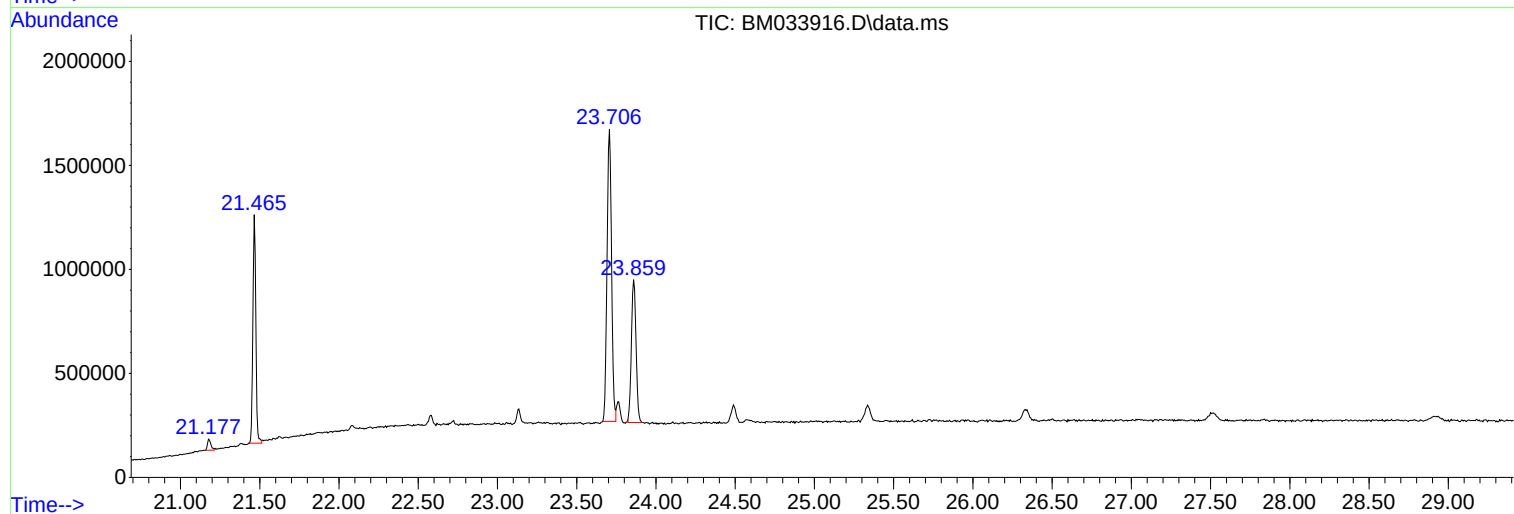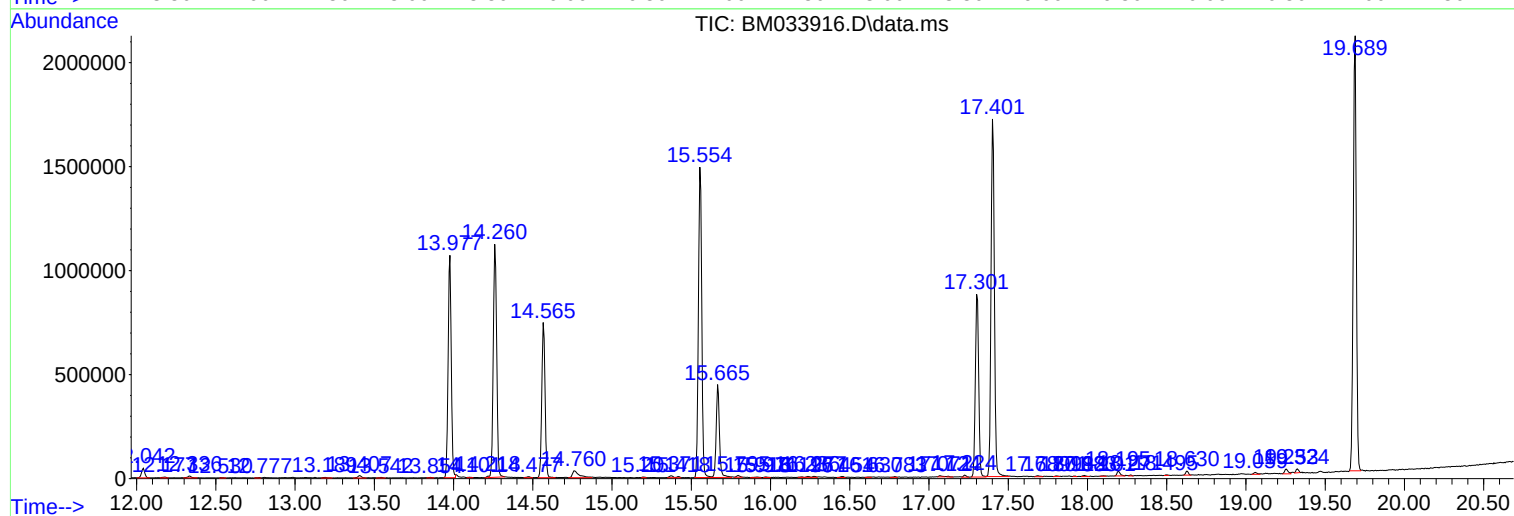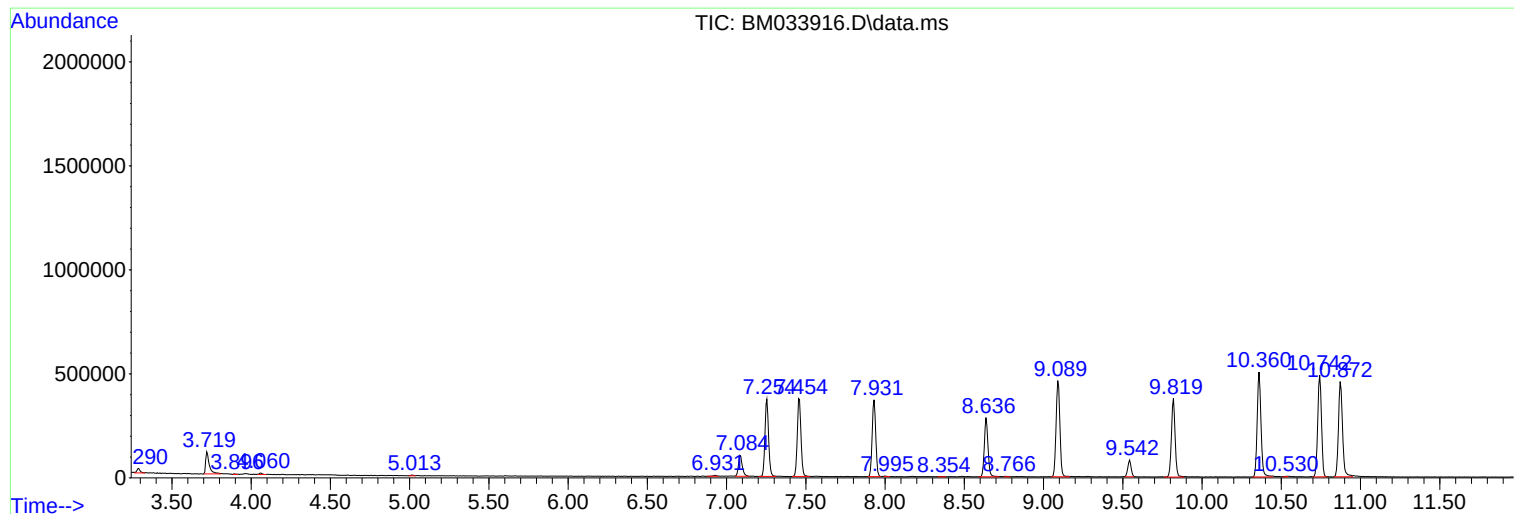

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033916.D
Acq On : 28 Jan 2022 22:29
Operator : CG/JU
Sample : N1302-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F30










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.542	2.85 ng/ul	115291	Naphthalene-d8	10.742

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	58
2			Bamethan, 2TMS derivative	353	C18H35NO2Si2	040629-66-1	38
3			4-(2-Acetylamino-1-(trimethylsil...	339	C16H29NO3Si2	1000373-43-5	38
4			4-(2-amino-1-hydroxypropyl)pheno...	311	C15H29NO2Si2	1000478-98-6	38
5			p-Trimethylsilyloxyphenyl-bis(tr...	370	C17H34O3Si3	1000079-08-1	35

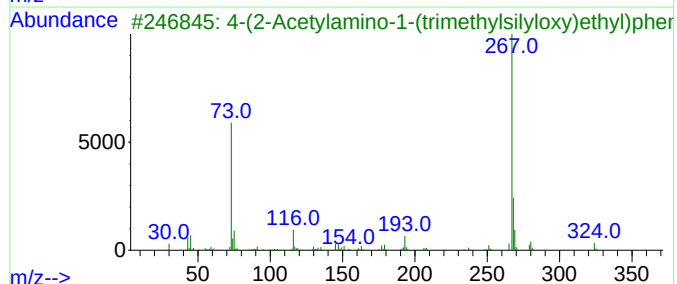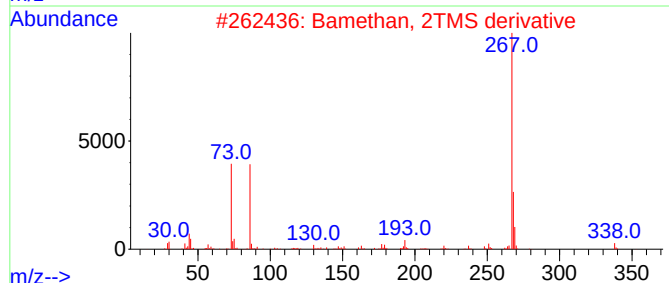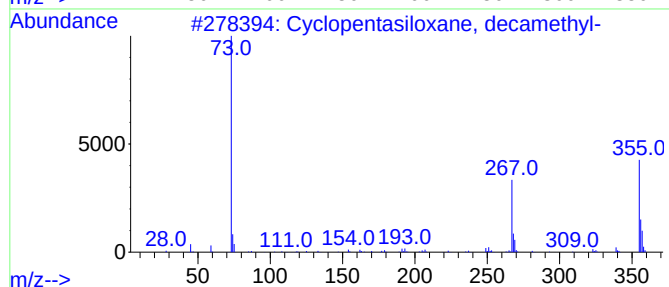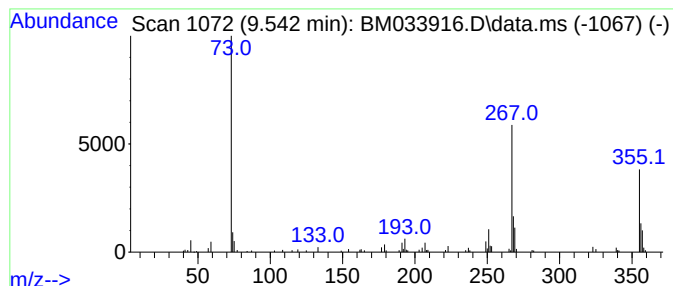

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033916.D
Acq On : 28 Jan 2022 22:29
Operator : CG/JU
Sample : N1302-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F30

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasilox...	9.542	2.9	ng/u1	115291	2	10.742	809113	20.0