

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033918.D
 Acq On : 28 Jan 2022 23:40
 Operator : CG/JU
 Sample : N1302-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	13	rVB	20851	25246	0.95%	0.101%
2	3.719	79	82	94	rBV	97215	161366	6.09%	0.648%
3	4.060	137	140	144	rVB2	6780	8376	0.32%	0.034%
4	4.584	224	229	232	rBV5	2253	3458	0.13%	0.014%
5	5.007	298	301	308	rVB3	5436	8043	0.30%	0.032%
6	5.778	427	432	434	rBV5	3138	4363	0.16%	0.018%
7	5.942	453	460	465	rVB10	6573	12123	0.46%	0.049%
8	6.931	625	628	632	rBV5	3657	4494	0.17%	0.018%
9	7.084	648	654	664	rBV2	87554	165781	6.25%	0.666%
10	7.254	674	683	692	rBV	336943	534388	20.16%	2.145%
11	7.454	711	717	729	rBV	335273	540776	20.40%	2.171%
12	7.566	732	736	739	rVB6	1994	2745	0.10%	0.011%
13	7.931	790	798	805	rBV	371753	578809	21.84%	2.324%
14	8.001	806	810	817	rVB6	5085	10116	0.38%	0.041%
15	8.178	835	840	844	rBV7	2619	4202	0.16%	0.017%
16	8.636	912	918	929	rBV	247658	394313	14.88%	1.583%
17	9.089	988	995	1006	rBV	416154	681802	25.72%	2.737%
18	9.272	1021	1026	1034	rVB8	2926	6020	0.23%	0.024%
19	9.542	1064	1072	1078	rVB2	21180	31998	1.21%	0.128%
20	9.819	1112	1119	1127	rBV	329696	535758	20.21%	2.151%
21	10.260	1189	1194	1198	rBV5	1612	3005	0.11%	0.012%
22	10.360	1204	1211	1224	rBV	454744	759399	28.65%	3.049%
23	10.530	1236	1240	1255	rVB8	9426	19447	0.73%	0.078%
24	10.742	1269	1276	1284	rBV	498750	816376	30.80%	3.278%
25	10.872	1291	1298	1318	rBV	431955	780287	29.44%	3.133%
26	12.042	1490	1497	1501	rVB3	7795	10996	0.41%	0.044%
27	12.171	1515	1519	1524	rVB2	8476	12631	0.48%	0.051%
28	12.330	1541	1546	1552	rVB2	7911	13256	0.50%	0.053%
29	12.801	1622	1626	1630	rBV5	2607	3941	0.15%	0.016%
30	12.848	1630	1634	1638	rVB5	1867	3225	0.12%	0.013%
31	12.907	1638	1644	1648	rBV7	2250	4753	0.18%	0.019%
32	12.989	1653	1658	1664	rVB6	3666	6514	0.25%	0.026%
33	13.071	1664	1672	1673	rBV5	2876	4726	0.18%	0.019%
34	13.118	1678	1680	1685	rVV5	2720	4114	0.16%	0.017%
35	13.189	1686	1692	1697	rVB5	4016	7107	0.27%	0.029%
36	13.407	1723	1729	1736	rBV2	18977	28434	1.07%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033918.D
 Acq On : 28 Jan 2022 23:40
 Operator : CG/JU
 Sample : N1302-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	13.977	1820	1826	1832	rBV	958750	1329341	50.16%	5.337%
38	14.101	1844	1847	1855	rVB9	3785	5758	0.22%	0.023%
39	14.218	1862	1867	1868	rBV2	11506	14363	0.54%	0.058%
40	14.260	1868	1874	1885	rVB	1004827	1496477	56.46%	6.008%
41	14.383	1894	1895	1900	rVB4	2430	2755	0.10%	0.011%
42	14.471	1906	1910	1915	rVB4	8098	12649	0.48%	0.051%
43	14.565	1920	1926	1936	rBV	733453	1064346	40.16%	4.273%
44	14.765	1955	1960	1974	rBV3	30396	82961	3.13%	0.333%
45	15.083	2009	2014	2015	rBV3	2232	3615	0.14%	0.015%
46	15.201	2030	2034	2038	rVB2	4604	6974	0.26%	0.028%
47	15.371	2058	2063	2068	rBV2	12701	22914	0.86%	0.092%
48	15.418	2068	2071	2075	rVB3	8091	9824	0.37%	0.039%
49	15.554	2088	2094	2107	rBV	1338317	1945424	73.40%	7.810%
50	15.665	2107	2113	2127	rVV	402007	578083	21.81%	2.321%
51	15.801	2129	2136	2139	rVB5	7936	13348	0.50%	0.054%
52	15.918	2153	2156	2159	rVB4	4984	5002	0.19%	0.020%
53	15.971	2161	2165	2170	rVB5	4443	6752	0.25%	0.027%
54	16.195	2199	2203	2207	rBV4	4210	7002	0.26%	0.028%
55	16.236	2207	2210	2214	rVB5	6656	8151	0.31%	0.033%
56	16.271	2214	2216	2219	rBV3	6397	7730	0.29%	0.031%
57	16.336	2225	2227	2230	rVB4	4173	4418	0.17%	0.018%
58	16.454	2242	2247	2251	rBV3	6633	9133	0.34%	0.037%
59	16.624	2273	2276	2278	rBV3	1964	2721	0.10%	0.011%
60	16.701	2287	2289	2293	rVB4	3563	4836	0.18%	0.019%
61	16.783	2299	2303	2310	rBV8	5719	11530	0.44%	0.046%
62	17.018	2339	2343	2347	rBV7	2277	4613	0.17%	0.019%
63	17.071	2347	2352	2355	rVV3	8707	15760	0.59%	0.063%
64	17.118	2358	2360	2364	rVB5	5754	7525	0.28%	0.030%
65	17.224	2374	2378	2382	rBV4	13605	15883	0.60%	0.064%
66	17.301	2385	2391	2401	rBV	861454	1266152	47.77%	5.083%
67	17.401	2402	2408	2421	rBV	1630479	2278592	85.97%	9.148%
68	17.612	2440	2444	2446	rBV5	3641	5708	0.22%	0.023%
69	17.806	2475	2477	2481	rVB4	3955	4120	0.16%	0.017%
70	17.977	2502	2506	2510	rVB4	8794	10212	0.39%	0.041%
71	18.089	2521	2525	2526	rBV3	3370	3738	0.14%	0.015%
72	18.195	2539	2543	2551	rBV	71472	103396	3.90%	0.415%
73	18.500	2592	2595	2600	rVB6	6472	7355	0.28%	0.030%
74	18.624	2613	2616	2621	rBV7	7283	8601	0.32%	0.035%
75	18.818	2645	2649	2650	rBV4	3593	5561	0.21%	0.022%
76	18.971	2672	2675	2677	rBV4	4624	5227	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033918.D
 Acq On : 28 Jan 2022 23:40
 Operator : CG/JU
 Sample : N1302-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

77	19.053	2686	2689	2692	rBV5	10459	15090	0.57%	0.061%
78	19.118	2698	2700	2703	rBV4	5020	5309	0.20%	0.021%
79	19.253	2719	2723	2727	rBV2	19644	25576	0.96%	0.103%
80	19.289	2727	2729	2732	rBV3	7657	8138	0.31%	0.033%
81	19.324	2732	2735	2739	rBV	19344	22741	0.86%	0.091%
82	19.465	2756	2759	2764	rBV2	31116	42236	1.59%	0.170%
83	19.689	2790	2797	2803	rBV	1947993	2650421	100.00%	10.641%
84	21.177	3047	3050	3057	rBV4	57209	81252	3.07%	0.326%
85	21.465	3094	3099	3105	rBV	1107626	1401648	52.88%	5.627%
86	23.706	3473	3480	3486	rBV2	1364121	2616608	98.72%	10.505%
87	23.859	3500	3506	3517	rVB2	728994	1448510	54.65%	5.815%




Sum of corrected areas: 24908467

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033918.D
Acq On : 28 Jan 2022 23:40
Operator : CG/JU
Sample : N1302-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

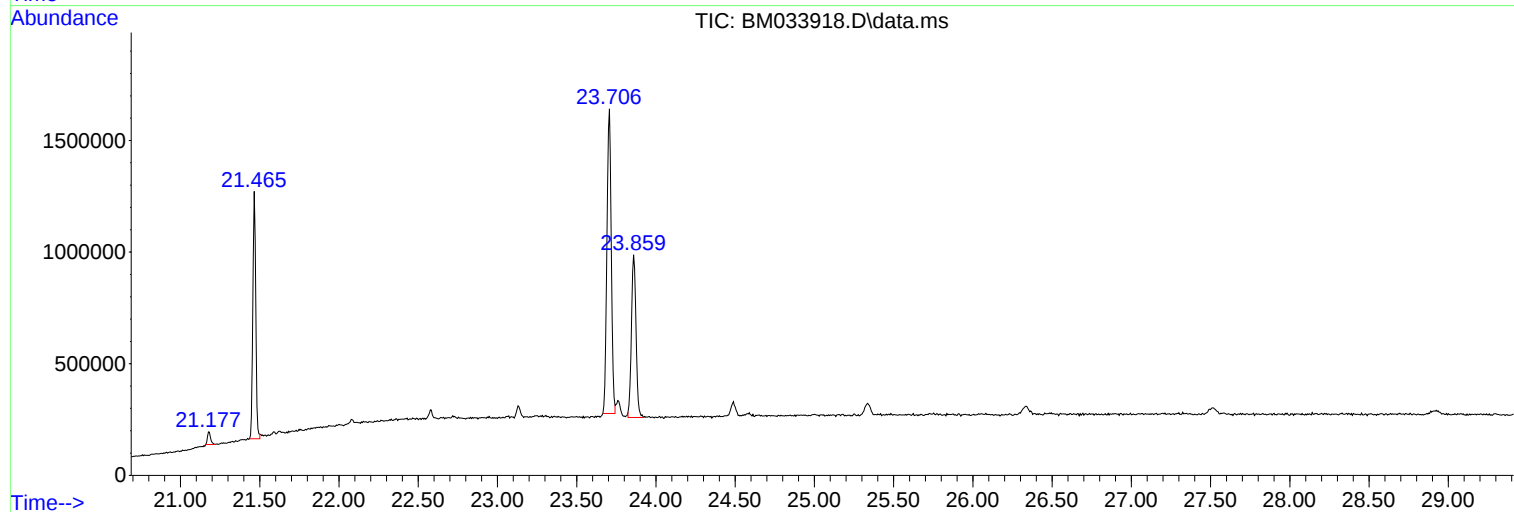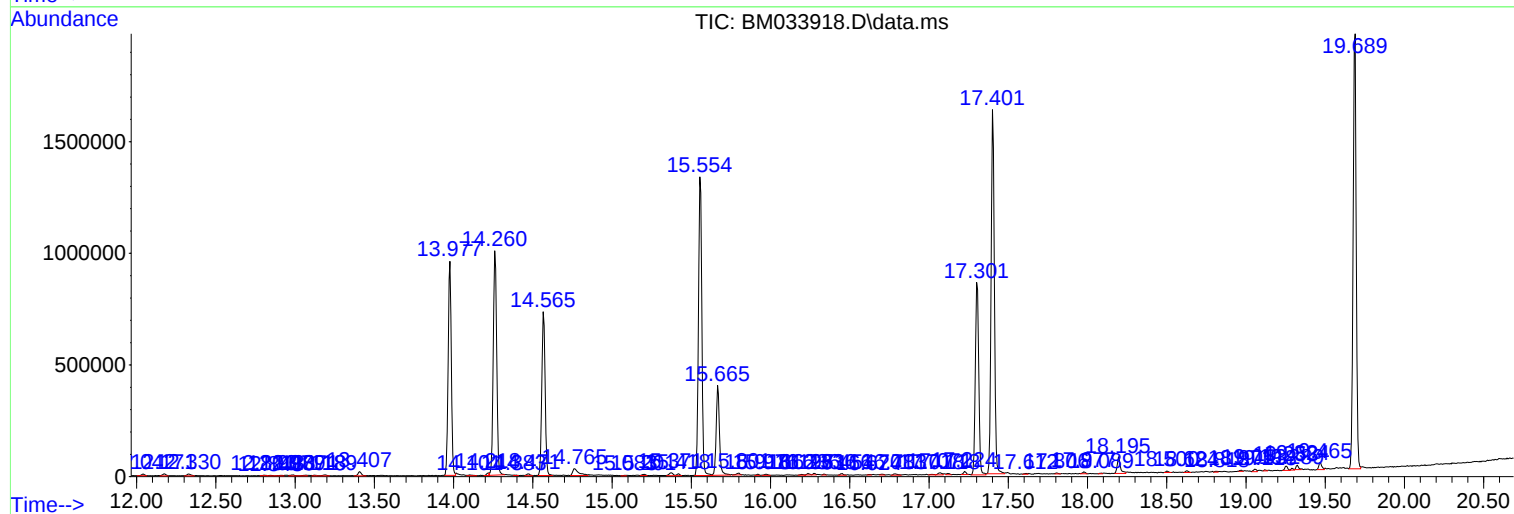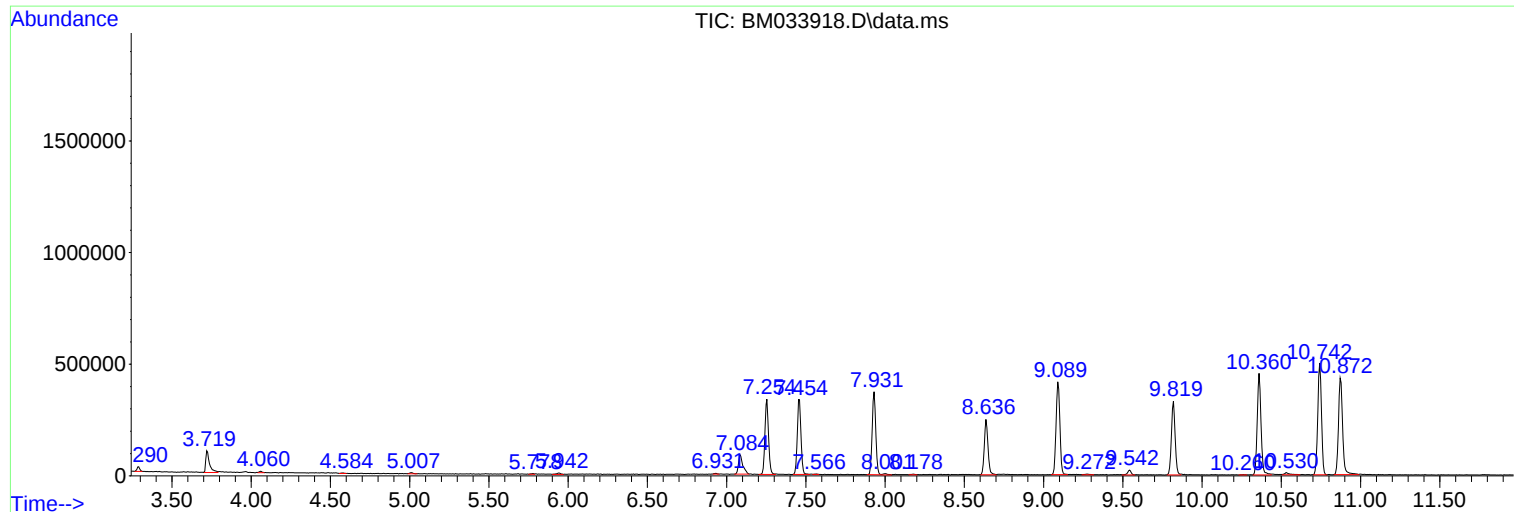

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033918.D
Acq On : 28 Jan 2022 23:40
Operator : CG/JU
Sample : N1302-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033918.D
Acq On : 28 Jan 2022 23:40
Operator : CG/JU
Sample : N1302-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc