

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033919.D
 Acq On : 29 Jan 2022 00:15
 Operator : CG/JU
 Sample : N1302-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	15	rVB	21069	29168	1.05%	0.117%
2	3.719	78	82	93	rBV	109781	171658	6.19%	0.691%
3	3.960	120	123	129	rVB5	4059	6280	0.23%	0.025%
4	4.060	137	140	144	rVB3	5841	8452	0.30%	0.034%
5	5.007	297	301	308	rVB	5433	8770	0.32%	0.035%
6	6.007	468	471	476	rVB6	1831	2955	0.11%	0.012%
7	6.931	624	628	631	rBV4	3506	4868	0.18%	0.020%
8	7.084	649	654	664	rVB2	81138	152709	5.51%	0.615%
9	7.254	673	683	694	rBV	348560	562371	20.29%	2.264%
10	7.454	711	717	728	rVB	345690	560659	20.23%	2.257%
11	7.931	791	798	805	rBV	343968	539242	19.45%	2.171%
12	7.995	805	809	814	rVB8	2693	5143	0.19%	0.021%
13	8.636	911	918	928	rBV	241974	390006	14.07%	1.570%
14	9.089	988	995	1007	rBV	442477	716040	25.83%	2.882%
15	9.278	1022	1027	1032	rVB5	2749	5646	0.20%	0.023%
16	9.542	1067	1072	1079	rVB	13543	21146	0.76%	0.085%
17	9.819	1111	1119	1133	rBV	346439	568486	20.51%	2.288%
18	10.360	1204	1211	1228	rBV	475129	789356	28.48%	3.178%
19	10.525	1235	1239	1246	rBV	14735	27579	0.99%	0.111%
20	10.742	1269	1276	1284	rVB	451713	755739	27.26%	3.042%
21	10.872	1291	1298	1309	rBV	432134	758094	27.35%	3.052%
22	12.036	1489	1496	1502	rBV4	3702	7173	0.26%	0.029%
23	12.171	1513	1519	1524	rBV5	4207	5943	0.21%	0.024%
24	12.330	1538	1546	1552	rBV4	8257	13234	0.48%	0.053%
25	13.189	1689	1692	1697	rBV6	2759	4947	0.18%	0.020%
26	13.407	1725	1729	1735	rBV5	9989	14083	0.51%	0.057%
27	13.536	1747	1751	1756	rBV5	1933	2965	0.11%	0.012%
28	13.860	1802	1806	1808	rBV3	2587	2961	0.11%	0.012%
29	13.977	1819	1826	1838	rBV	972802	1365940	49.28%	5.499%
30	14.260	1868	1874	1888	rVB	1085689	1523143	54.95%	6.131%
31	14.477	1906	1911	1914	rBV5	4517	6348	0.23%	0.026%
32	14.565	1920	1926	1939	rVB	656071	977349	35.26%	3.934%
33	14.765	1955	1960	1976	rBV4	22497	68730	2.48%	0.277%
34	14.918	1984	1986	1991	rVB4	1945	2820	0.10%	0.011%
35	14.971	1991	1995	2000	rVB8	2373	4585	0.17%	0.018%
36	15.195	2028	2033	2036	rBV6	3058	3690	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
 Data File : BM033919.D
 Acq On : 29 Jan 2022 00:15
 Operator : CG/JU
 Sample : N1302-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
 Title : SVOA CALIBRATION

37	15.377	2057	2064	2068	rBV6	3384	6203	0.22%	0.025%
38	15.418	2068	2071	2078	rVB5	7062	8865	0.32%	0.036%
39	15.554	2088	2094	2107	rBV	1371993	1995974	72.00%	8.035%
40	15.665	2107	2113	2126	rVB	394977	551789	19.91%	2.221%
41	15.795	2131	2135	2141	rVB4	8426	12601	0.45%	0.051%
42	15.971	2161	2165	2168	rBV6	3666	6109	0.22%	0.025%
43	16.242	2206	2211	2213	rVV6	4654	7269	0.26%	0.029%
44	16.277	2213	2217	2220	rVV6	6535	10124	0.37%	0.041%
45	16.301	2220	2221	2225	rVV4	5626	5854	0.21%	0.024%
46	16.336	2225	2227	2233	rVB5	3791	4298	0.16%	0.017%
47	16.448	2241	2246	2249	rBV6	5006	7529	0.27%	0.030%
48	16.624	2269	2276	2278	rBV6	3634	5956	0.21%	0.024%
49	16.671	2283	2284	2287	rBV3	2532	3060	0.11%	0.012%
50	16.706	2287	2290	2293	rVB4	2528	3749	0.14%	0.015%
51	16.783	2299	2303	2306	rBV4	2214	3689	0.13%	0.015%
52	16.842	2311	2313	2319	rBV6	2339	4283	0.15%	0.017%
53	16.918	2322	2326	2330	rBV7	2041	3976	0.14%	0.016%
54	17.065	2348	2351	2354	rBV3	7577	10377	0.37%	0.042%
55	17.118	2358	2360	2368	rVB7	6589	11048	0.40%	0.044%
56	17.301	2385	2391	2401	rBV	819165	1169954	42.21%	4.710%
57	17.401	2402	2408	2420	rVV	1589069	2283451	82.38%	9.192%
58	17.689	2452	2457	2462	rBV9	7534	13436	0.48%	0.054%
59	17.724	2462	2463	2469	rVB5	3968	4888	0.18%	0.020%
60	17.806	2475	2477	2481	rVB4	4873	4414	0.16%	0.018%
61	17.889	2488	2491	2494	rBV5	2425	3835	0.14%	0.015%
62	17.977	2503	2506	2510	rVB3	7401	8626	0.31%	0.035%
63	18.195	2539	2543	2547	rBV2	48270	61760	2.23%	0.249%
64	18.306	2559	2562	2564	rBV4	2673	3409	0.12%	0.014%
65	18.630	2612	2617	2621	rBV2	54155	64595	2.33%	0.260%
66	19.059	2686	2690	2693	rBV6	8188	11662	0.42%	0.047%
67	19.253	2720	2723	2727	rBV3	18467	22591	0.81%	0.091%
68	19.324	2732	2735	2743	rVV	20928	32299	1.17%	0.130%
69	19.465	2756	2759	2763	rBV5	17338	22354	0.81%	0.090%
70	19.689	2791	2797	2807	rBV	1982263	2730409	98.50%	10.991%
71	19.783	2809	2813	2819	rVV2	56929	78348	2.83%	0.315%
72	21.177	3047	3050	3057	rVB2	63797	87266	3.15%	0.351%
73	21.383	3082	3085	3092	rVB	41744	47729	1.72%	0.192%
74	21.465	3094	3099	3107	rBV	1009813	1319263	47.59%	5.311%
75	23.706	3473	3480	3487	rBV2	1406759	2772005	100.00%	11.159%
76	23.859	3500	3506	3517	rVB2	649295	1348051	48.63%	5.427%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033919.D
Acq On : 29 Jan 2022 00:15
Operator : CG/JU
Sample : N1302-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F23

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Title : SVOA CALIBRATION


Sum of corrected areas: 24841376

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033919.D
Acq On : 29 Jan 2022 00:15
Operator : CG/JU
Sample : N1302-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

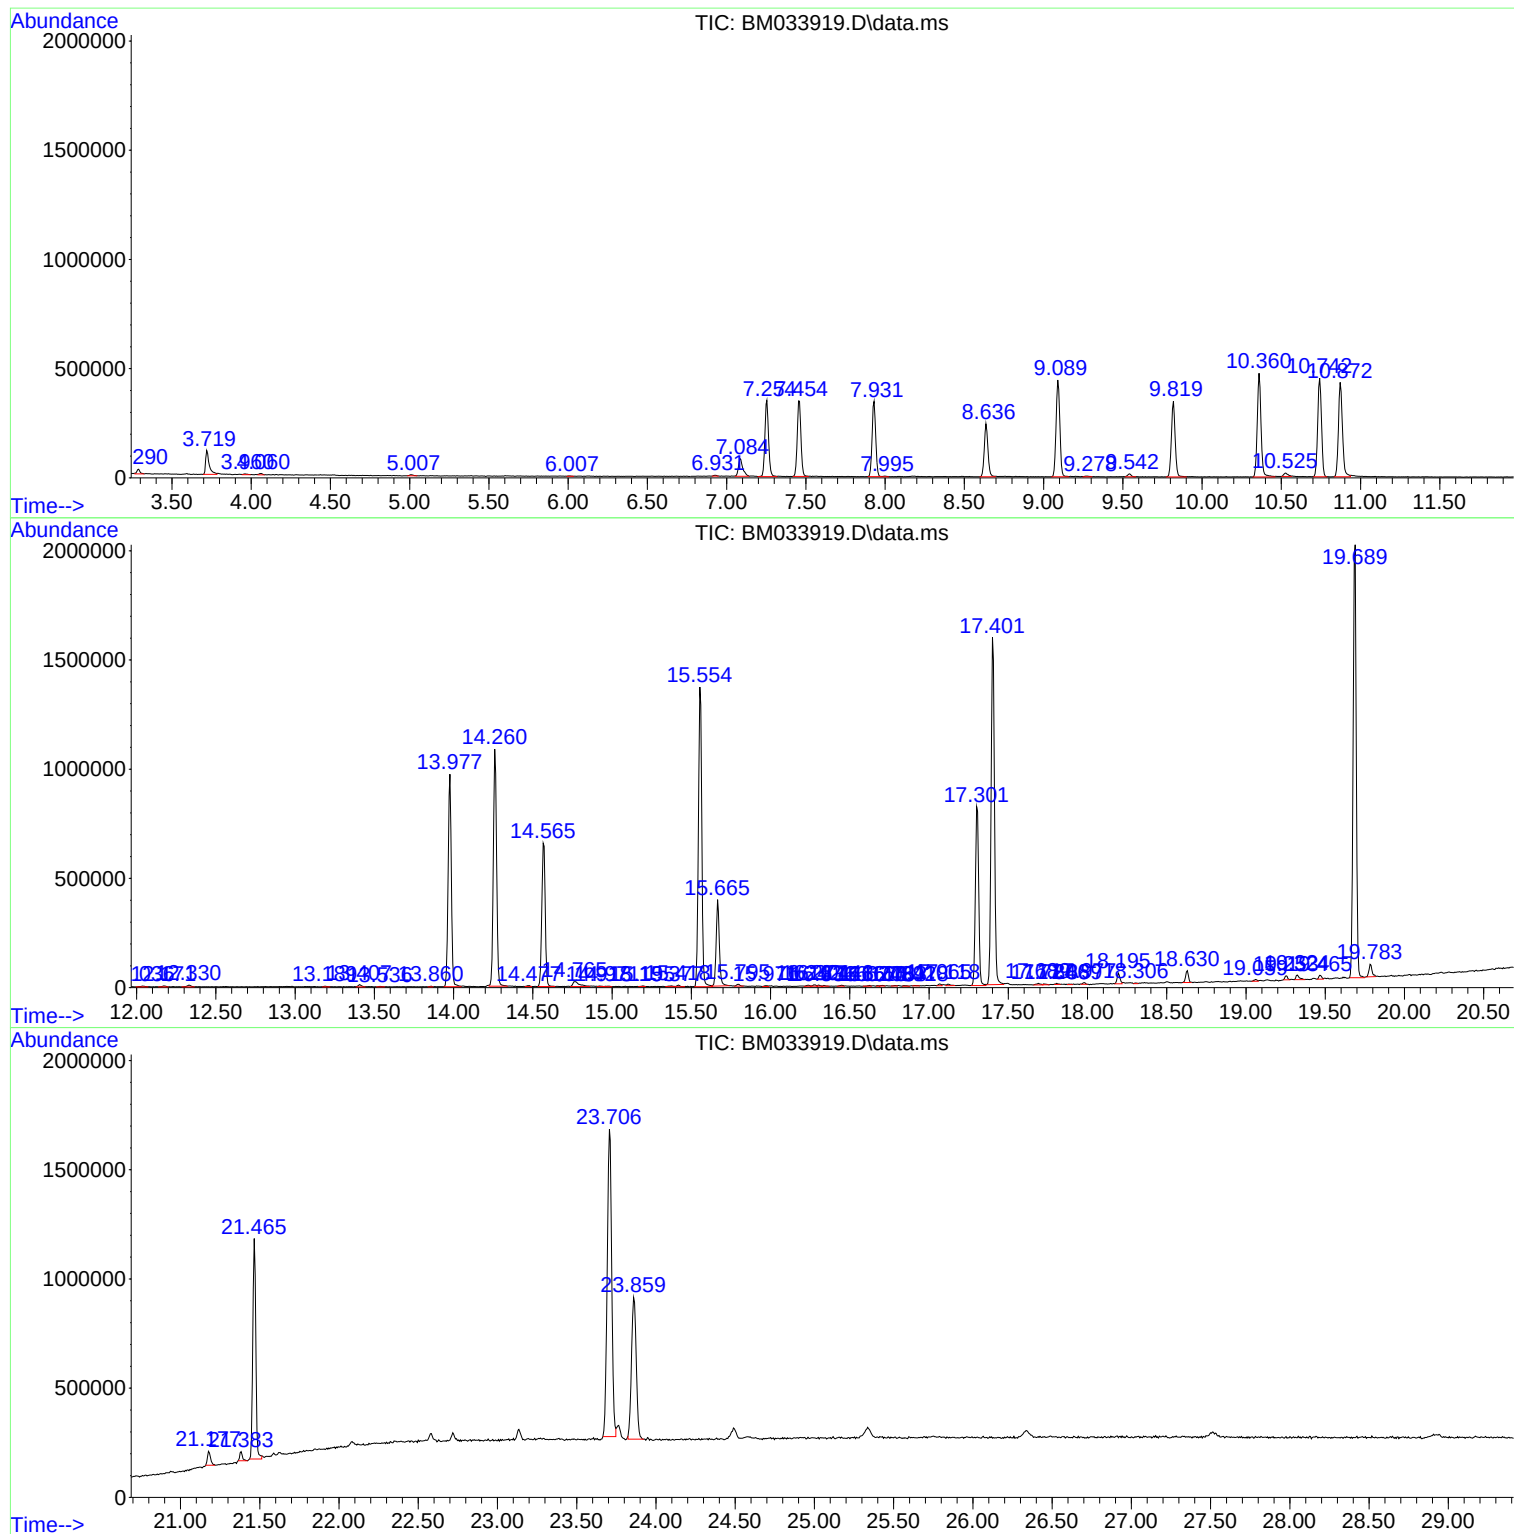

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033919.D
Acq On : 29 Jan 2022 00:15
Operator : CG/JU
Sample : N1302-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012822\
Data File : BM033919.D
Acq On : 29 Jan 2022 00:15
Operator : CG/JU
Sample : N1302-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc