
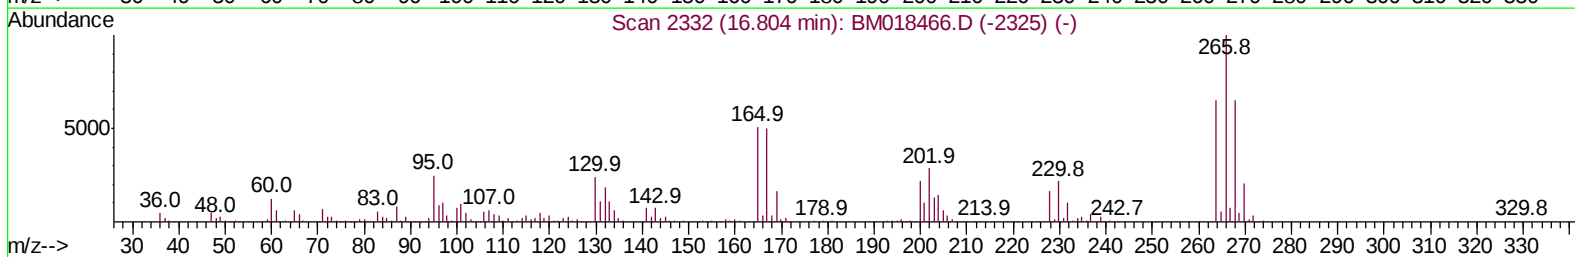
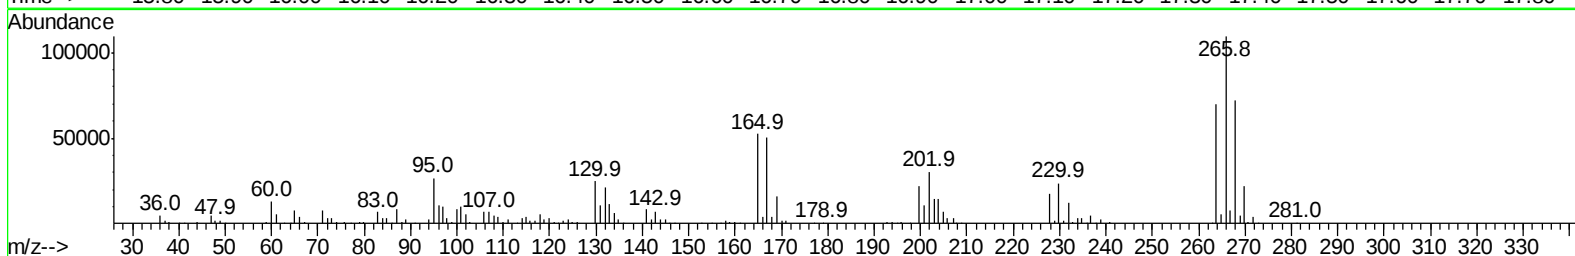


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012919\
Data File : BM018676.D
Acq On : 29 Jan 2019 14:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 00:51:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

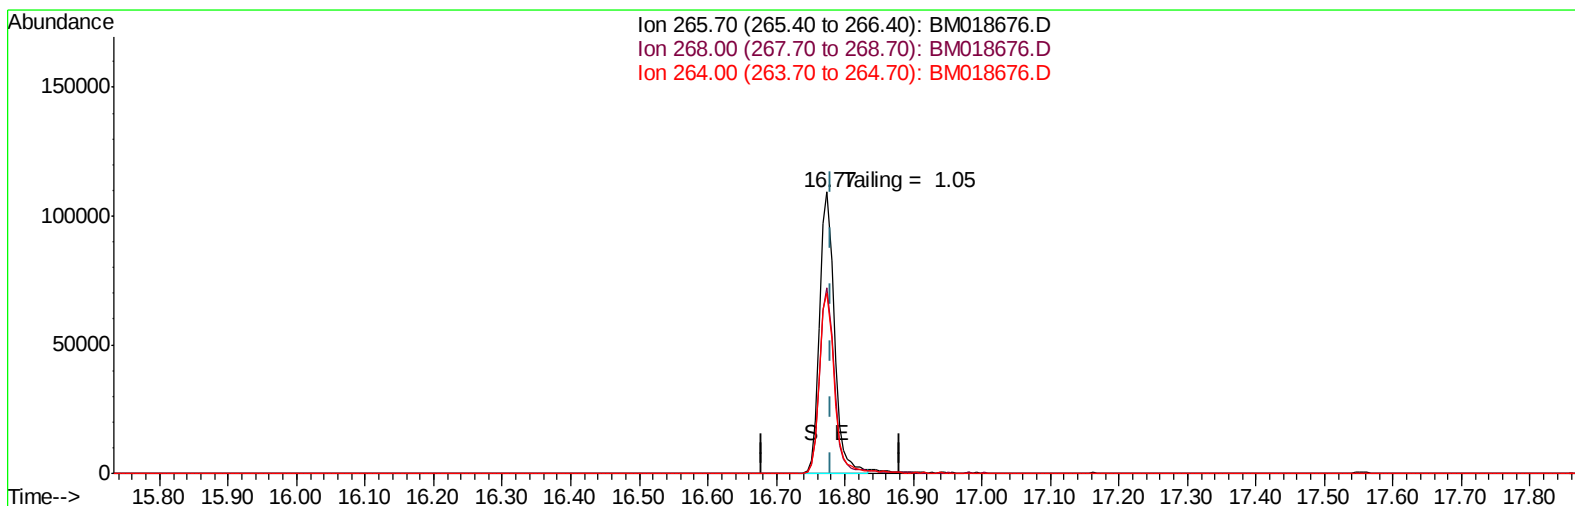

TIC: BM018676.D

(70) Pentachlorophenol (C)




16.774min (-0.006) 186061.62ng

response 164870

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	65.78
264.00	62.60	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012919\
Data File : BM018676.D
Acq On : 29 Jan 2019 14:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 00:51:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

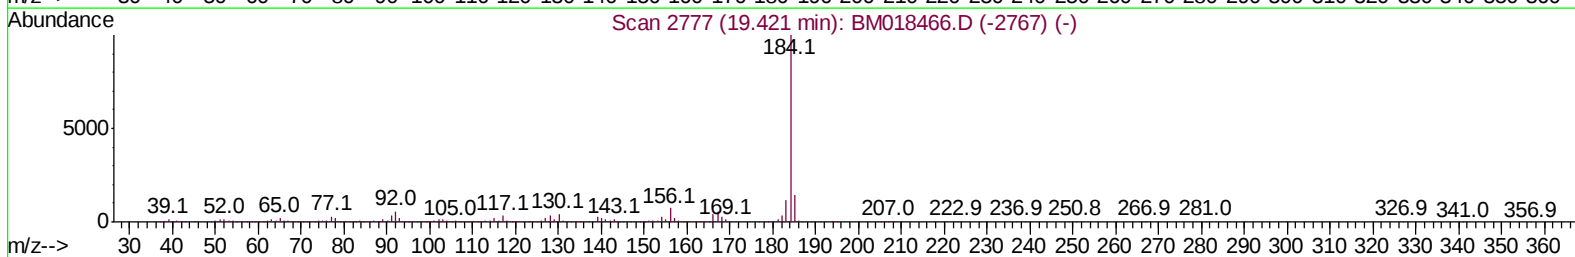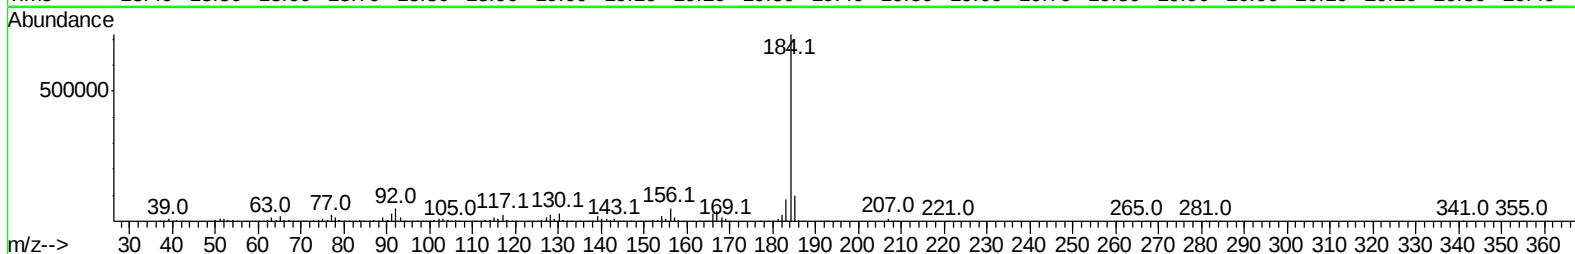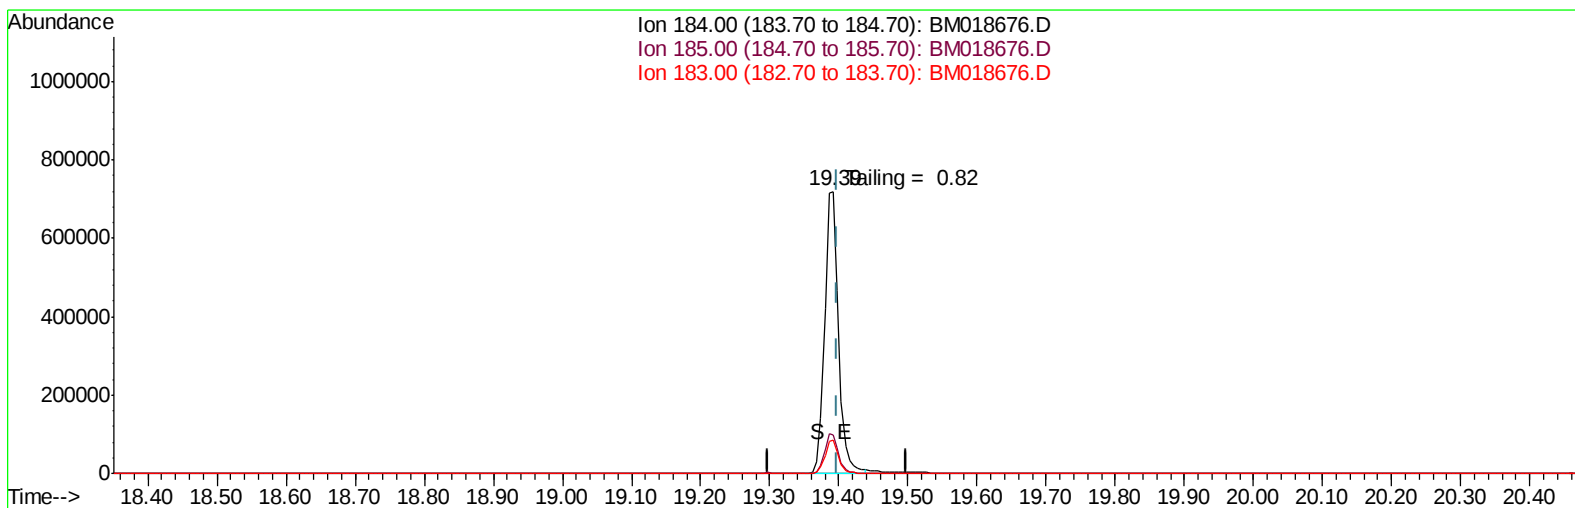

TIC: BM018676.D

(77) Benzidine

19.392min (-0.006) 3224.86ng

response 1011576

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.75
183.00	11.90	11.88
0.00	0.00	0.00