

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012919\
 Data File : BM018684.D
 Acq On : 29 Jan 2019 19:12
 Operator : JU/SJ
 Sample : K1008-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 HD-01-012819

Quant Time: Jan 30 00:25:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 22:01:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	218921	20.00	ng	-0.01
21) Naphthalene-d8	10.52	136	803339	20.00	ng	-0.01
39) Acenaphthene-d10	14.37	164	413938	20.00	ng	-0.01
64) Phenanthrene-d10	17.13	188	853322	20.00	ng	-0.01
76) Chrysene-d12	21.32	240	778350	20.00	ng	-0.02
87) Perylene-d12	23.59	264	777032	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	1638804	138.23	ng	-0.01
7) Phenol-d6	6.90	99	1883634	125.09	ng	-0.01
23) Nitrobenzene-d5	8.89	82	1490621	107.57	ng	-0.01
42) 2,4,6-Tribromophenol	15.87	330	728667	138.25	ng	-0.02
45) 2-Fluorobiphenyl	12.99	172	3105049	97.88	ng	-0.01
79) Terphenyl-d14	19.76	244	3747514	101.50	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM012919\
Data File : BM018684.D
Acq On : 29 Jan 2019 19:12
Operator : JU/SJ
Sample : K1008-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
HD-01-012819

Quant Time: Jan 30 00:25:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

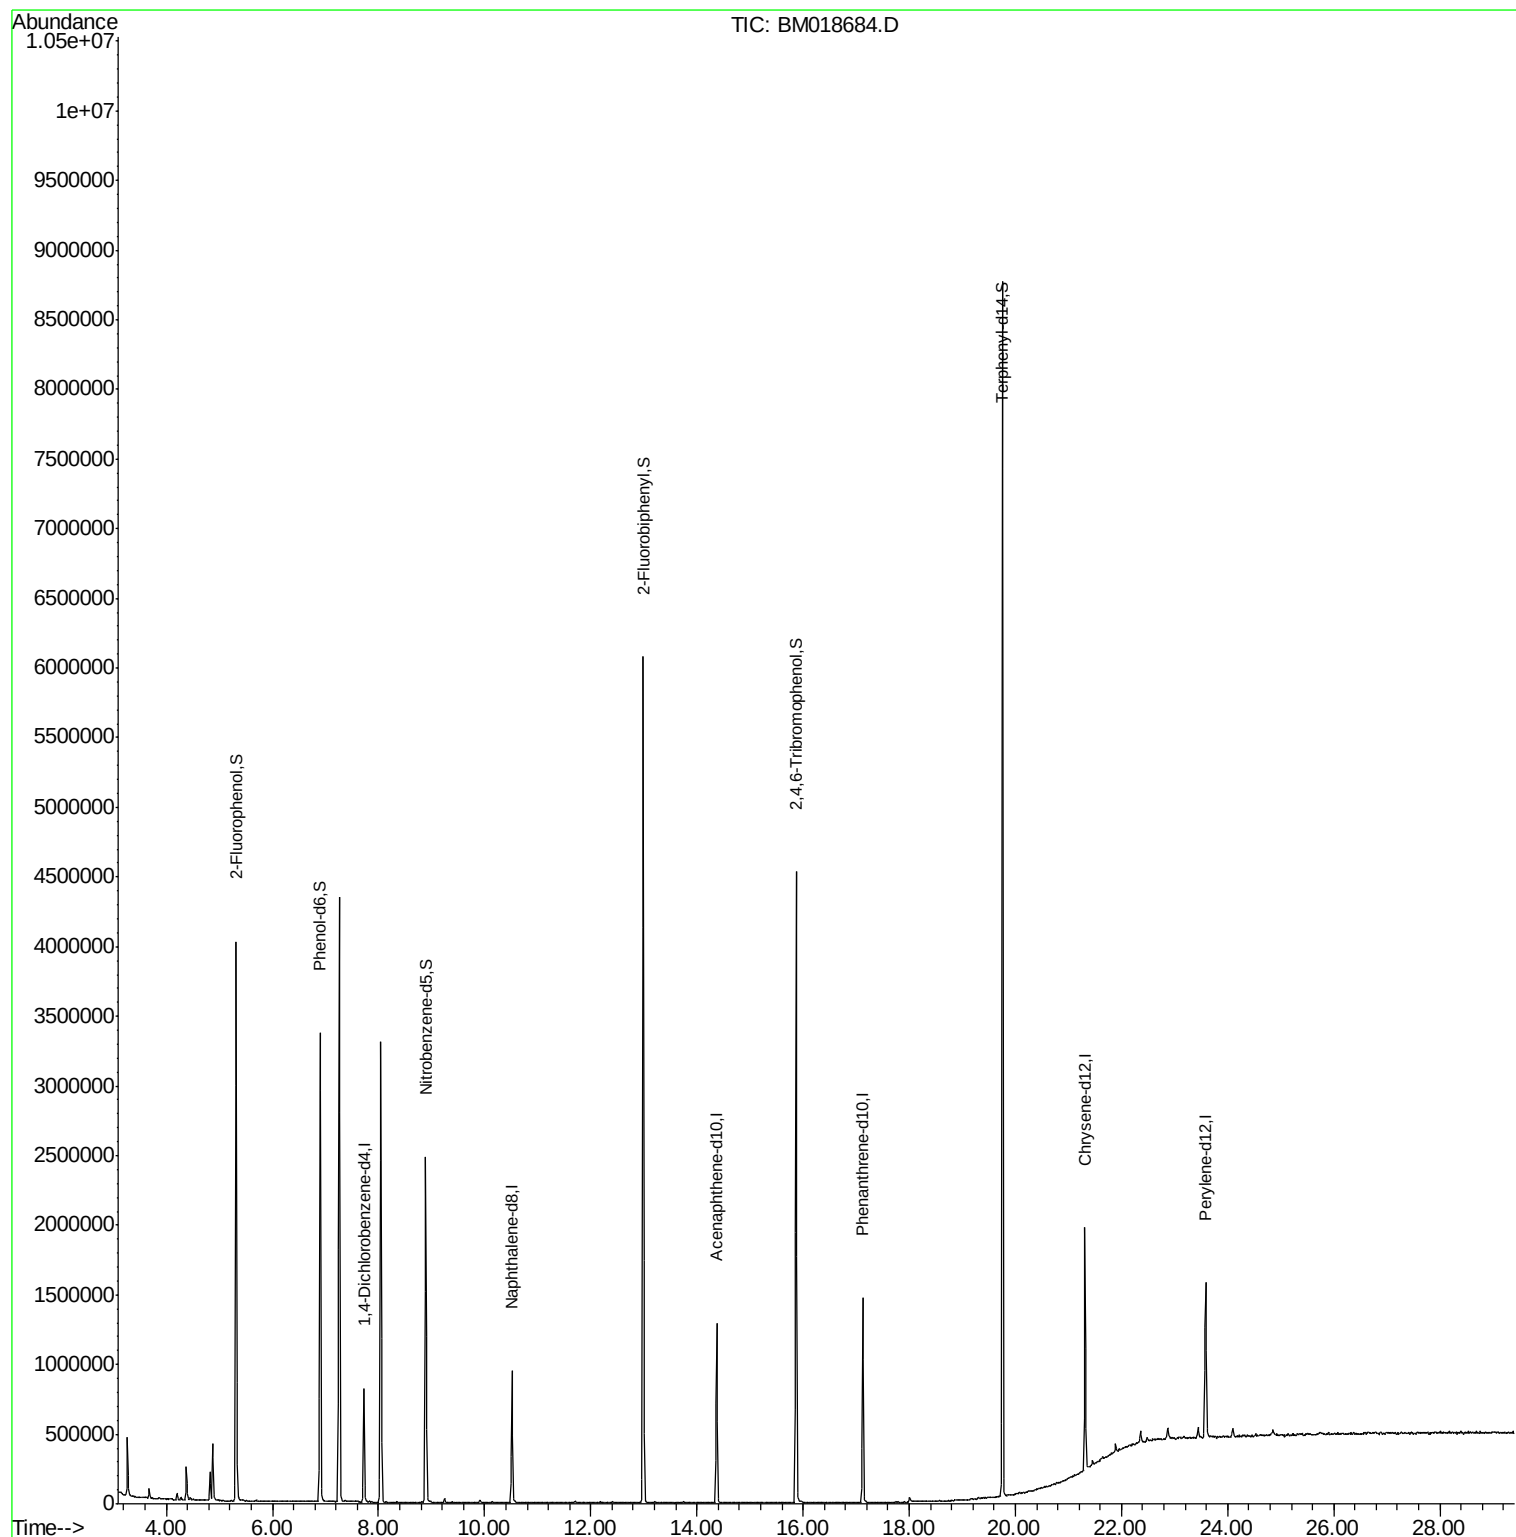

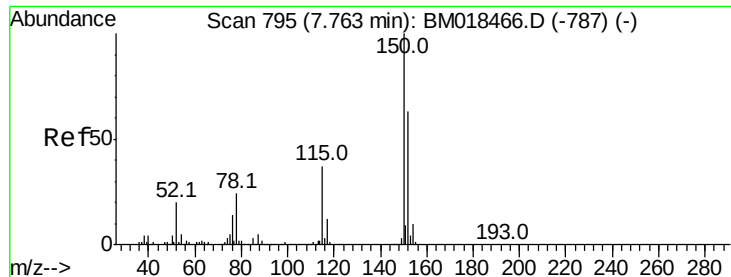


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BM018684.D
Acq: 29 Jan 2019 19:12

Instrument :
BNA_M
ClientSampleId :
HD-01-012819

Tot Ion:152 Resp: 218921
Ion Ratio Lower Upper
152 100
150 152.4 126.9 190.3
115 59.7 45.5 68.3

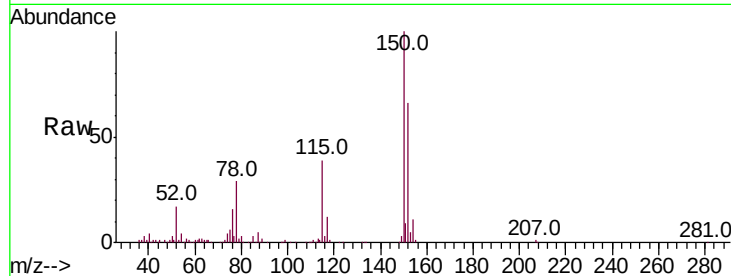


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

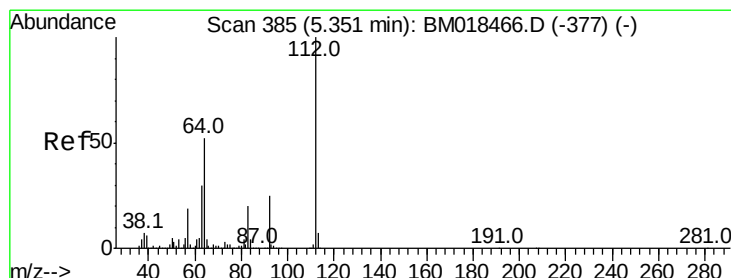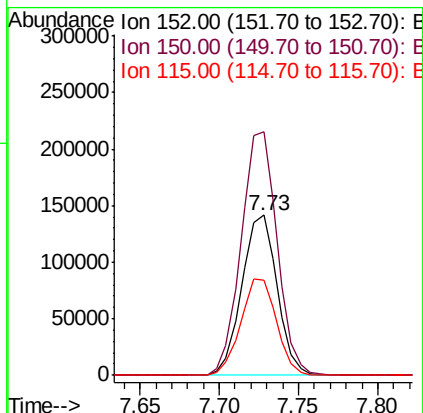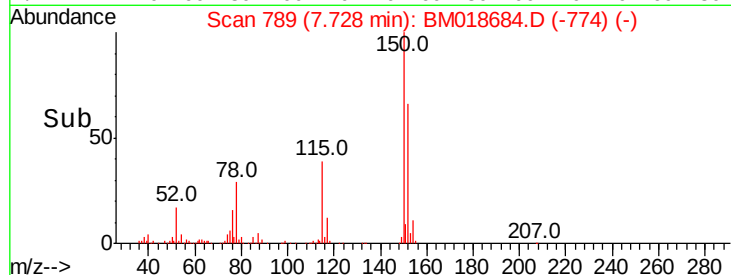



#5


2-Fluorophenol
Concen: 138.225 ng
RT: 5.32 min Scan# 379
Delta R.T. -0.01 min
Lab File: BM018684.D
Acq: 29 Jan 2019 19:12

Tgt Ion:112 Resp: 1638804
Ion Ratio Lower Upper
112 100
64 57.5 46.5 69.7
63 30.6 25.2 37.8

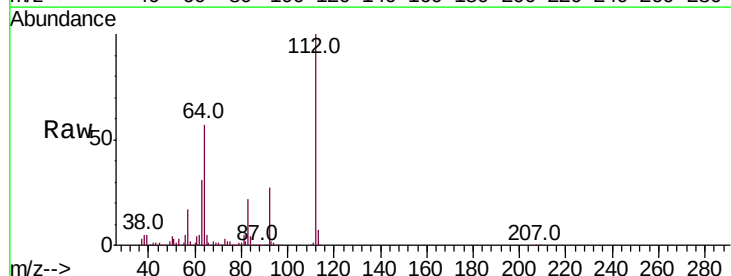

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

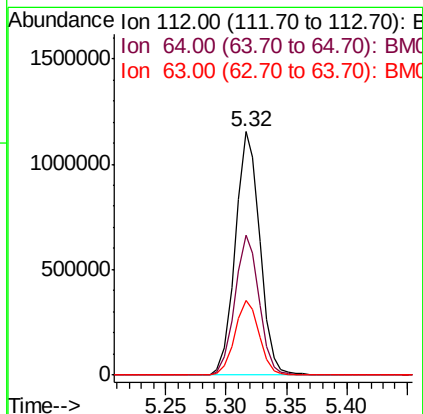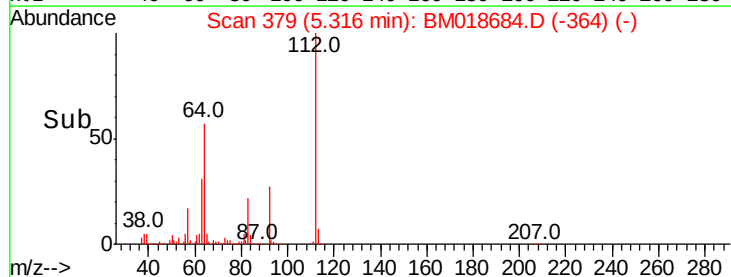

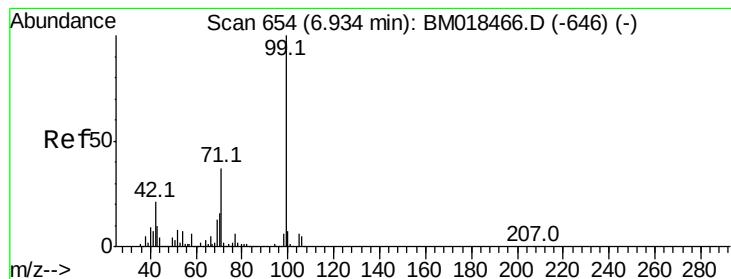

#7

Phenol-d6

Concen: 125.087 ng

RT: 6.90 min Scan# 648

Delta R.T. -0.01 min

Lab File: BM018684.D

Acq: 29 Jan 2019 19:12

Instrument :


BNA_M

ClientSampleId :




HD-01-012819

Tot Ion: 99 Resp: 1883634

Ion	Ratio	Lower	Upper
99	100		
42	14.6	17.3	25.9#
71	40.0	28.0	42.0

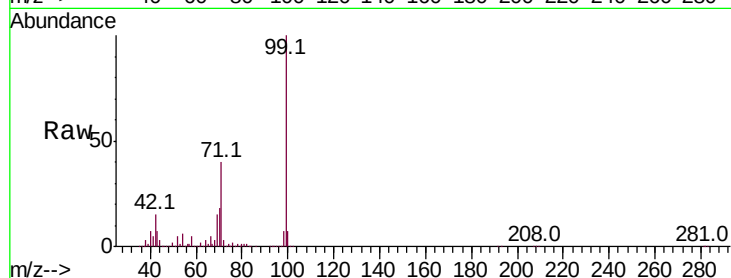

Abundance Ion 99.00 (98.70 to 99.70): BM018466.D (-646) (-)

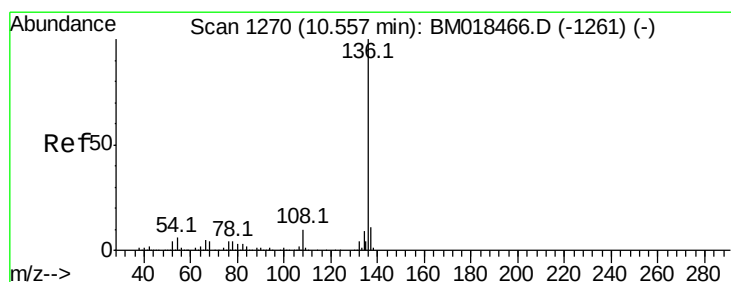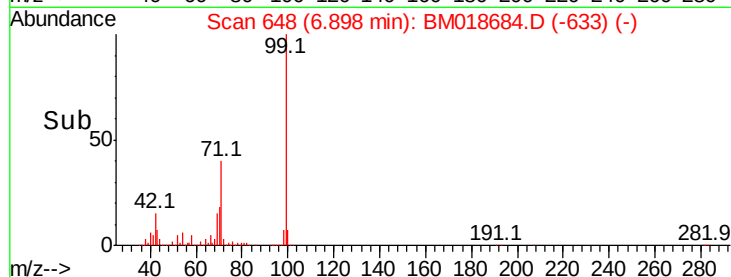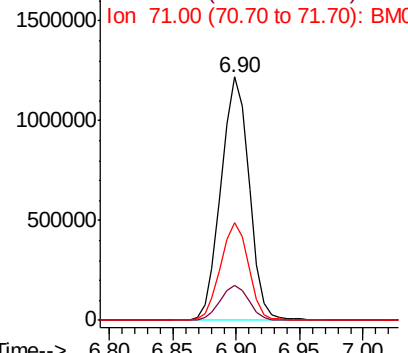

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.52 min Scan# 1263


Delta R.T. -0.01 min

Lab File: BM018684.D



Acq: 29 Jan 2019 19:12


Tgt Ion: 136 Resp: 803339

Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.5	12.7
54	5.6	6.0	9.0#
68	5.2	4.5	6.7

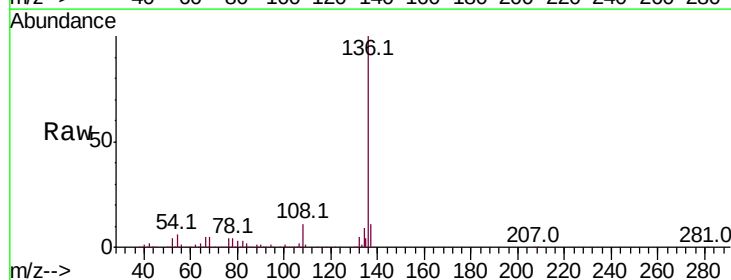

Abundance Ion 136.00 (135.70 to 136.70): BM018466.D (-1261) (-)



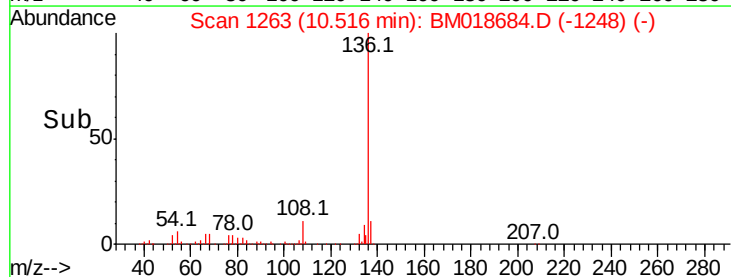
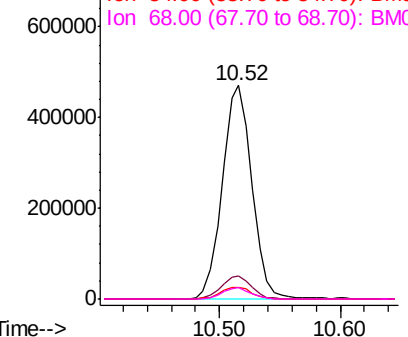


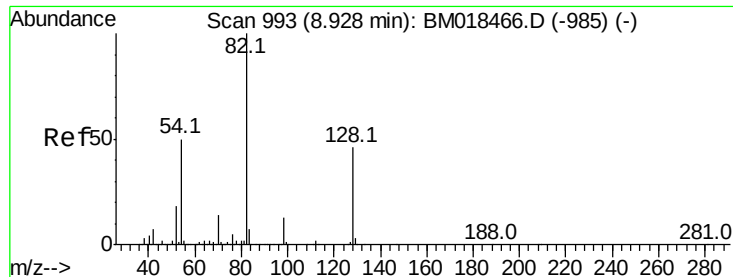

#23
Nitrobenzene-d5
Concen: 107.567 ng
RT: 8.89 min Scan# 987
Delta R.T. -0.01 min
Lab File: BM018684.D
Acq: 29 Jan 2019 19:12




Instrument :
BNA_M
ClientSampleId :
HD-01-012819


Tot Ion: 82 Resp: 1490621
Ion Ratio Lower Upper
82 100
128 40.2 36.3 54.5
54 39.2 41.7 62.5#

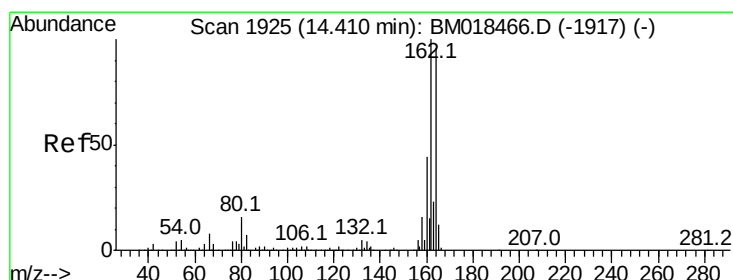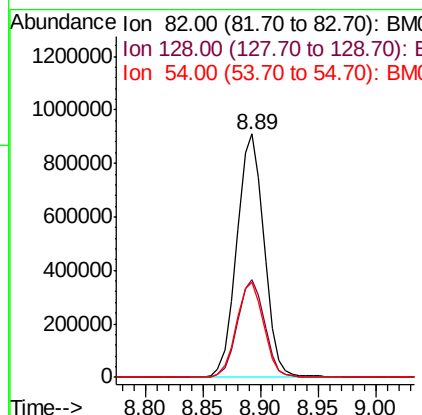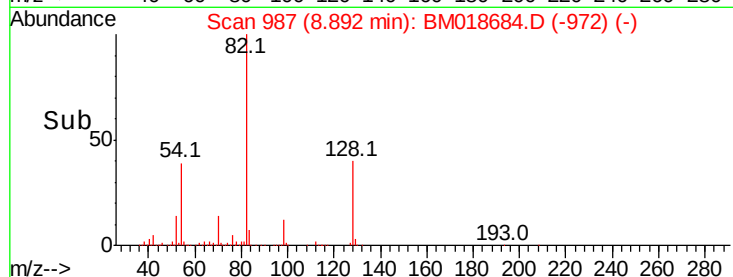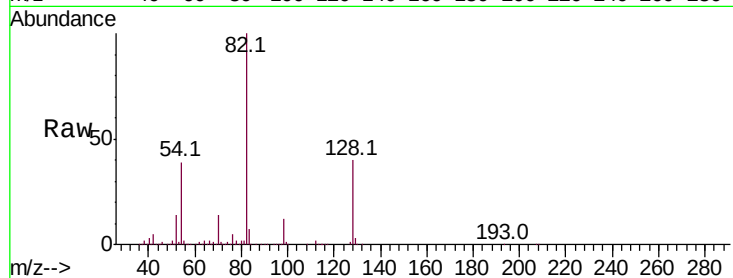

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.37 min Scan# 1919
Delta R.T. -0.01 min
Lab File: BM018684.D
Acq: 29 Jan 2019 19:12

Tgt Ion:164 Resp: 413938
Ion Ratio Lower Upper
164 100
162 104.7 83.0 124.4
160 45.7 37.1 55.7

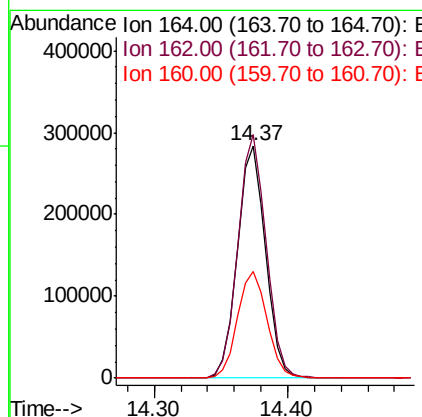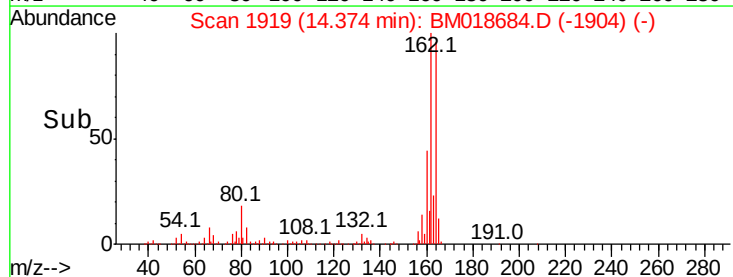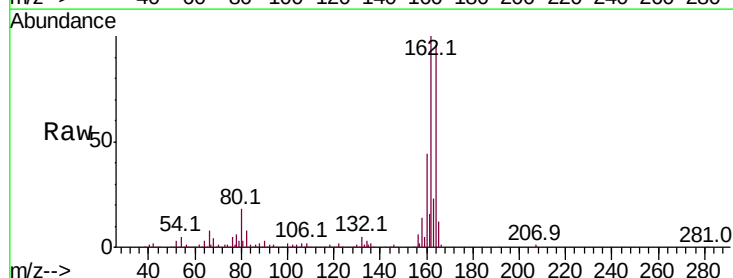


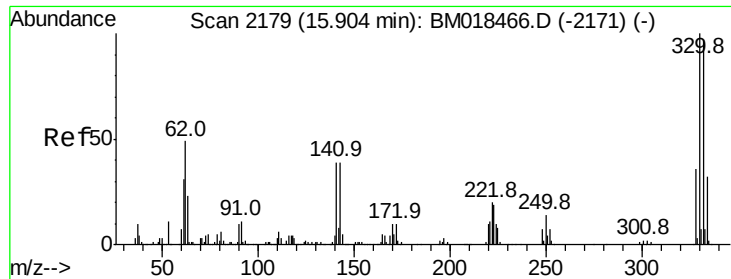




#42
 2,4,6-Tribromophenol
 Concen: 138.251 ng
 RT: 15.87 min Scan# 2173
 Delta R.T. -0.02 min
 Lab File: BM018684.D
 Acq: 29 Jan 2019 19:12

Instrument :
 BNA_M
 ClientSampleId :
 HD-01-012819

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	77.6	116.4
141	39.4	31.7	47.5

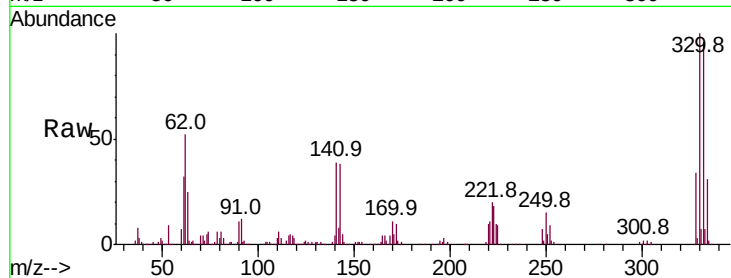


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

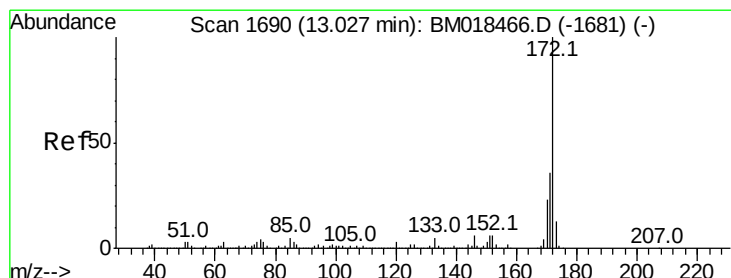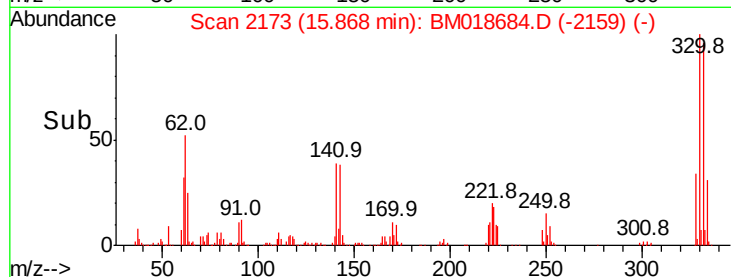
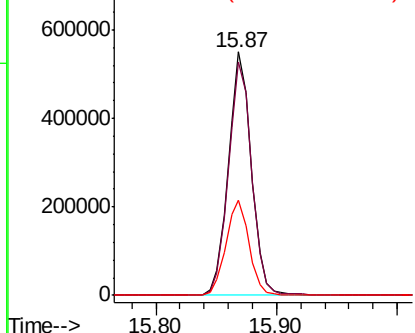



#45
 2-Fluorobiphenyl
 Concen: 97.881 ng
 RT: 12.99 min Scan# 1684
 Delta R.T. -0.01 min
 Lab File: BM018684.D
 Acq: 29 Jan 2019 19:12

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.2	42.4
170	23.0	18.9	28.3

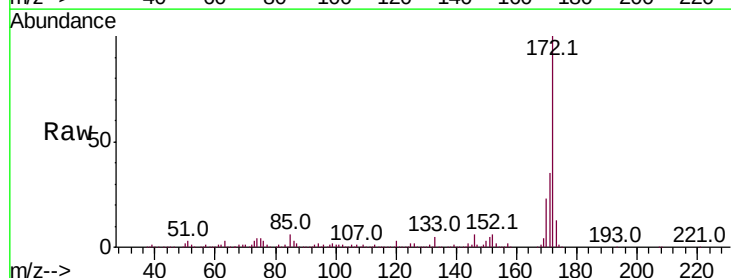

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



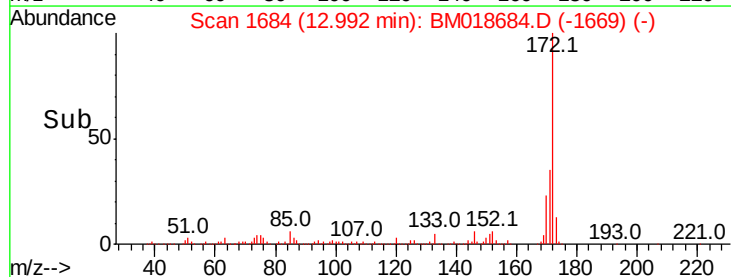
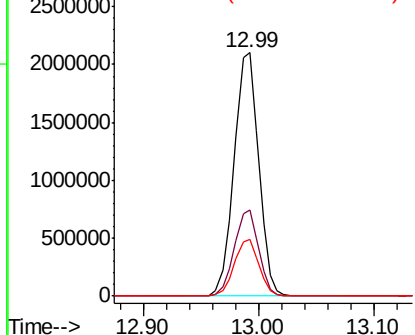


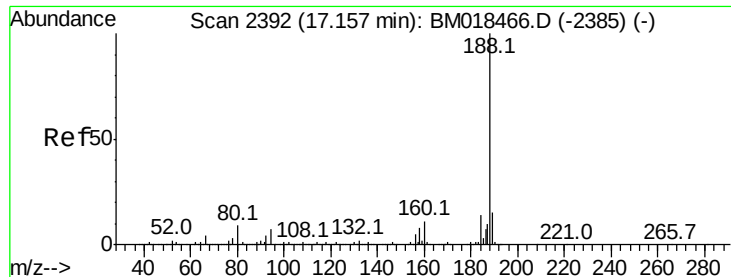

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.13 min Scan# 2387
Delta R.T. -0.01 min
Lab File: BM018684.D
Acq: 29 Jan 2019 19:12




Instrument :
BNA_M
ClientSampleId :
HD-01-012819


Tot Ion:188 Resp: 853322
Ion Ratio Lower Upper
188 100
94 7.7 7.1 10.7
80 8.6 7.6 11.4

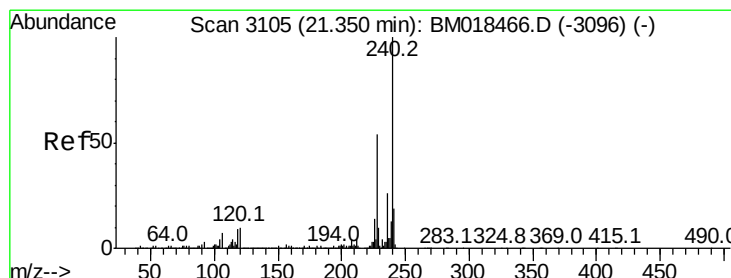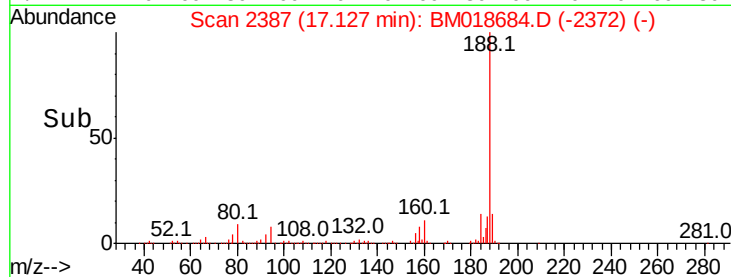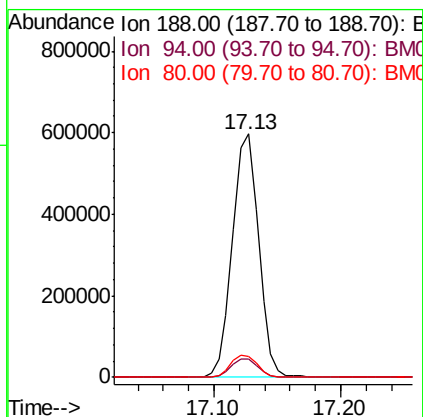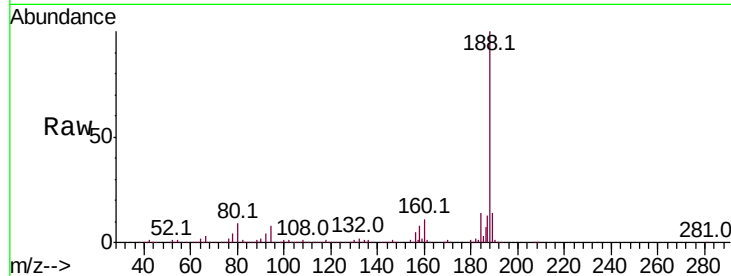

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.32 min Scan# 3099
Delta R.T. -0.02 min
Lab File: BM018684.D
Acq: 29 Jan 2019 19:12

Tgt Ion:240 Resp: 778350
Ion Ratio Lower Upper
240 100
120 10.0 8.4 12.6
236 25.3 20.7 31.1

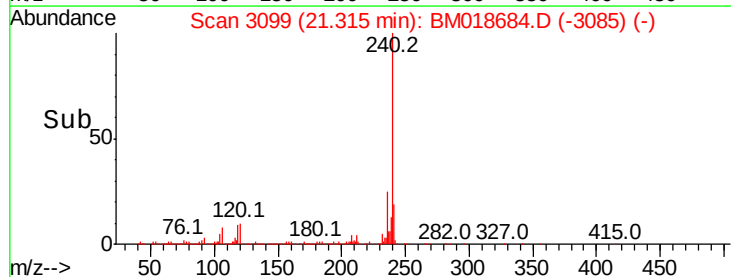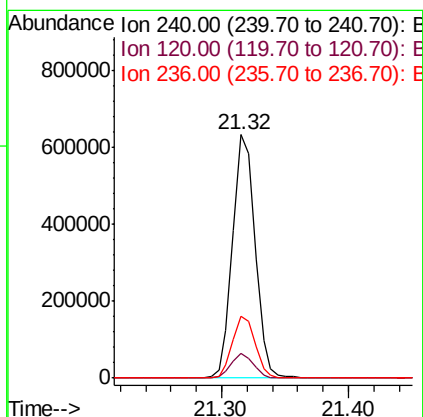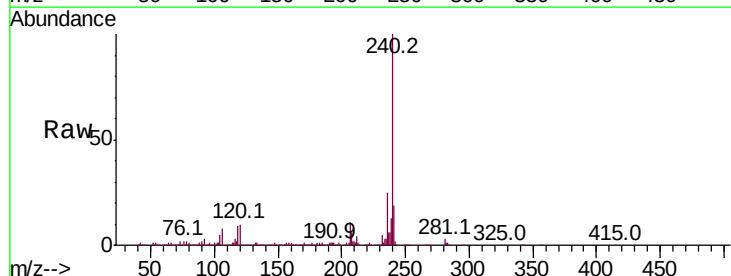

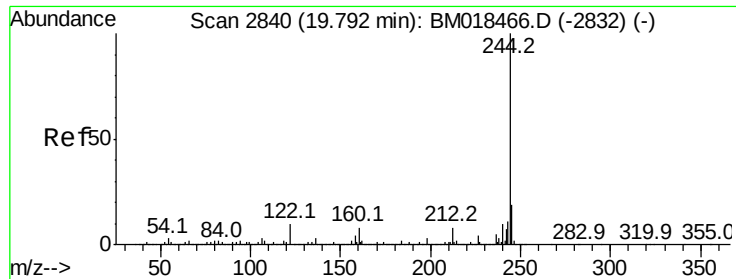

#79

Terphenyl-d14

Concen: 101.495 ng

RT: 19.76 min Scan# 2834

Delta R.T. -0.01 min

Lab File: BM018684.D

Acq: 29 Jan 2019 19:12

Instrument :

BNA_M

ClientSampleId :

HD-01-012819


Tot Ion:244 Resp: 3747514

Ion Ratio Lower Upper




244 100

212 7.8 5.9 8.9

122 10.1 9.0 13.4

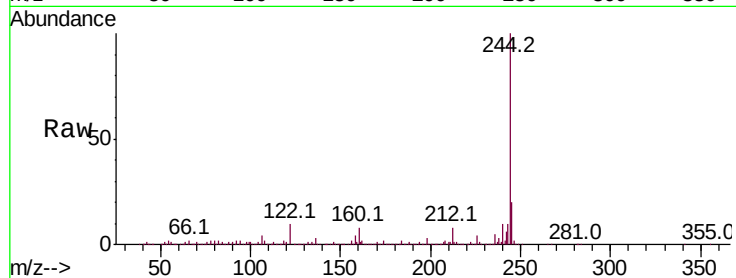

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

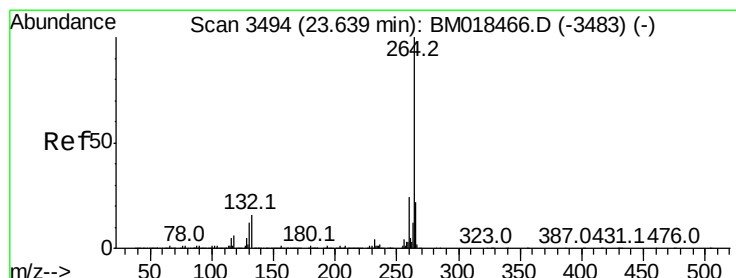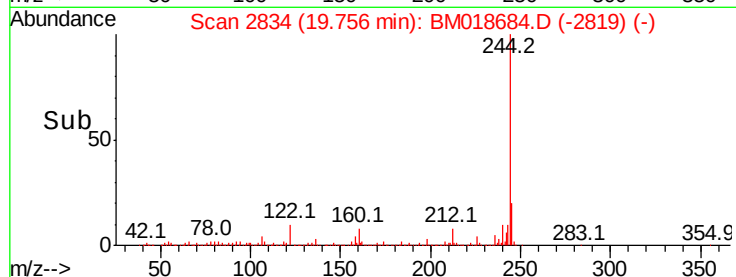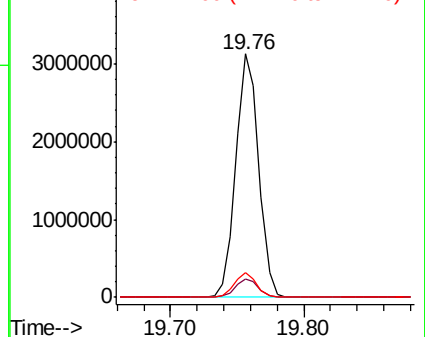

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.59 min Scan# 3485

Delta R.T. -0.02 min

Lab File: BM018684.D

Acq: 29 Jan 2019 19:12


Tgt Ion:264 Resp: 777032

Ion Ratio Lower Upper

264 100

260 23.7 18.9 28.3

265 22.4 16.8 25.2

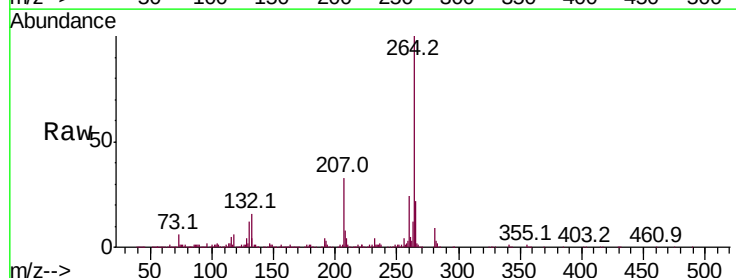

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

