


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM012919\
 Data File : BM018676.D
 Acq On : 29 Jan 2019 14:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 22:01:30 2019

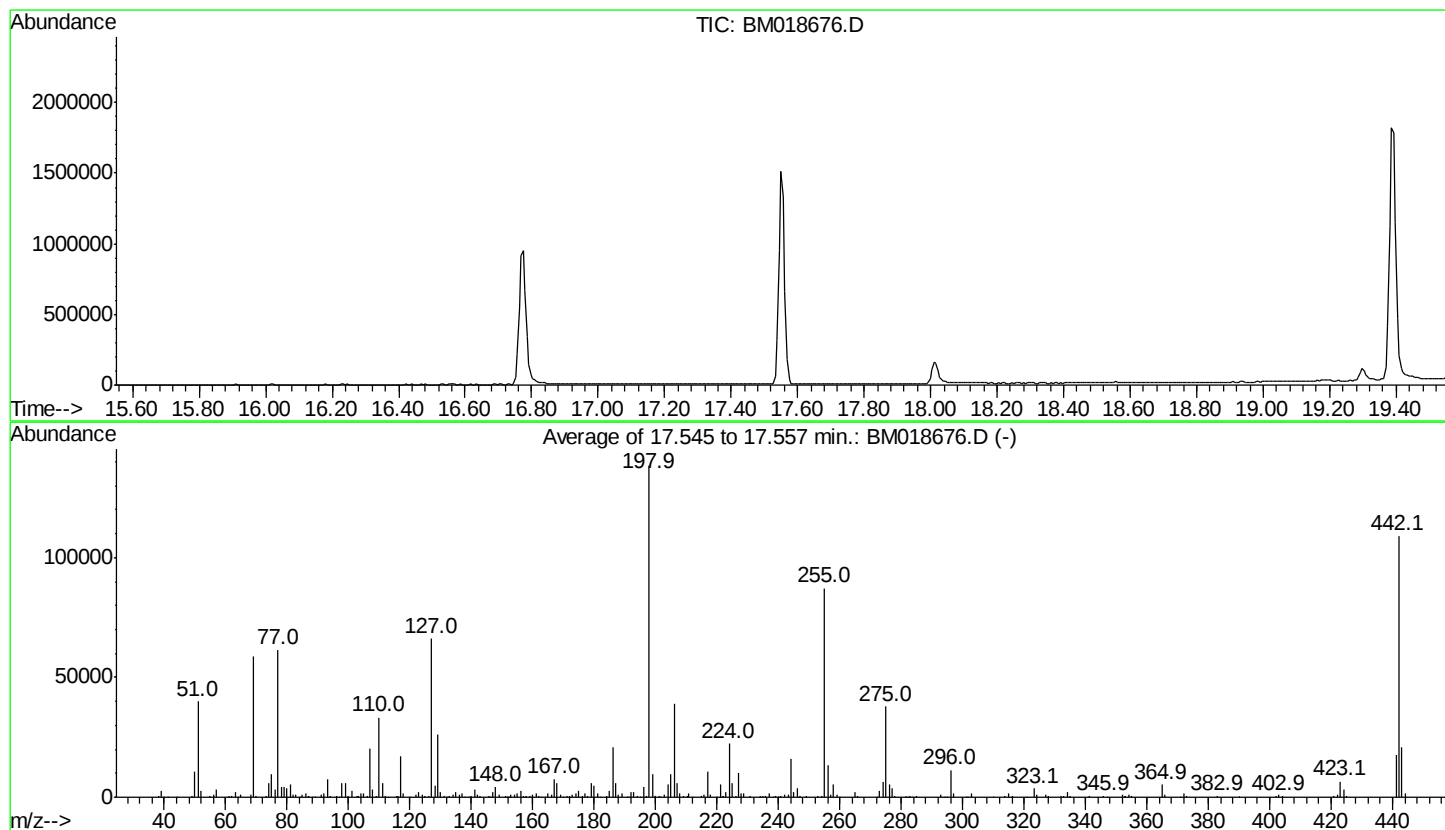

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	39917	PASS
68	69	0.00	2	2.0	1161	PASS
69	198	0.00	100	42.4	58621	PASS
70	69	0.00	2	0.6	379	PASS
127	198	10	80	47.7	66082	PASS
197	198	0.00	2	0.5	705	PASS
198	198	100	100	100.0	138400	PASS
199	198	5	9	6.8	9472	PASS
275	198	10	60	27.4	37869	PASS
365	198	1	100	3.8	5325	PASS
441	198	0.01	100	12.6	17469	PASS
442	198	50	100	78.8	109008	PASS
443	442	15	24	19.2	20969	PASS