
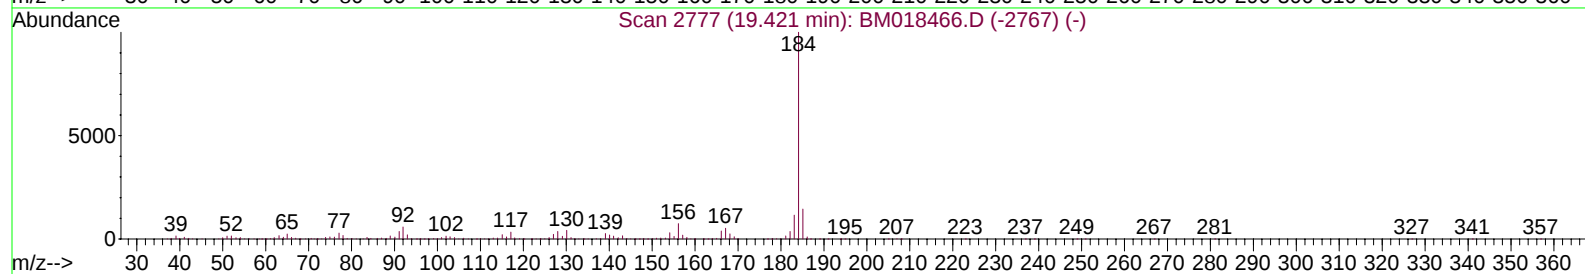
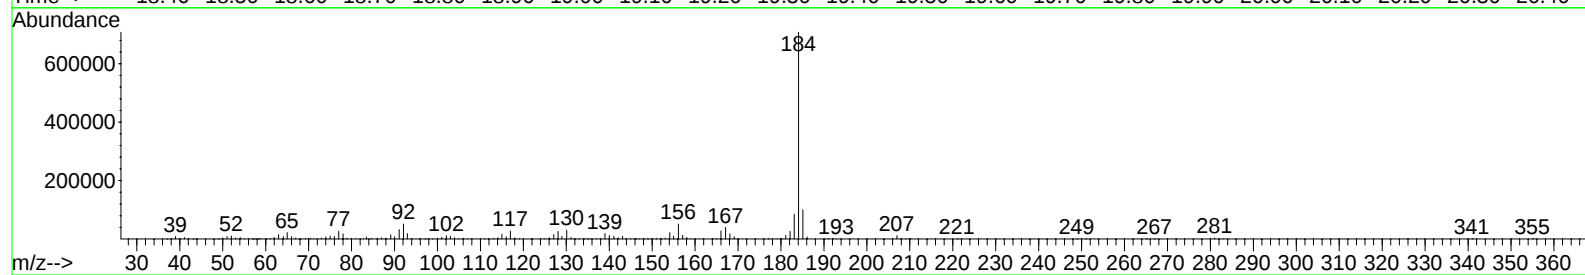


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM013019\
 Data File : BM018690.D
 Acq On : 30 Jan 2019 09:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 13:44:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 22:01:30 2019
 Response via : Initial Calibration

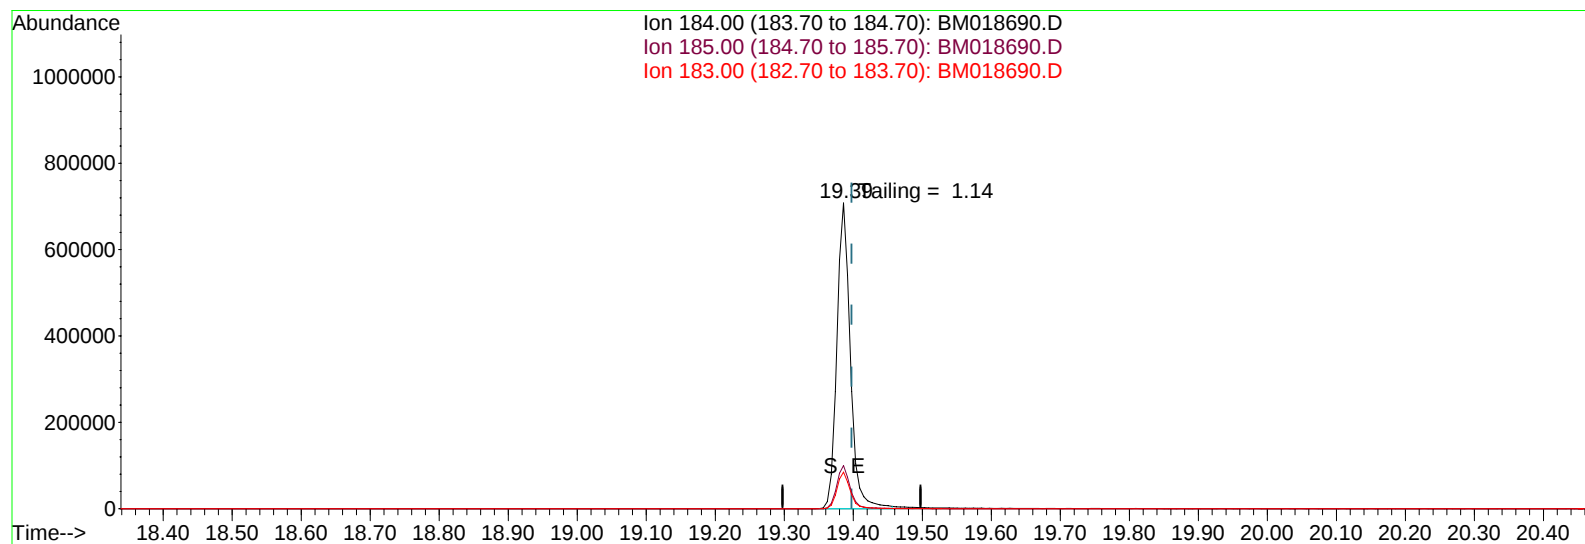

TIC: BM018690.D

(77) Benzidine




19.386min (-0.012) 12148.61ng

response 961694

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.12
183.00	11.90	12.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM013019\
Data File : BM018690.D
Acq On : 30 Jan 2019 09:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 13:44:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

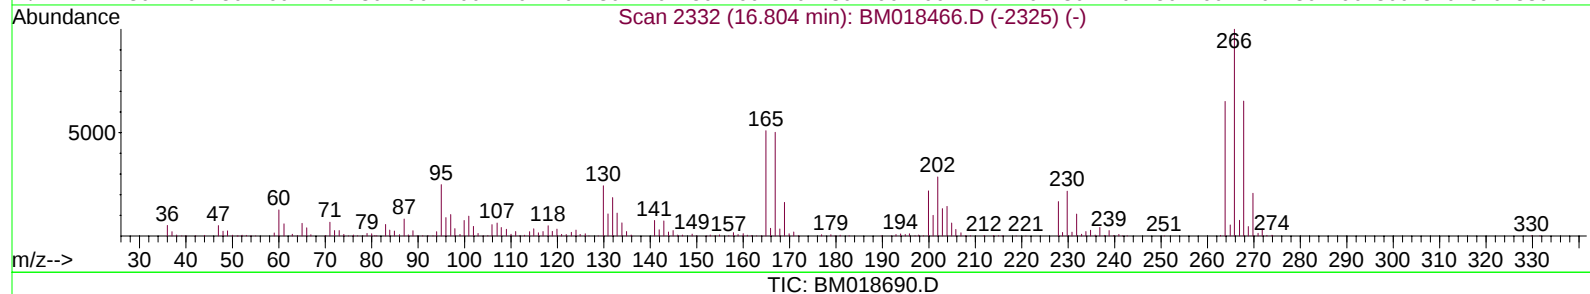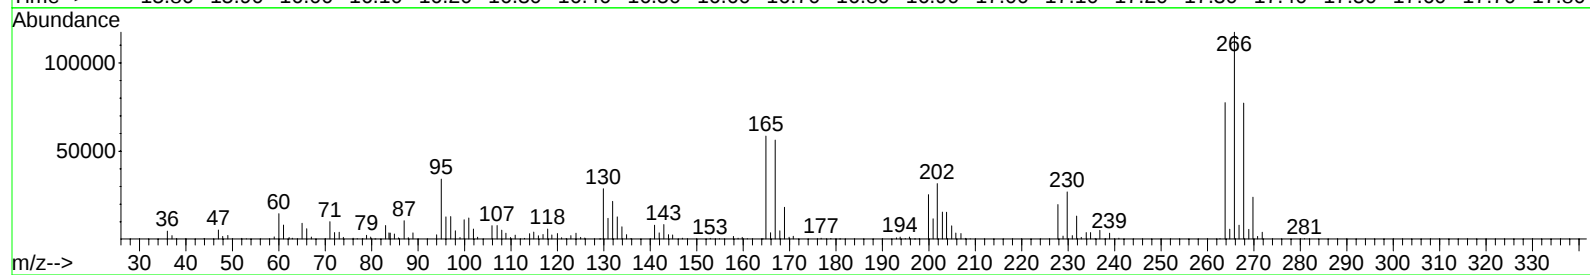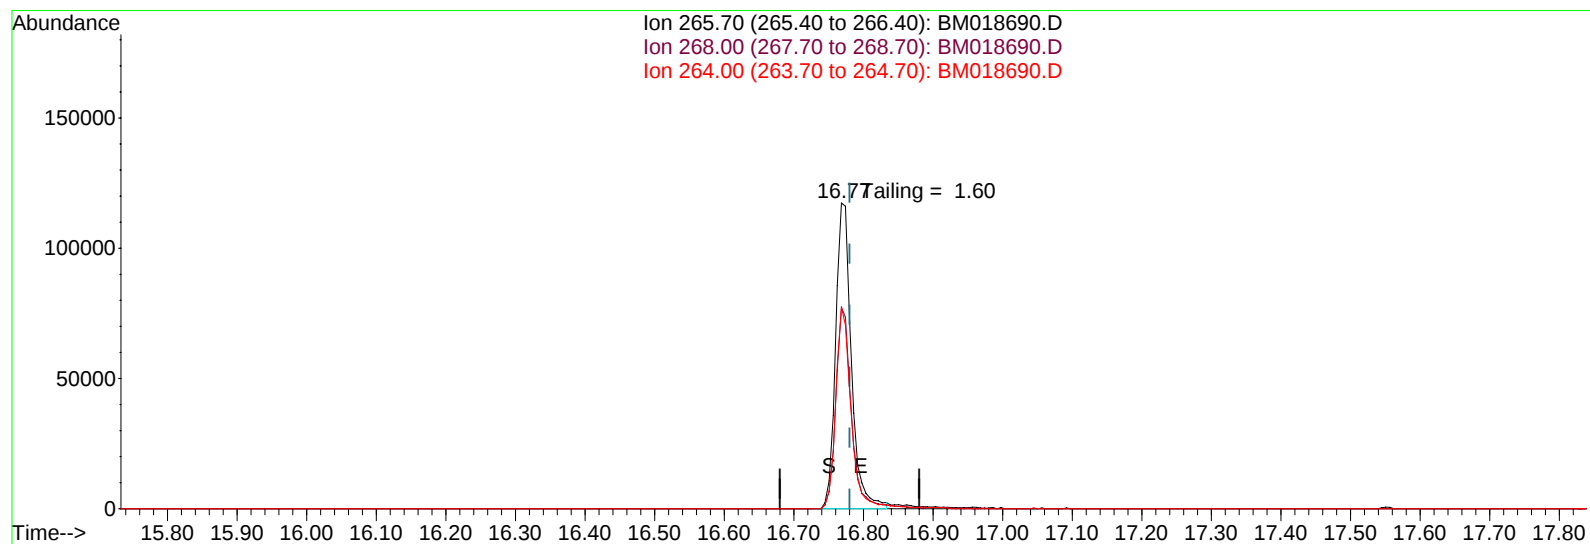

(70) Pentachlorophenol (C)

16.768min (-0.012) 41497.29ng

response 185557

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	65.84
264.00	62.60	66.06
0.00	0.00	0.00