


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM013019\
 Data File : BM018690.D
 Acq On : 30 Jan 2019 09:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 22:01:30 2019

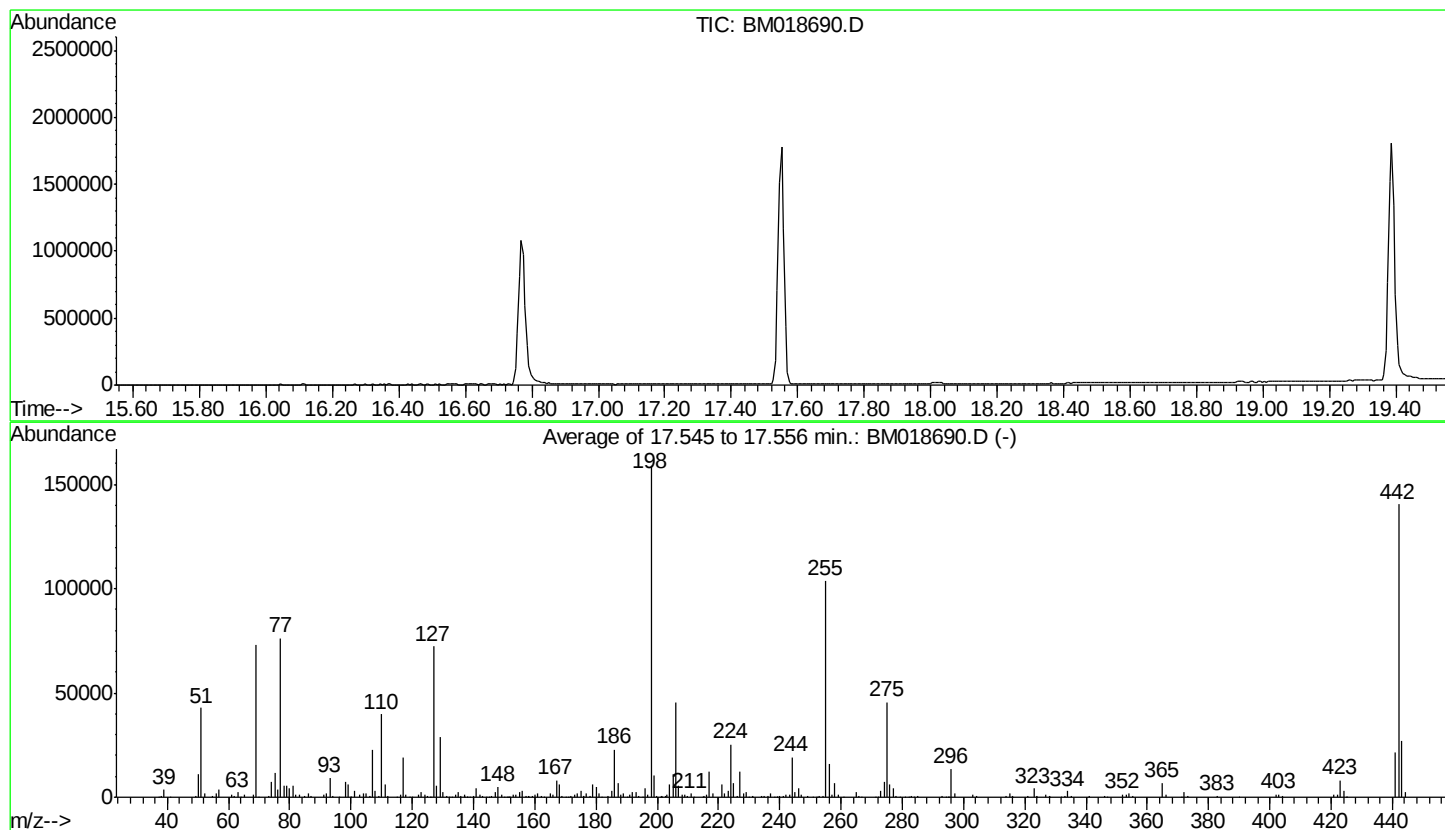

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	42869	PASS
68	69	0.00	2	2.0	1481	PASS
69	198	0.00	100	46.0	73202	PASS
70	69	0.00	2	0.4	314	PASS
127	198	10	80	45.5	72392	PASS
197	198	0.00	2	0.6	1021	PASS
198	198	100	100	100.0	159026	PASS
199	198	5	9	6.6	10555	PASS
275	198	10	60	28.6	45461	PASS
365	198	1	100	4.3	6911	PASS
441	198	0.01	100	13.7	21781	PASS
442	198	50	100	88.3	140418	PASS
443	442	15	24	19.4	27226	PASS