

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013023\
 Data File : BM038609.D
 Acq On : 30 Jan 2023 16:46
 Operator : CG/JU
 Sample : SSTD08025
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD080030

Quant Time: Jan 31 00:22:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 00:17:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	32415	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	105732	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	86749	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.333	188	213503	20.000	ng/u1	0.00
79) Chrysene-d12	21.509	240	261979	20.000	ng/u1	0.00
88) Perylene-d12	23.921	264	327550	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	29172	32.233	ng/uL	0.00
4) Pyridine-d5	3.763	84	192018	84.348	ng/u1	0.00
7) Phenol-d5	7.128	99	169332	78.259	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.292	67	97505	77.204	ng/u1	0.00
11) 2-Chlorophenol-d4	7.486	132	149028	83.053	ng/u1	0.00
15) 4-Methylphenol-d8	8.680	113	136378	78.995	ng/u1	0.00
21) Nitrobenzene-d5	9.133	128	67741	84.523	ng/u1	0.00
24) 2-Nitrophenol-d4	9.857	143	95736	90.453	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	222103	94.818	ng/u1	0.00
31) 4-Chloroaniline-d4	10.916	131	187921	82.553	ng/u1	0.00
46) Dimethylphthalate-d6	14.010	166	610474	85.191	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	683143	89.584	ng/u1	0.00
54) 4-Nitrophenol-d4	14.815	143	82519	83.242	ng/u1	0.02
60) Fluorene-d10	15.586	176	589879	92.048	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.715	200	153677	84.087	ng/u1	0.00
73) Anthracene-d10	17.439	188	996233	92.784	ng/u1	0.00
81) Pyrene-d10	19.727	212	1185069	87.789	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.768	264	1530594	91.038	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.369	88	28835	29.437	ng/uL	97
5) Pyridine	3.781	79	189045	80.863	ng/u1	95
6) Benzaldehyde	7.098	77	71756	71.925	ng/u1	94
8) Phenol	7.157	94	170117	78.528	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.386	93	121330	78.388	ng/u1	89
12) 2-Chlorophenol	7.522	128	147638	81.995	ng/u1	97
13) 2-Methylphenol	8.410	108	129469	78.659	ng/u1	90
14) 2,2'-oxybis(1-Chloropr...	8.492	45	121070	75.709	ng/u1	99
16) Acetophenone	8.792	105	240064	78.710	ng/u1	93
17) N-Nitroso-di-n-propyla...	8.786	70	121576	86.736	ng/u1	96
18) 4-Methylphenol	8.745	108	137754	78.848	ng/u1	94
19) Hexachloroethane	9.033	117	75112	82.704	ng/u1	85
22) Nitrobenzene	9.180	77	194301	80.550	ng/u1	99
23) Isophorone	9.710	82	309723	84.854	ng/u1	95
25) 2-Nitrophenol	9.886	139	92316	87.995	ng/u1	97
26) 2,4-Dimethylphenol	9.945	107	193179	84.775	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.180	93	155778	83.699	ng/u1	97
29) 2,4-Dichlorophenol	10.422	162	208200	93.518	ng/u1	96
30) Naphthalene	10.822	128	443764	84.591	ng/u1	98
32) 4-Chloroaniline	10.939	127	190896	83.572	ng/u1	99
33) Hexachlorobutadiene	11.092	225	187637	81.099	ng/u1	98
34) Caprolactam	11.751	113	22440	51.295	ng/u1	88
35) 4-Chloro-3-methylphenol	12.063	107	159436	90.659	ng/u1#	85
36) 2-Methylnaphthalene	12.421	142	366702	93.980	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013023\
 Data File : BM038609.D
 Acq On : 30 Jan 2023 16:46
 Operator : CG/JU
 Sample : SSTD08025
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD080030

Quant Time: Jan 31 00:22:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 00:17:30 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.645	142	376894	93.572	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.792	216	329653	77.198	ng/ul	98
40) Hexachlorocyclopentadiene	12.757	237	242929	79.722	ng/ul	98
41) 2,4,6-Trichlorophenol	13.033	196	217894	83.809	ng/ul	95
42) 2,4,5-Trichlorophenol	13.104	196	231876	83.514	ng/ul	95
43) 1,1'-Biphenyl	13.433	154	574655	86.151	ng/ul	99
44) 2-Chloronaphthalene	13.474	162	479908	86.606	ng/ul#	92
45) 2-Nitroaniline	13.692	65	124507	84.005	ng/ul	93
47) Dimethylphthalate	14.057	163	601136	85.254	ng/ul	100
48) 2,6-Dinitrotoluene	14.186	165	120600	92.349	ng/ul	86
50) Acenaphthylene	14.321	152	667609	87.547	ng/ul	97
51) 3-Nitroaniline	14.515	138	78537	83.550	ng/ul	100
52) Acenaphthene	14.657	153	489745	86.282	ng/ul	97
53) 2,4-Dinitrophenol	14.721	184	96144	91.582	ng/ul	92
55) 4-Nitrophenol	14.827	109	136679	82.183	ng/ul	91
56) Dibenzofuran	14.992	168	760484	90.082	ng/ul	87
57) 2,4-Dinitrotoluene	14.974	165	181412	94.249	ng/ul#	87
58) 2,3,4,6-Tetrachlorophenol	15.215	232	200244	82.373	ng/ul#	95
59) Diethylphthalate	15.409	149	562810	85.141	ng/ul	96
61) Fluorene	15.639	166	705996	99.299	ng/ul	95
62) 4-Chlorophenyl-phenyle...	15.633	204	440406	88.033	ng/ul	90
63) 4-Nitroaniline	15.680	138	59778	78.927	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.733	198	145491	84.355	ng/ul#	92
67) N-Nitrosodiphenylamine	15.851	169	541824	90.012	ng/ul	95
68) 4-Bromophenyl-phenylether	16.521	248	246414	81.911	ng/ul	97
69) Hexachlorobenzene	16.639	284	299050	85.157	ng/ul#	91
70) Atrazine	16.803	200	243834	80.732	ng/ul	98
71) Pentachlorophenol	16.986	266	183168	81.539	ng/ul	92
72) Phenanthrene	17.380	178	1046247	93.770	ng/ul	98
74) Anthracene	17.474	178	1114420	95.381	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.398	216	314323	76.596	ng/uL	98
76) Pentachlorobenzene	14.909	250	333640	78.135	ng/uL	98
77) Carbazole	17.745	167	849201	83.734	ng/ul	96
78) Di-n-butylphthalate	18.292	149	914754	93.228	ng/ul	98
80) Fluoranthene	19.392	202	1405333	89.816	ng/ul#	98
82) Pyrene	19.756	202	1528772	92.068	ng/ul#	98
83) Butylbenzylphthalate	20.639	149	445827	93.084	ng/ul	93
84) 3,3'-Dichlorobenzidine	21.427	252	531329	82.557	ng/ul	98
85) Benzo(a)anthracene	21.497	228	1596252	86.014	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.409	149	658924	96.686	ng/ul	94
87) Chrysene	21.550	228	1521725	88.589	ng/ul	99
89) Di-n-octyl phthalate	22.333	149	1198186	86.374	ng/ul	100
90) Benzo(b)fluoranthene	23.185	252	1889031	93.282	ng/ul	100
91) Benzo(k)fluoranthene	23.185	252	1889031	93.622	ng/ul	99
93) Benzo(a)pyrene	23.821	252	1703988	90.863	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.450	276	2606154	87.918	ng/ul	99
95) Dibenzo(a,h)anthracene	26.456	278	2260051	89.832	ng/ul	99
96) Benzo(g,h,i)perylene	27.220	276	1987006	82.585	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013023\
 Data File : BM038609.D
 Acq On : 30 Jan 2023 16:46
 Operator : CG/JU
 Sample : SSTD08025
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD080030

Quant Time: Jan 31 00:22:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 00:17:30 2023
 Response via : Initial Calibration




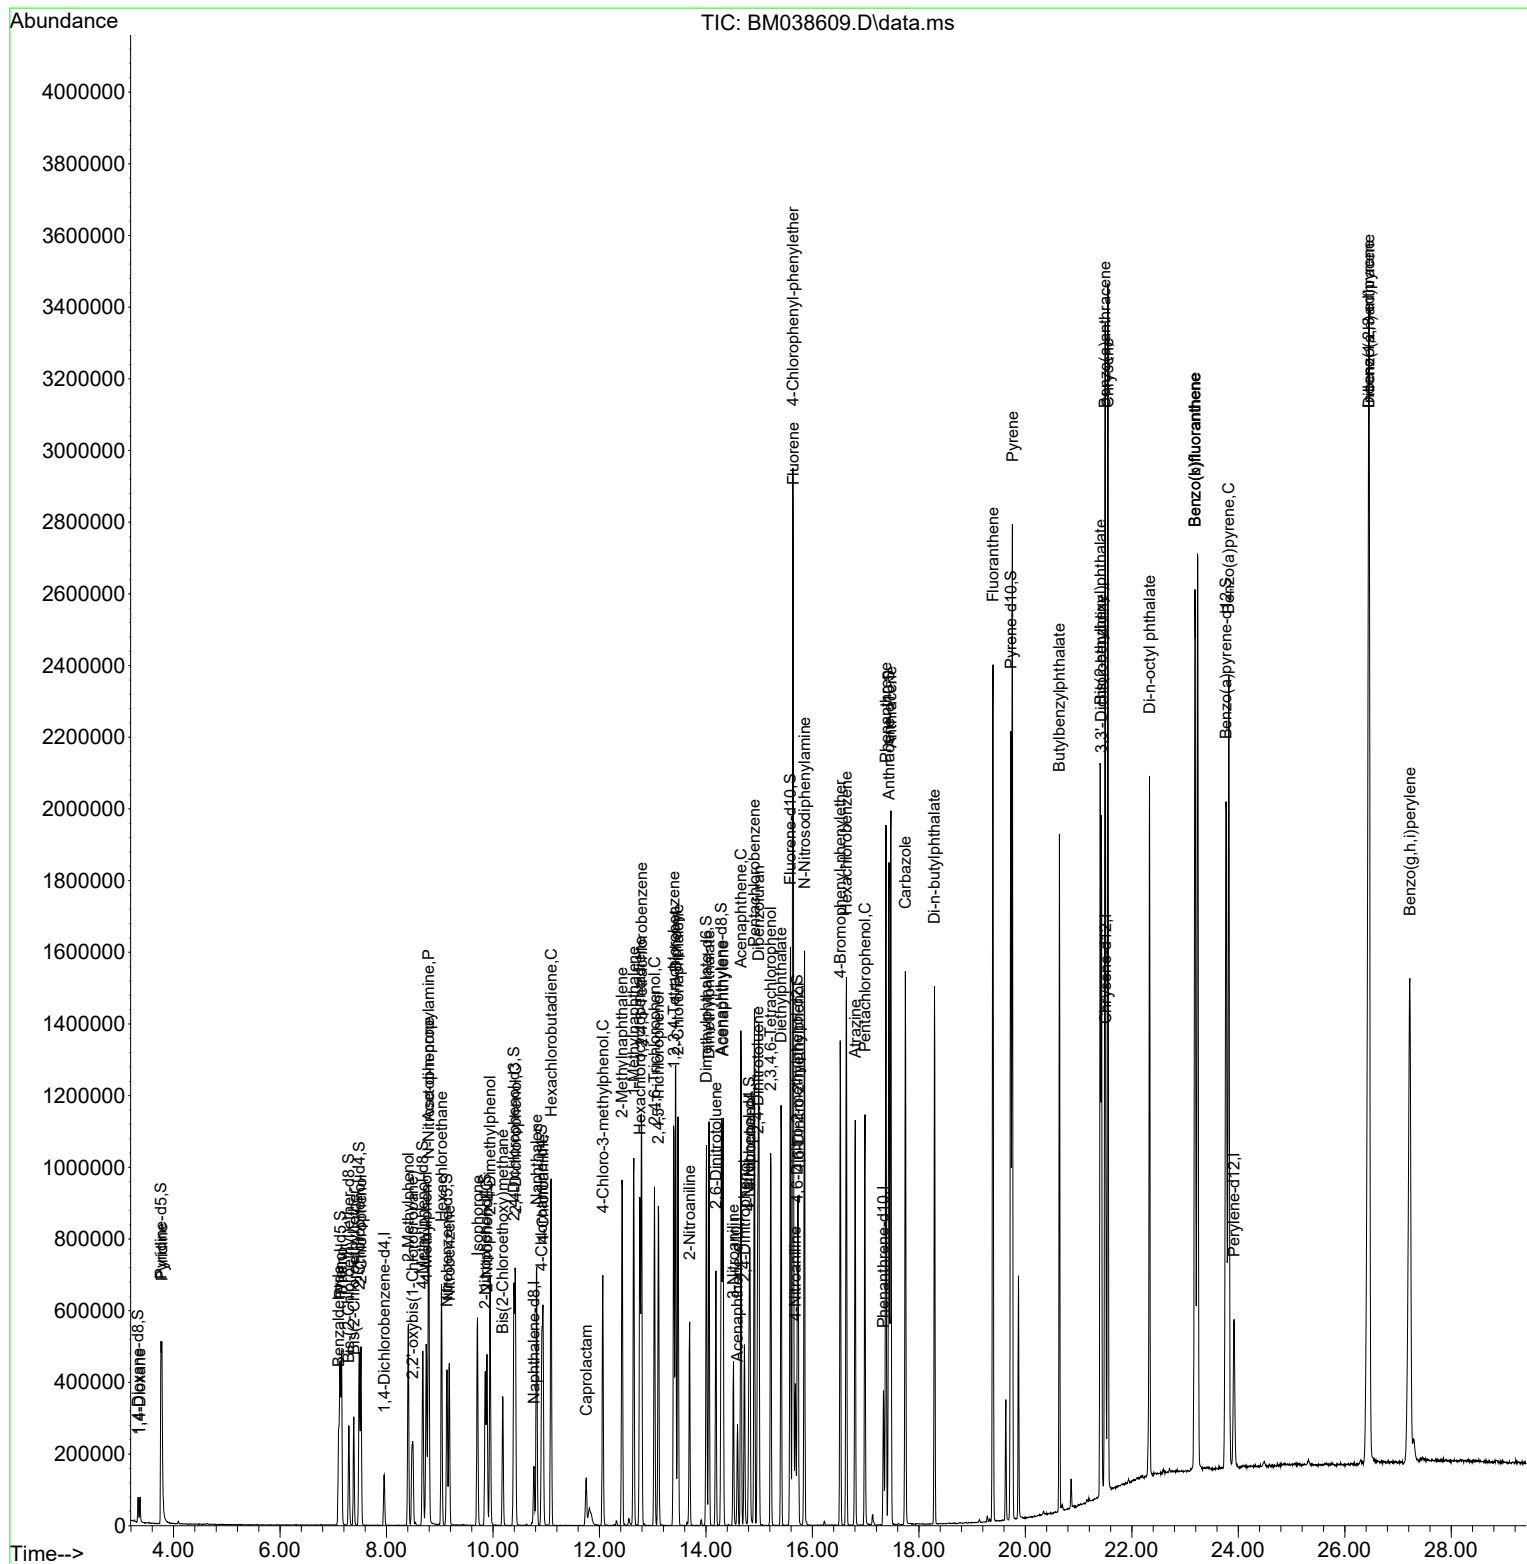




#2
1,4-Dioxane
Concen: 29.437 ng/uL
RT: 3.369 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion: 88 Resp: 28835
Ion Ratio Lower Upper
88 100
43 43.0 33.8 50.8
58 67.8 52.1 78.1



#5
Pyridine
Concen: 80.863 ng/uL
RT: 3.781 min Scan# 101
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 79 Resp: 189045
Ion Ratio Lower Upper
79 100
52 77.6 67.4 101.0
51 51.6 40.7 61.1









#6
Benzaldehyde
Concen: 71.925 ng/ul
RT: 7.098 min Scan# 609
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion: 77 Resp: 71756
Ion Ratio Lower Upper
77 100
105 85.9 68.3 102.5
106 83.4 57.7 86.5

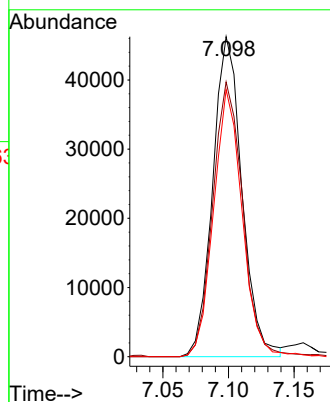

#8
Phenol
Concen: 78.528 ng/ul
RT: 7.157 min Scan# 675
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 94 Resp: 170117
Ion Ratio Lower Upper
94 100
65 43.6 38.2 57.2
66 68.9 57.9 86.9









#10
Bis(2-Chloroethyl)ether
Concen: 78.388 ng/ul
RT: 7.386 min Scan# 714
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion: 93 Resp: 121330
Ion Ratio Lower Upper
93 100
63 79.6 73.9 110.9
95 33.3 28.0 42.0



#12
2-Chlorophenol
Concen: 81.995 ng/ul
RT: 7.522 min Scan# 737
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 128 Resp: 147638
Ion Ratio Lower Upper
128 100
64 47.9 40.0 60.0
130 32.6 24.4 36.6




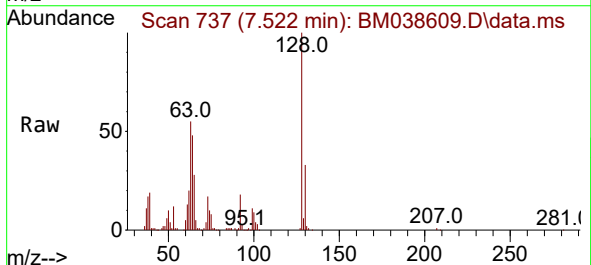




#13
2-Methylphenol
Concen: 78.659 ng/ul
RT: 8.410 min Scan# 887
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:108 Resp: 129469
Ion Ratio Lower Upper
108 100
107 92.3 66.6 100.0



#14
2,2'-oxybis(1-Chloropropane)
Concen: 75.709 ng/ul
RT: 8.492 min Scan# 902
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 45 Resp: 121070
Ion Ratio Lower Upper
45 100
77 21.7 16.9 25.3
79 15.4 11.8 17.6




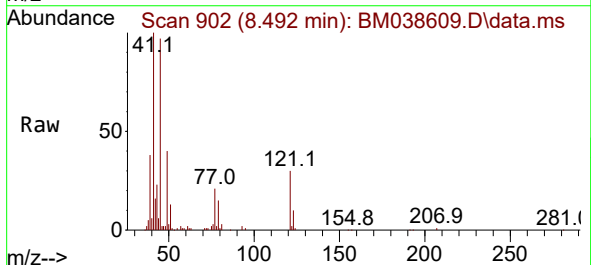




#16
Acetophenone
Concen: 78.710 ng/ul
RT: 8.792 min Scan# 91
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:105 Resp: 240064
Ion Ratio Lower Upper
105 100
77 90.1 78.6 117.8
51 43.8 37.2 55.8



#17
N-Nitroso-di-n-propylamine
Concen: 86.736 ng/ul
RT: 8.786 min Scan# 952
Delta R.T. 0.017 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 70 Resp: 121576
Ion Ratio Lower Upper
70 100
42 75.8 63.6 95.4
101 9.3 6.3 9.5
130 20.2 17.6 26.4









#18
4-Methylphenol
Concen: 78.848 ng/ul
RT: 8.745 min Scan# 943
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:108 Resp: 137754
Ion Ratio Lower Upper
108 100
107 112.7 95.1 142.7

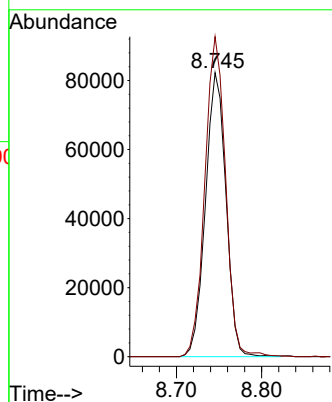

#19
Hexachloroethane
Concen: 82.704 ng/ul
RT: 9.033 min Scan# 994
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:117 Resp: 75112
Ion Ratio Lower Upper
117 100
201 177.6 124.4 186.6
199 108.0 76.3 114.5



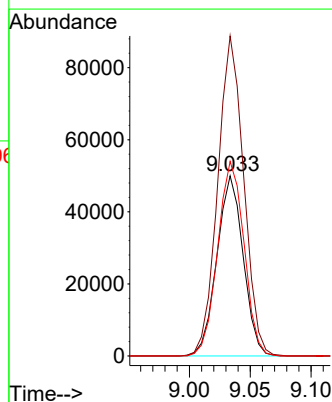



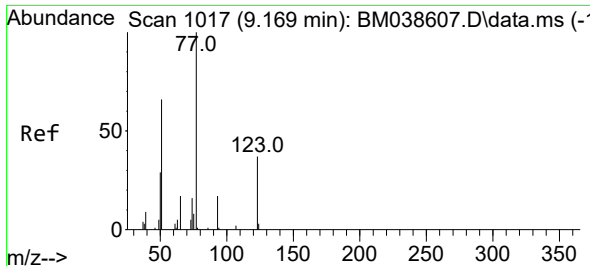

#22
Nitrobenzene
Concen: 80.550 ng/ul
RT: 9.180 min Scan# 1109
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion: 77 Resp: 194301
Ion Ratio Lower Upper
77 100
123 37.5 29.5 44.3
65 16.8 13.6 20.4

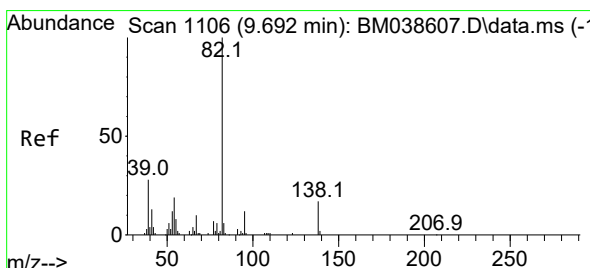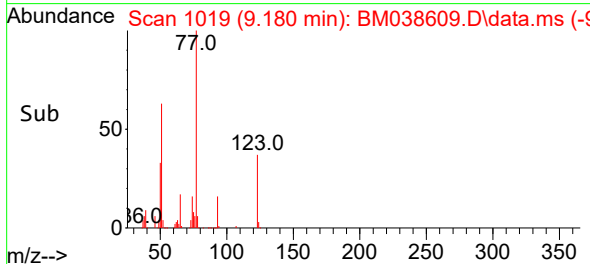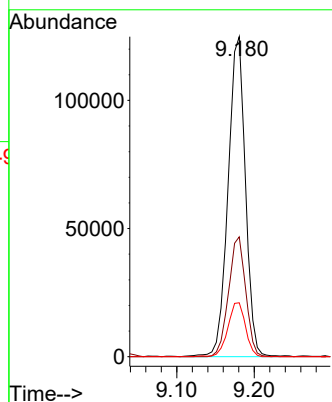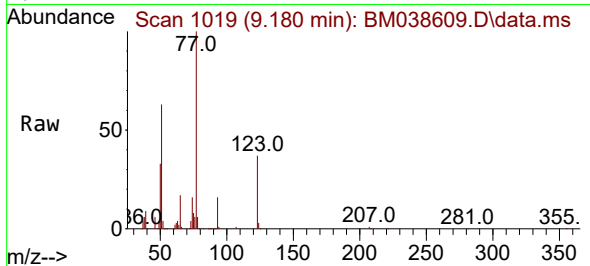

#23
Isophorone
Concen: 84.854 ng/ul
RT: 9.710 min Scan# 1109
Delta R.T. 0.017 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 82 Resp: 309723
Ion Ratio Lower Upper
82 100
95 11.2 9.3 13.9
138 19.9 13.4 20.0


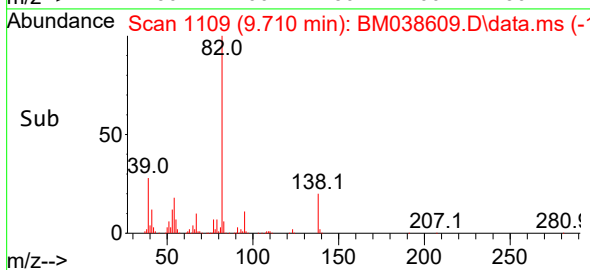

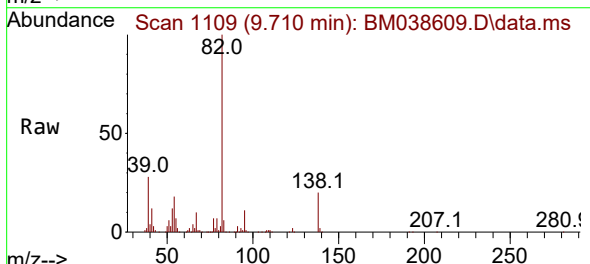


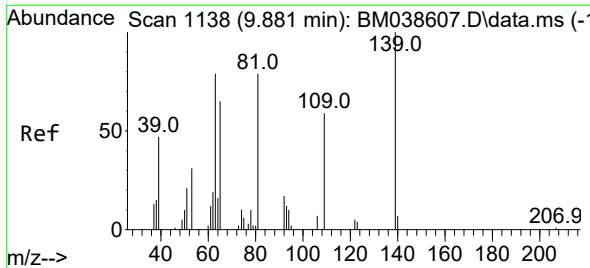

#25
2-Nitrophenol
Concen: 87.995 ng/ul
RT: 9.886 min Scan# 1138
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:139 Resp: 92316
Ion Ratio Lower Upper
139 100
65 68.8 58.6 87.8
109 59.5 46.8 70.2

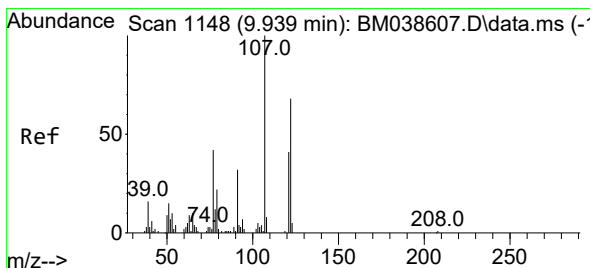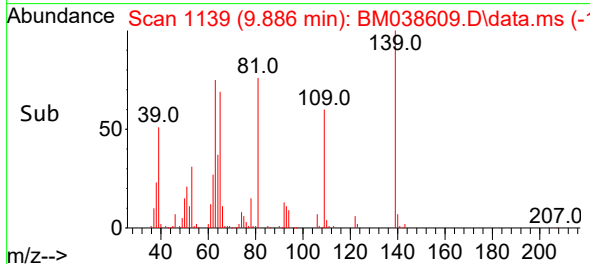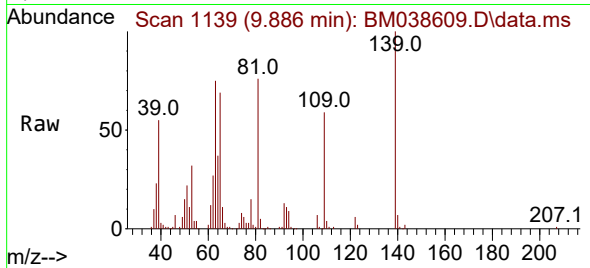

#26
2,4-Dimethylphenol
Concen: 84.775 ng/ul
RT: 9.945 min Scan# 1149
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:107 Resp: 193179
Ion Ratio Lower Upper
107 100
121 41.8 32.6 48.8
122 71.6 54.8 82.2


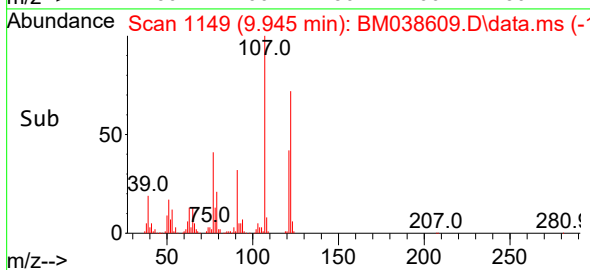

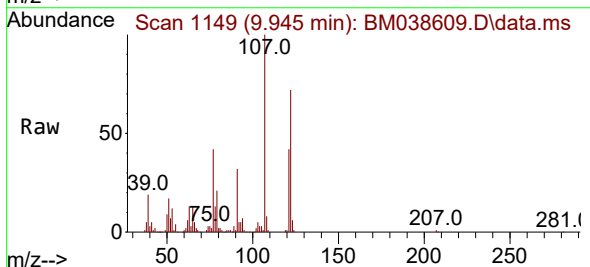




#27
 Bis(2-Chloroethoxy)methane
 Concen: 83.699 ng/ul
 RT: 10.180 min Scan# 1189
 Delta R.T. -0.000 min
 Lab File: BM038609.D
 Acq: 30 Jan 2023 16:46




Instrument :
 BNA_M
 ClientSampleId :
 SSTD080030


Tgt Ion: 93 Resp: 155778
 Ion Ratio Lower Upper
 93 100
 95 33.6 25.3 37.9
 123 11.3 8.6 13.0

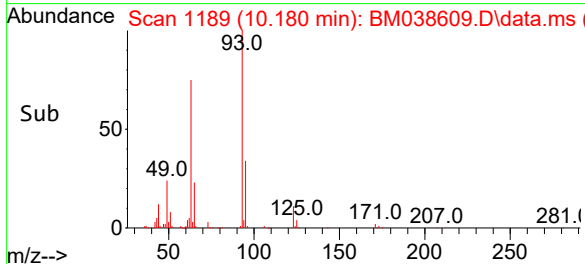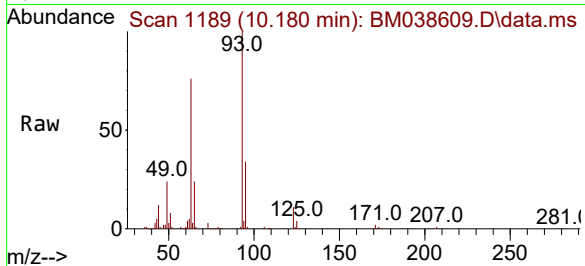

#29
 2,4-Dichlorophenol
 Concen: 93.518 ng/ul
 RT: 10.422 min Scan# 1230
 Delta R.T. 0.006 min
 Lab File: BM038609.D
 Acq: 30 Jan 2023 16:46

Tgt Ion:162 Resp: 208200
 Ion Ratio Lower Upper
 162 100
 164 68.5 56.3 84.5
 98 25.6 24.6 37.0


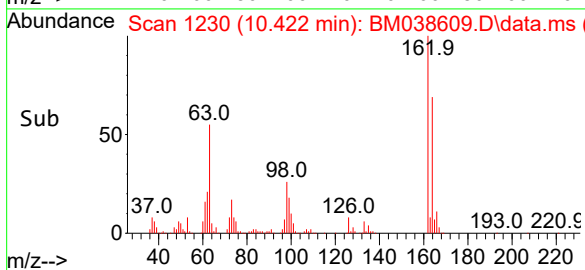

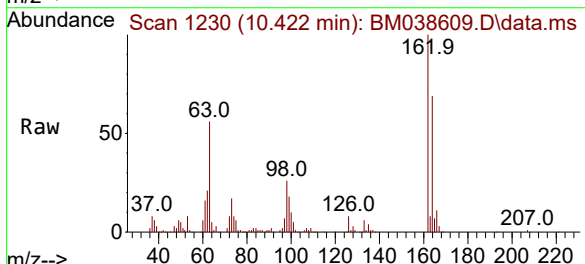




#30
Naphthalene
Concen: 84.591 ng/ul
RT: 10.822 min Scan# 1298
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:128 Resp: 443764
Ion Ratio Lower Upper
128 100
129 11.1 8.0 12.0
127 13.6 10.5 15.7

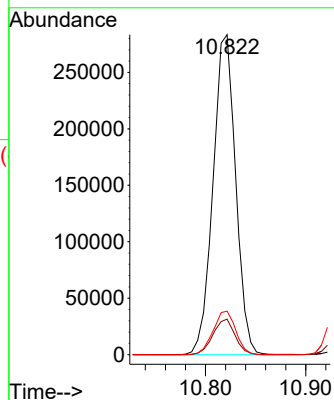

#32
4-Chloroaniline
Concen: 83.572 ng/ul
RT: 10.939 min Scan# 1318
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:127 Resp: 190896
Ion Ratio Lower Upper
127 100
129 32.8 26.9 40.3



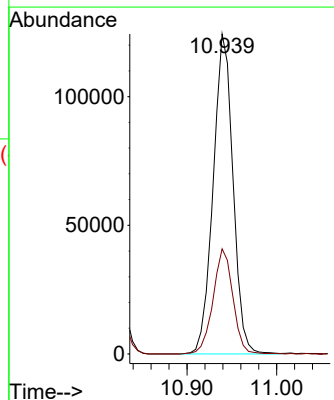





#33
Hexachlorobutadiene
Concen: 81.099 ng/ul
RT: 11.092 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:225 Resp: 187637
Ion Ratio Lower Upper
225 100
223 62.9 48.0 72.0
227 66.2 53.6 80.4



#34
Caprolactam
Concen: 51.295 ng/ul
RT: 11.751 min Scan# 1456
Delta R.T. 0.035 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:113 Resp: 22440
Ion Ratio Lower Upper
113 100
55 140.6 107.6 161.4
56 142.1 96.5 144.7




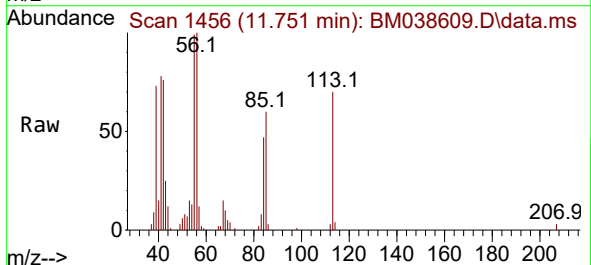




#35
4-Chloro-3-methylphenol
Concen: 90.659 ng/ul
RT: 12.063 min Scan# 1509
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:107 Resp: 159436
Ion Ratio Lower Upper
107 100
144 28.7 18.1 27.1#
142 88.8 60.2 90.4

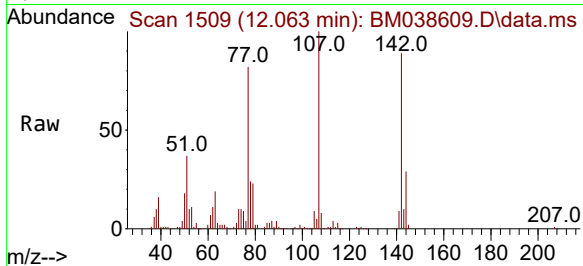

#36
2-Methylnaphthalene
Concen: 93.980 ng/ul
RT: 12.421 min Scan# 1570
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:142 Resp: 366702
Ion Ratio Lower Upper
142 100
141 90.6 73.7 110.5

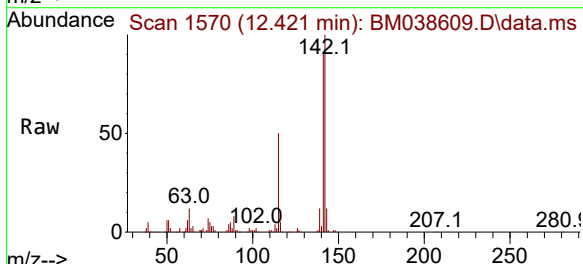



#37

1-Methylnaphthalene

Concen: 93.572 ng/ul

RT: 12.645 min Scan# 1608

Delta R.T. 0.006 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Instrument :

BNA_M

ClientSampleId :

SSTD080030





Tgt Ion:142 Resp: 376894

Ion Ratio Lower Upper

142 100

141 91.8 75.2 112.8

116 5.5 5.0 7.4

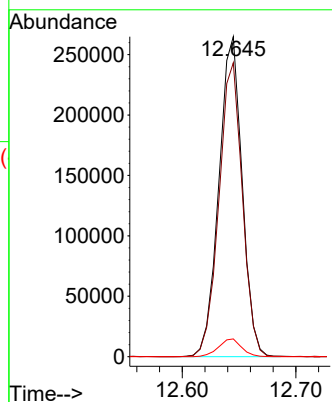

#39

1,2,4,5-Tetrachlorobenzene

Concen: 77.198 ng/ul

RT: 12.792 min Scan# 1633

Delta R.T. 0.006 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Tgt Ion:216 Resp: 329653




Ion Ratio Lower Upper


216 100

214 77.1 61.1 91.7

179 19.6 17.0 25.4

108 13.0 11.4 17.2


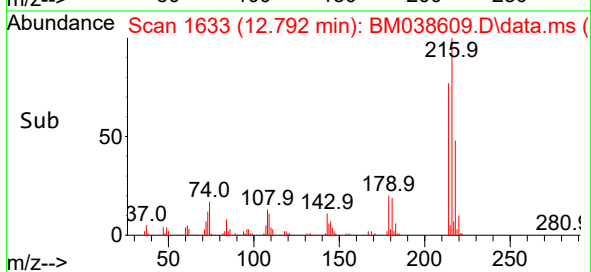






#40
Hexachlorocyclopentadiene
Concen: 79.722 ng/ul
RT: 12.757 min Scan# 1627
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:237 Resp: 242929
Ion Ratio Lower Upper
237 100
235 62.7 49.2 73.8
272 14.4 11.0 16.6



#41
2,4,6-Trichlorophenol
Concen: 83.809 ng/ul
RT: 13.033 min Scan# 1674
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:196 Resp: 217894
Ion Ratio Lower Upper
196 100
198 98.8 83.6 125.4
200 31.6 27.5 41.3


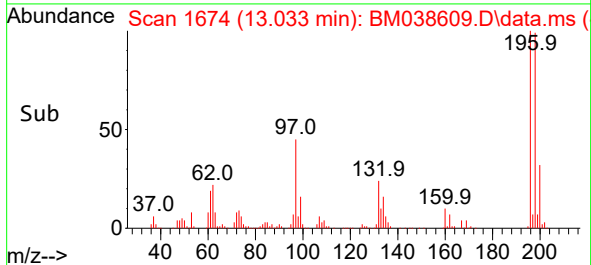






#42
2,4,5-Trichlorophenol
Concen: 83.514 ng/ul
RT: 13.104 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:196 Resp: 231876
Ion Ratio Lower Upper
196 100
198 96.2 73.2 109.8
200 30.2 25.8 38.8



#43
1,1'-Biphenyl
Concen: 86.151 ng/ul
RT: 13.433 min Scan# 1742
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:154 Resp: 574655
Ion Ratio Lower Upper
154 100
153 40.8 33.2 49.8
76 7.4 6.7 10.1




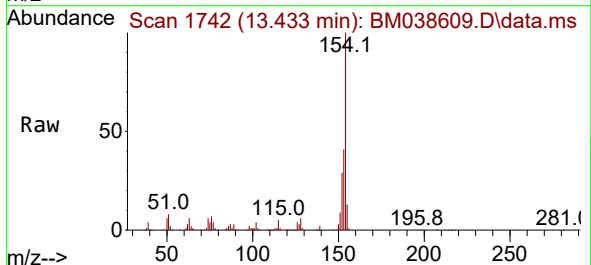




#44
2-Chloronaphthalene
Concen: 86.606 ng/ul
RT: 13.474 min Scan# 1748
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:162 Resp: 479908
Ion Ratio Lower Upper
162 100
164 33.8 26.6 40.0
127 30.6 31.6 47.4#



#45
2-Nitroaniline
Concen: 84.005 ng/ul
RT: 13.692 min Scan# 1786
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion: 65 Resp: 124507
Ion Ratio Lower Upper
65 100
92 54.0 41.5 62.3
138 86.8 63.3 94.9

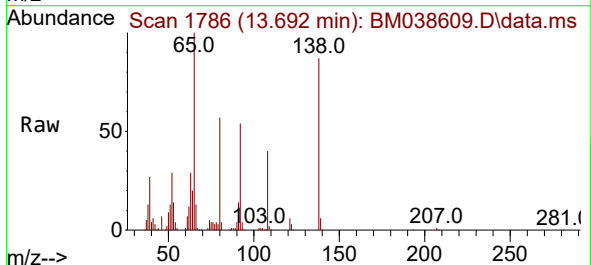



#47

Dimethylphthalate

Concen: 85.254 ng/ul

RT: 14.057 min Scan# 1847

Delta R.T. 0.006 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Instrument :

BNA_M

ClientSampleId :

SSTD080030





Tgt Ion:163 Resp: 601136

Ion Ratio Lower Upper

163 100

194 4.9 3.5 5.3

164 10.0 8.0 12.0

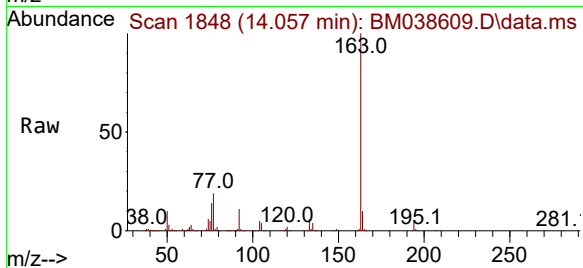

#48

2,6-Dinitrotoluene

Concen: 92.349 ng/ul

RT: 14.186 min Scan# 1870

Delta R.T. 0.006 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46




Tgt Ion:165 Resp: 120600


Ion Ratio Lower Upper

165 100

89 69.9 66.7 100.1

121 18.3 18.2 27.4




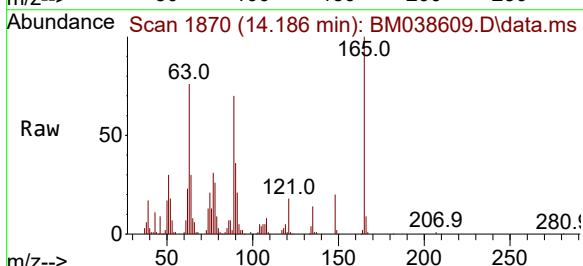




#50
Acenaphthylene
Concen: 87.547 ng/ul
RT: 14.321 min Scan# 1893
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:152 Resp: 667609
Ion Ratio Lower Upper
152 100
151 20.2 17.7 26.5
153 13.0 10.6 16.0

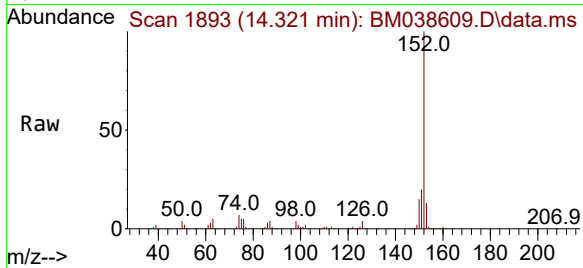

#51
3-Nitroaniline
Concen: 83.550 ng/ul
RT: 14.515 min Scan# 1926
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:138 Resp: 78537
Ion Ratio Lower Upper
138 100
108 10.6 8.2 12.4
92 117.6 94.2 141.4




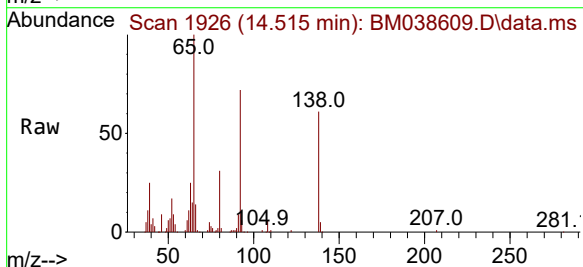




#52
Acenaphthene
Concen: 86.282 ng/ul
RT: 14.657 min Scan# 1950
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:153 Resp: 489745
Ion Ratio Lower Upper
153 100
152 47.9 40.6 61.0
154 88.3 68.7 103.1

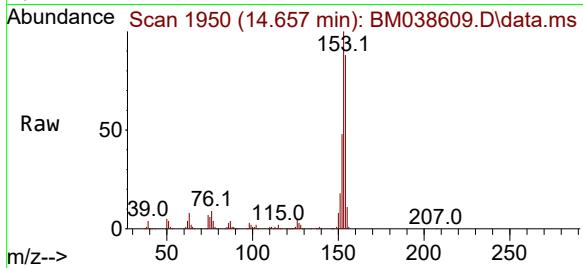

#53
2,4-Dinitrophenol
Concen: 91.582 ng/ul
RT: 14.721 min Scan# 1961
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:184 Resp: 96144
Ion Ratio Lower Upper
184 100
63 74.5 59.7 89.5
154 86.0 79.6 119.4




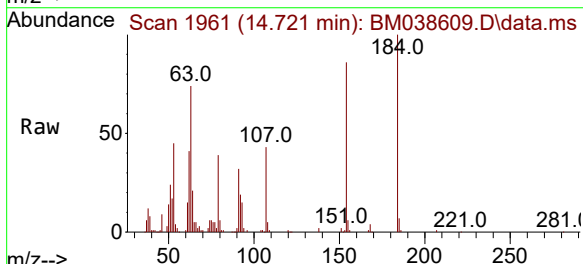




#55
4-Nitrophenol
Concen: 82.183 ng/ul
RT: 14.827 min Scan# 1977
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:109 Resp: 136679
Ion Ratio Lower Upper
109 100
139 61.2 41.3 61.9
65 84.0 63.4 95.2

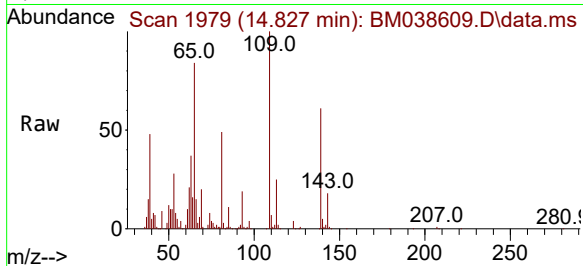

#56
Dibenzofuran
Concen: 90.082 ng/ul
RT: 14.992 min Scan# 2007
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:168 Resp: 760484
Ion Ratio Lower Upper
168 100
139 35.6 35.4 53.0




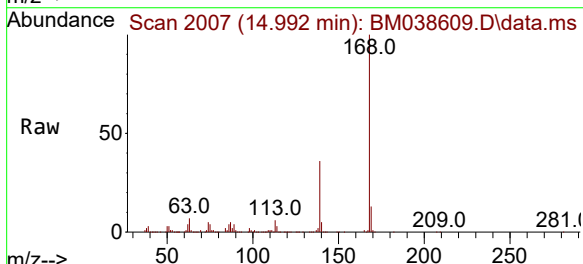




#57
2,4-Dinitrotoluene
Concen: 94.249 ng/ul
RT: 14.974 min Scan# 2004
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:165 Resp: 181412
Ion Ratio Lower Upper
165 100
63 55.2 53.1 79.7
182 2.6 2.8 4.2#

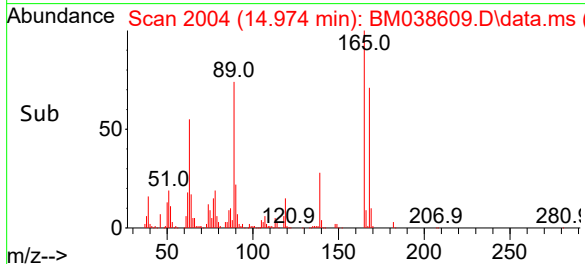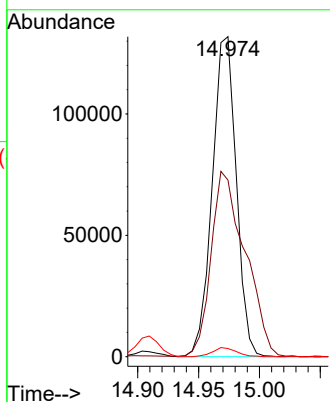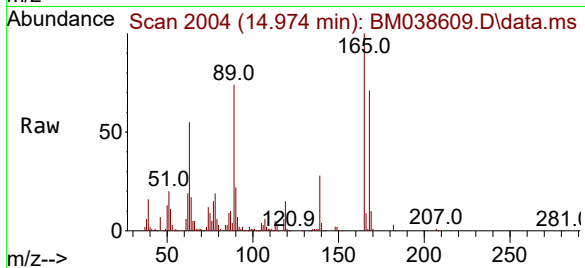

#58
2,3,4,6-Tetrachlorophenol
Concen: 82.373 ng/ul
RT: 15.215 min Scan# 2045
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:232 Resp: 200244
Ion Ratio Lower Upper
232 100
131 33.4 30.4 45.6
130 2.4 2.4 3.6#
166 26.3 22.2 33.2


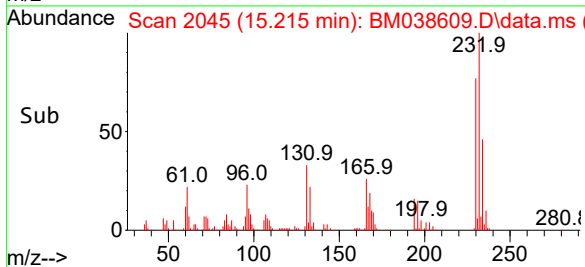

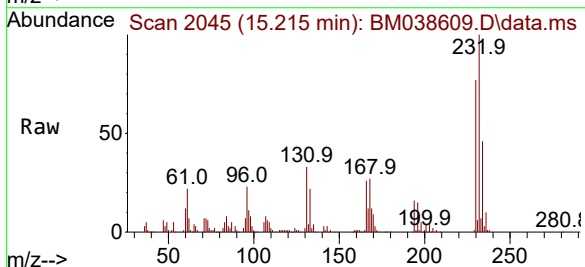




#59
Diethylphthalate
Concen: 85.141 ng/ul
RT: 15.409 min Scan# 2077
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:149 Resp: 562810
Ion Ratio Lower Upper
149 100
177 25.9 18.0 27.0
150 13.0 10.4 15.6



#61
Fluorene
Concen: 99.299 ng/ul
RT: 15.639 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:166 Resp: 705996
Ion Ratio Lower Upper
166 100
165 98.7 83.3 124.9
167 13.6 10.6 16.0









#62
4-Chlorophenyl-phenylether
Concen: 88.033 ng/ul
RT: 15.633 min Scan# 2116
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:204 Resp: 440406
Ion Ratio Lower Upper
204 100
206 32.2 27.9 41.9
141 42.8 41.4 62.0

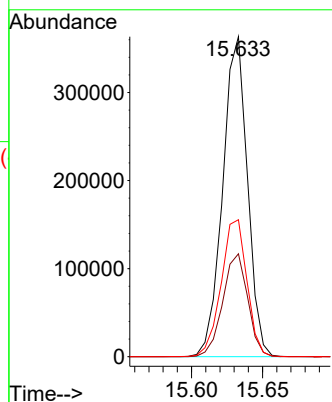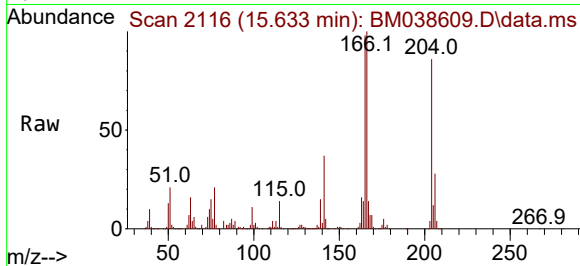

#63
4-Nitroaniline
Concen: 78.927 ng/ul
RT: 15.680 min Scan# 2124
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:138 Resp: 59778
Ion Ratio Lower Upper
138 100
92 57.3 51.9 77.9
108 191.8 156.2 234.4




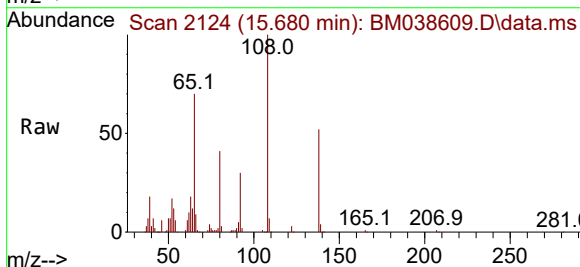




#66
4,6-Dinitro-2-methylphenol
Concen: 84.355 ng/ul
RT: 15.733 min Scan# 2133
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:198 Resp: 145491
Ion Ratio Lower Upper
198 100
182 2.5 2.7 4.1#
77 25.3 23.9 35.9

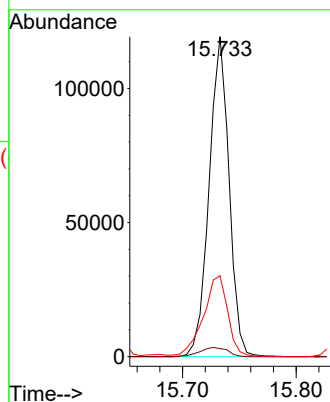

#67
N-Nitrosodiphenylamine
Concen: 90.012 ng/ul
RT: 15.851 min Scan# 2153
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:169 Resp: 541824
Ion Ratio Lower Upper
169 100
168 69.4 59.1 88.7
167 37.2 31.6 47.4









#68
4-Bromophenyl-phenylether
Concen: 81.911 ng/ul
RT: 16.521 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:248 Resp: 246414
Ion Ratio Lower Upper
248 100
250 97.8 77.8 116.6
141 61.0 52.3 78.5

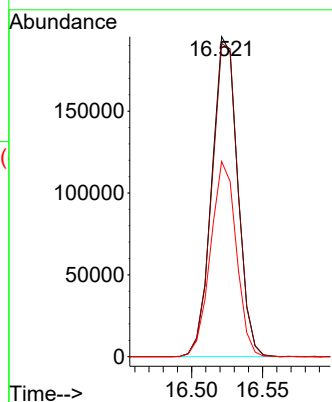

#69
Hexachlorobenzene
Concen: 85.157 ng/ul
RT: 16.639 min Scan# 2287
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:284 Resp: 299050
Ion Ratio Lower Upper
284 100
142 26.9 28.0 42.0#
249 28.5 23.9 35.9









#70
Atrazine
Concen: 80.732 ng/ul
RT: 16.803 min Scan# 21
Delta R.T. 0.012 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:200 Resp: 243834
Ion Ratio Lower Upper
200 100
173 21.1 15.2 22.8
215 46.7 36.6 54.8

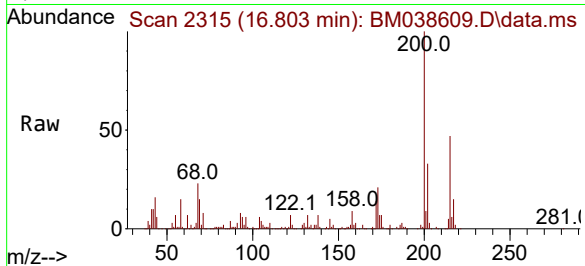

#71
Pentachlorophenol
Concen: 81.539 ng/ul
RT: 16.986 min Scan# 2346
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:266 Resp: 183168
Ion Ratio Lower Upper
266 100
264 62.5 47.2 70.8
268 65.3 45.8 68.6




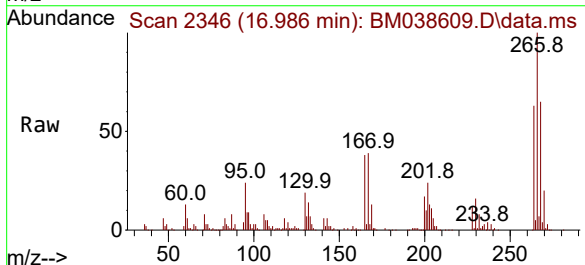




#72
Phenanthrene
Concen: 93.770 ng/ul
RT: 17.380 min Scan# 2412
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:178 Resp: 1046247
Ion Ratio Lower Upper
178 100
179 15.6 11.7 17.5
176 19.6 16.2 24.2



#74
Anthracene
Concen: 95.381 ng/ul
RT: 17.474 min Scan# 2429
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:178 Resp: 1114420
Ion Ratio Lower Upper
178 100
179 15.5 12.3 18.5
176 19.3 16.3 24.5









#75
1,2,3,4-Tetrachlorobenzene
Concen: 76.596 ng/uL
RT: 13.398 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:216 Resp: 314323
Ion Ratio Lower Upper
216 100
214 76.1 62.5 93.7
218 46.9 37.4 56.0



#76
Pentachlorobenzene
Concen: 78.135 ng/uL
RT: 14.909 min Scan# 1993
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:250 Resp: 333640
Ion Ratio Lower Upper
250 100
248 64.4 50.6 75.8
252 62.6 51.3 76.9


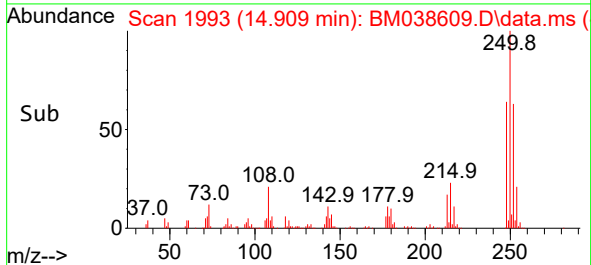






#77
 Carbazole
 Concen: 83.734 ng/ul
 RT: 17.745 min Scan# 2475
 Delta R.T. 0.006 min
 Lab File: BM038609.D
 Acq: 30 Jan 2023 16:46




Instrument :
 BNA_M
 ClientSampleId :
 SST080030


Tgt Ion:167 Resp: 849201
 Ion Ratio Lower Upper
 167 100
 166 22.5 19.5 29.3
 139 12.1 11.3 16.9

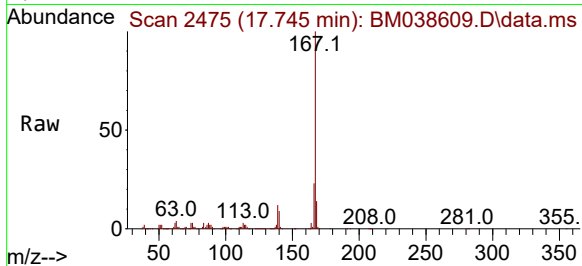

#78
 Di-n-butylphthalate
 Concen: 93.228 ng/ul
 RT: 18.292 min Scan# 2568
 Delta R.T. -0.000 min
 Lab File: BM038609.D
 Acq: 30 Jan 2023 16:46

Tgt Ion:149 Resp: 914754
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.2 10.8
 104 7.0 6.2 9.4




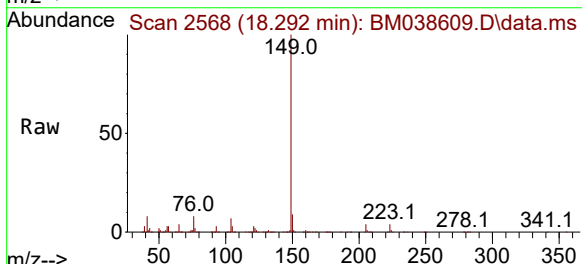




#80
Fluoranthene
Concen: 89.816 ng/ul
RT: 19.392 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:202 Resp: 1405333
Ion Ratio Lower Upper
202 100
101 2.7 2.8 4.2#
100 2.2 2.4 3.6#



#82
Pyrene
Concen: 92.068 ng/ul
RT: 19.756 min Scan# 2817
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:202 Resp: 1528772
Ion Ratio Lower Upper
202 100
101 3.2 3.3 4.9#
100 2.8 2.8 4.2





#83

Butylbenzylphthalate

Concen: 93.084 ng/ul

RT: 20.639 min Scan# 2967

Delta R.T. -0.000 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Instrument :

BNA_M

ClientSampleId :

SSTD080030





Tgt Ion:149 Resp: 445827

Ion Ratio Lower Upper

149 100

91 67.3 59.0 88.4

206 26.7 19.0 28.6

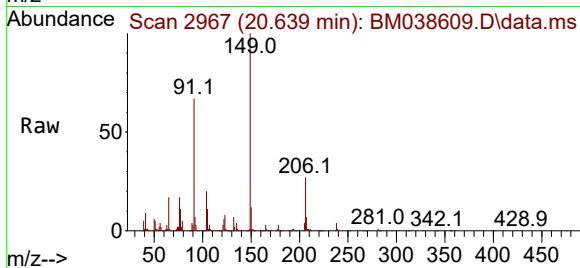

#84

3,3'-Dichlorobenzidine

Concen: 82.557 ng/ul

RT: 21.427 min Scan# 3101

Delta R.T. -0.000 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46




Tgt Ion:252 Resp: 531329


Ion Ratio Lower Upper

252 100

254 64.5 52.7 79.1

126 5.3 5.0 7.4




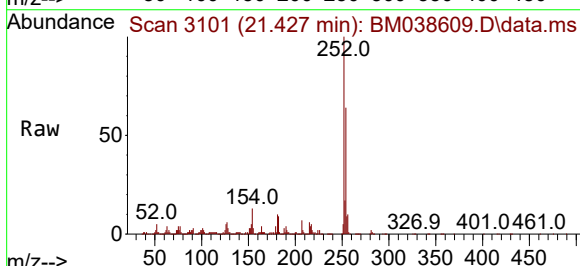




#85
Benzo(a)anthracene
Concen: 86.014 ng/ul
RT: 21.497 min Scan# 3112
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:228 Resp: 1596252
Ion Ratio Lower Upper
228 100
229 19.7 15.8 23.6
226 27.5 22.2 33.4

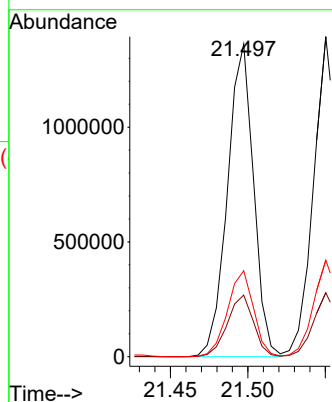

#86
Bis(2-ethylhexyl)phthalate
Concen: 96.686 ng/ul
RT: 21.409 min Scan# 3098
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:149 Resp: 658924
Ion Ratio Lower Upper
149 100
167 30.0 21.0 31.4
279 7.0 5.1 7.7

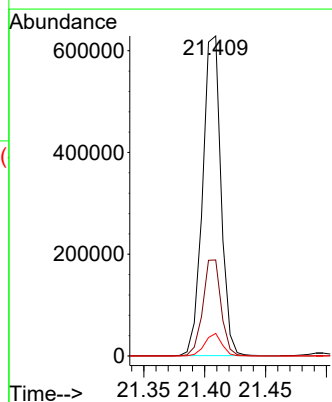



#87

Chrysene

Concen: 88.589 ng/ul

RT: 21.550 min Scan# 31

Delta R.T. 0.006 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Instrument :

BNA_M

ClientSampleId :

SSTD080030





Tgt Ion:228 Resp: 1521725

Ion Ratio Lower Upper

228 100

226 30.2 24.5 36.7

229 20.0 15.6 23.4



#89

Di-n-octyl phthalate

Concen: 86.374 ng/ul




RT: 22.333 min Scan# 3255


Delta R.T. -0.000 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Tgt Ion:149 Resp: 1198186









#90
Benzo(b)fluoranthene
Concen: 93.282 ng/ul
RT: 23.185 min Scan# 3400
Delta R.T. 0.006 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46




Instrument :
BNA_M
ClientSampleId :
SSTD080030


Tgt Ion:252 Resp: 1889031
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.6
125 2.8 2.6 3.8

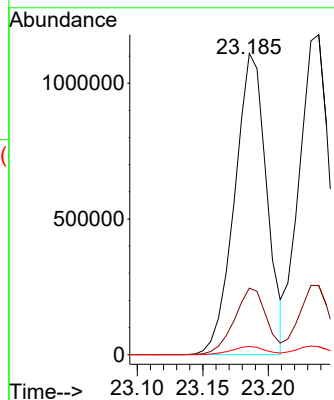

#91
Benzo(k)fluoranthene
Concen: 93.622 ng/ul
RT: 23.185 min Scan# 3400
Delta R.T. -0.041 min
Lab File: BM038609.D
Acq: 30 Jan 2023 16:46

Tgt Ion:252 Resp: 1889031
Ion Ratio Lower Upper
252 100
253 22.1 18.2 27.2
125 2.8 2.6 4.0

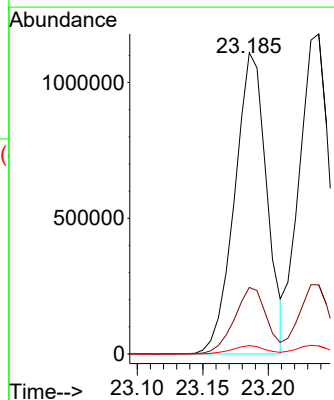



#93

Benzo(a)pyrene

Concen: 90.863 ng/ul

RT: 23.821 min Scan# 3

Delta R.T. 0.012 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Instrument :

BNA_M

ClientSampleId :

SSTD080030





Tgt Ion:252 Resp: 1703988

Ion Ratio Lower Upper

252 100

253 22.0 17.8 26.8

125 2.9 2.8 4.2

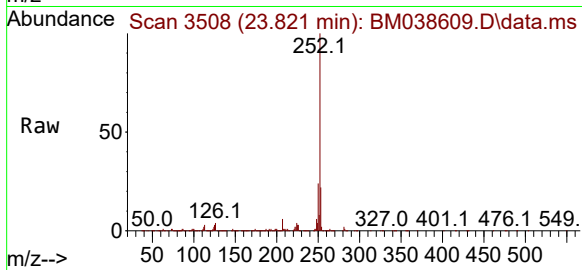

#94

Indeno(1,2,3-cd)pyrene

Concen: 87.918 ng/ul

RT: 26.450 min Scan# 3955

Delta R.T. 0.029 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46




Tgt Ion:276 Resp: 2606154


Ion Ratio Lower Upper

276 100

138 7.8 6.1 9.1

277 25.3 20.5 30.7

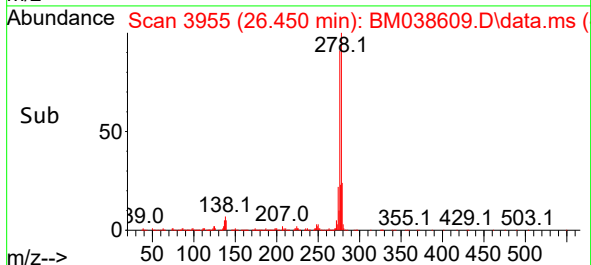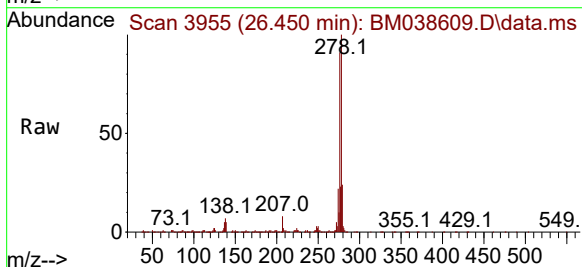



#95

Dibenzo(a,h)anthracene

Concen: 89.832 ng/ul

RT: 26.456 min Scan# 3956

Delta R.T. 0.023 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Instrument :

BNA_M

ClientSampleId :

SSTD080030





Tgt Ion:278 Resp: 2260051

Ion Ratio Lower Upper

278 100

139 4.9 4.3 6.5

279 24.0 18.9 28.3



#96

Benzo(g,h,i)perylene

Concen: 82.585 ng/ul

RT: 27.220 min Scan# 4086

Delta R.T. 0.023 min

Lab File: BM038609.D

Acq: 30 Jan 2023 16:46

Tgt Ion:276 Resp: 1987006

Ion Ratio Lower Upper

276 100

138 6.3 6.0 9.0

277 23.9 19.2 28.8

