

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038622.D
 Acq On : 31 Jan 2023 16:42
 Operator : CG/JU
 Sample : PB150488BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Quant Time: Feb 01 00:04:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 01:02:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	35785	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	97476	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	71267	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	183740	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.503	240	206762	20.000	ng/ul	0.00
88) Perylene-d12	23.909	264	318490	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	4686	4.669	ng/uL	0.00
4) Pyridine-d5	3.763	84	60410	24.037	ng/ul	0.00
7) Phenol-d5	7.116	99	58706	24.577	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	35820	25.691	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	51474	25.985	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	45541	23.895	ng/ul	0.00
21) Nitrobenzene-d5	9.128	128	21326	28.863	ng/ul	0.00
24) 2-Nitrophenol-d4	9.845	143	29859	30.601	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.386	165	64606	29.917	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	54429	25.935	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	176024	29.900	ng/ul	0.00
49) Acenaphthylene-d8	14.286	160	177462	28.327	ng/ul	0.00
54) 4-Nitrophenol-d4	14.798	143	19357	23.769	ng/ul	0.00
60) Fluorene-d10	15.580	176	159530	30.302	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	41727	26.530	ng/ul	0.00
73) Anthracene-d10	17.427	188	266605	28.826	ng/ul	0.00
81) Pyrene-d10	19.721	212	342924	32.188	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.756	264	484808	29.656	ng/ul	0.00
Target Compounds						
					Qvalue	
17) N-Nitroso-di-n-propyla...	8.663	70	1758	1.136	ng/ul#	1
23) Isophorone	9.845	82	4999	1.486	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038622.D
Acq On : 31 Jan 2023 16:42
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Time: Feb 01 00:04:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 01:02:54 2023
Response via : Initial Calibration

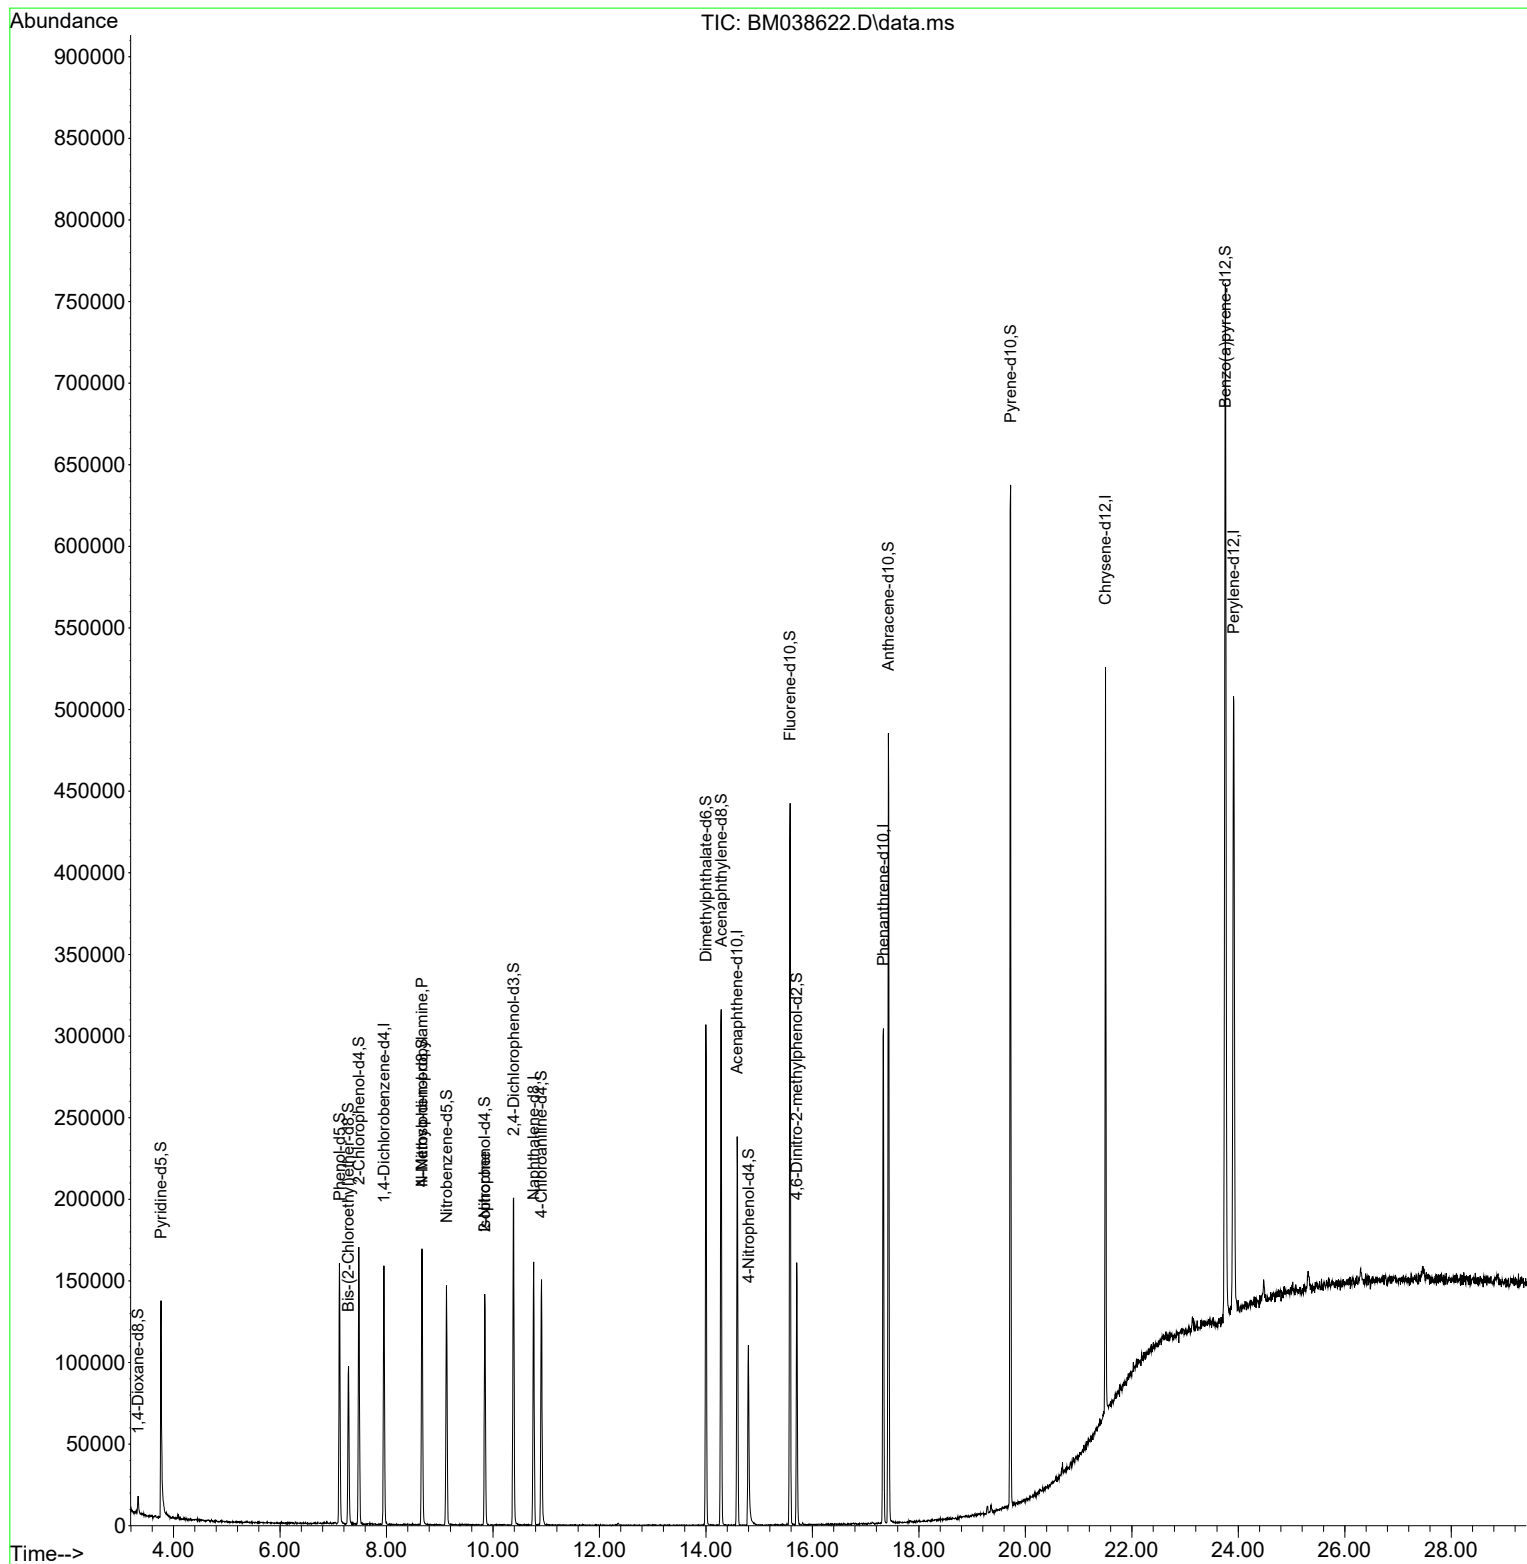




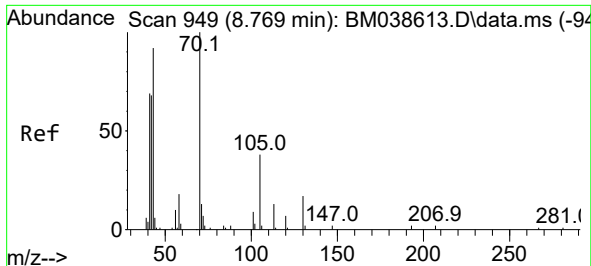


#17
N-Nitroso-di-n-propylamine
Concen: 1.136 ng/ul
RT: 8.663 min Scan# 911
Delta R.T. -0.106 min
Lab File: BM038622.D
Acq: 31 Jan 2023 16:42

Instrument :
BNA_M
ClientSampleId :
SBLK488

Tgt Ion: 70 Resp: 1758

Ion	Ratio	Lower	Upper
70	100		
42	356.4	63.6	95.4#
101	0.0	6.3	9.5#
130	0.0	17.6	26.4#

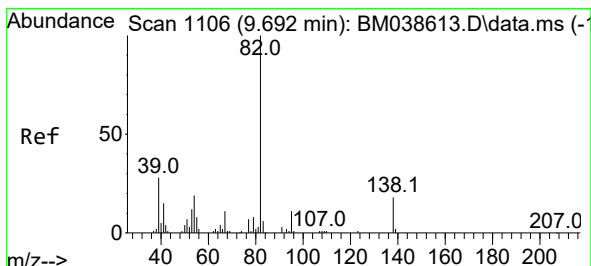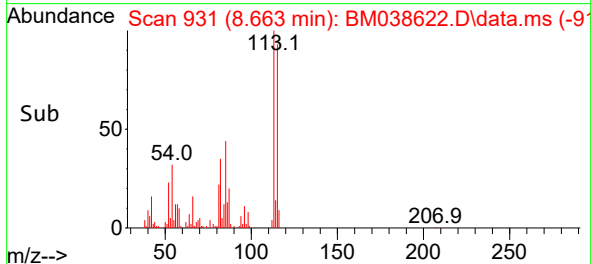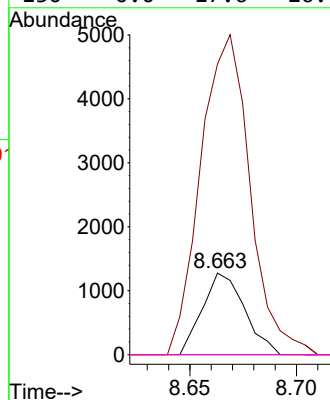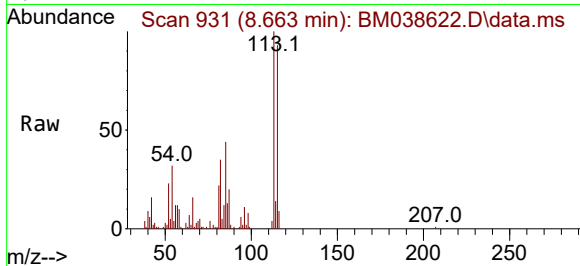

#23
Isophorone
Concen: 1.486 ng/ul
RT: 9.845 min Scan# 1132
Delta R.T. 0.153 min
Lab File: BM038622.D
Acq: 31 Jan 2023 16:42

Tgt Ion: 82 Resp: 4999

Ion	Ratio	Lower	Upper
82	100		
95	0.0	9.3	13.9#
138	0.0	13.4	20.0#

