




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038634.D
Acq On : 01 Feb 2023 00:06
Operator : CG/JU
Sample : 01277-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G8

Manual IntegrationsAPPROVED

Quant Time: Feb 01 02:03:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 01:02:54 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/01/2023
Supervised By :mohammad ahmed 02/01/2023

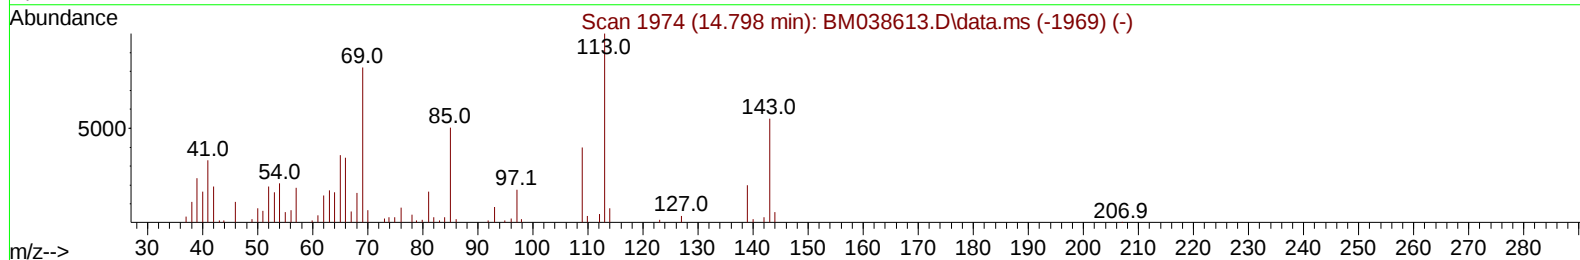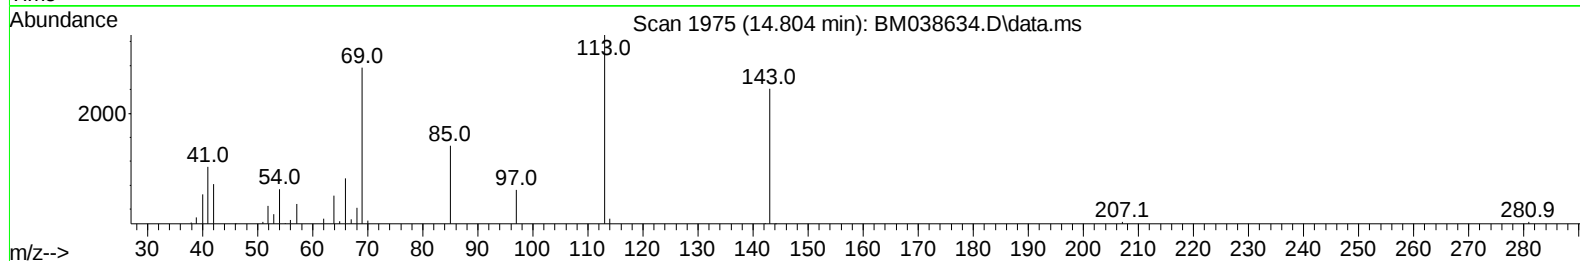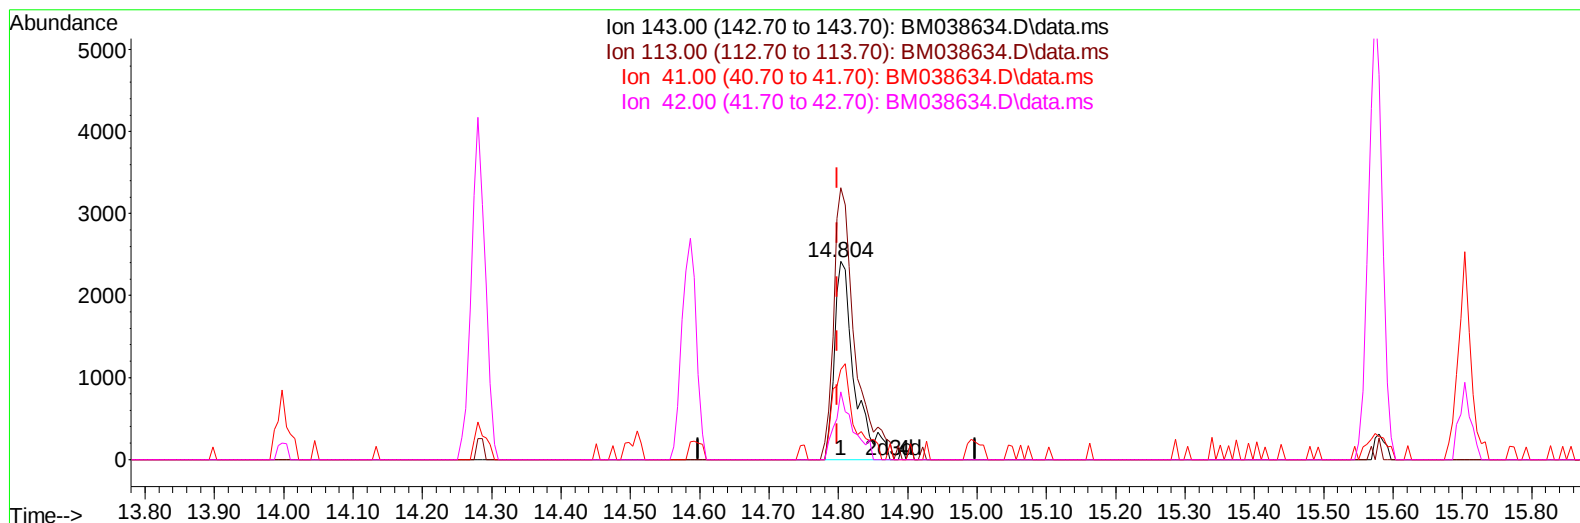

TIC: BM038634.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (+ 0.006) 5.88 ng/ul m

response 4872

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	145.20	137.09
41.00	54.70	45.57
42.00	40.10	33.98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038634.D
 Acq On : 01 Feb 2023 00:06
 Operator : CG/JU
 Sample : 01277-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9G8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/01/2023
 Supervised By :mohammad ahmed 02/01/2023

Quant Time: Feb 01 02:03:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 01:02:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	35308	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	94658	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.586	164	72533	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.327	188	190663	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.503	240	223623	20.000	ng/ul	0.00
88) Perylene-d12	23.909	264	319286	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	4500	4.544	ng/uL	0.00
4) Pyridine-d5	3.769	84	24862	10.026	ng/ul	0.00
7) Phenol-d5	7.116	99	17330	7.353	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	43991	31.978	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	51721	26.462	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	32191	17.118	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	28111	39.178	ng/ul	0.00
24) 2-Nitrophenol-d4	9.845	143	37616	39.698	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.380	165	79062	37.701	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	53693	26.346	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	241753	40.349	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	252631	39.622	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	4872m	5.878	ng/ul	0.00
60) Fluorene-d10	15.574	176	223967	41.799	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	53616	32.851	ng/ul	0.00
73) Anthracene-d10	17.427	188	385844	40.204	ng/ul	0.00
81) Pyrene-d10	19.715	212	499999	43.393	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.750	264	674173	41.137	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038634.D
Acq On : 01 Feb 2023 00:06
Operator : CG/JU
Sample : 01277-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/01/2023
Supervised By :mohammad ahmed 02/01/2023

Quant Time: Feb 01 02:03:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 01:02:54 2023
Response via : Initial Calibration

