

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038636.D
 Acq On : 01 Feb 2023 01:19
 Operator : CG/JU
 Sample : 01277-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9H0

Quant Time: Feb 01 02:11:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 31 01:02:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.951	152	36243	20.000 ng/ul	0.00
20) Naphthalene-d8	10.757	136	97308	20.000 ng/ul	-0.01
38) Acenaphthene-d10	14.586	164	75453	20.000 ng/ul	0.00
64) Phenanthrene-d10	17.327	188	199469	20.000 ng/ul	# 0.00
79) Chrysene-d12	21.503	240	232456	20.000 ng/ul	0.00
88) Perylene-d12	23.909	264	320830	20.000 ng/ul	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.328	96	4143	4.076 ng/uL	0.00
4) Pyridine-d5	3.769	84	21789	8.560 ng/ul	0.00
7) Phenol-d5	7.116	99	21131	8.735 ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	35740	25.310 ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	44262	22.062 ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	35157	18.213 ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	23055	31.257 ng/ul	0.00
24) 2-Nitrophenol-d4	9.845	143	32039	32.892 ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	72637	33.694 ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	36276	17.315 ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	206062	33.061 ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	218355	32.921 ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	3909	4.534 ng/ul	0.00
60) Fluorene-d10	15.574	176	197273	35.392 ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	47480	27.807 ng/ul	0.00
73) Anthracene-d10	17.427	188	335836	33.448 ng/ul	0.00
81) Pyrene-d10	19.715	212	442067	36.907 ng/ul	0.00
92) Benzo(a)pyrene-d12	23.756	264	577543	35.071 ng/ul	0.00
Target Compounds					
26) 2,4-Dimethylphenol	9.969	107	2368	1.129 ng/ul#	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038636.D
Acq On : 01 Feb 2023 01:19
Operator : CG/JU
Sample : 01277-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9H0


Quant Time: Feb 01 02:11:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 31 01:02:54 2023
Response via : Initial Calibration

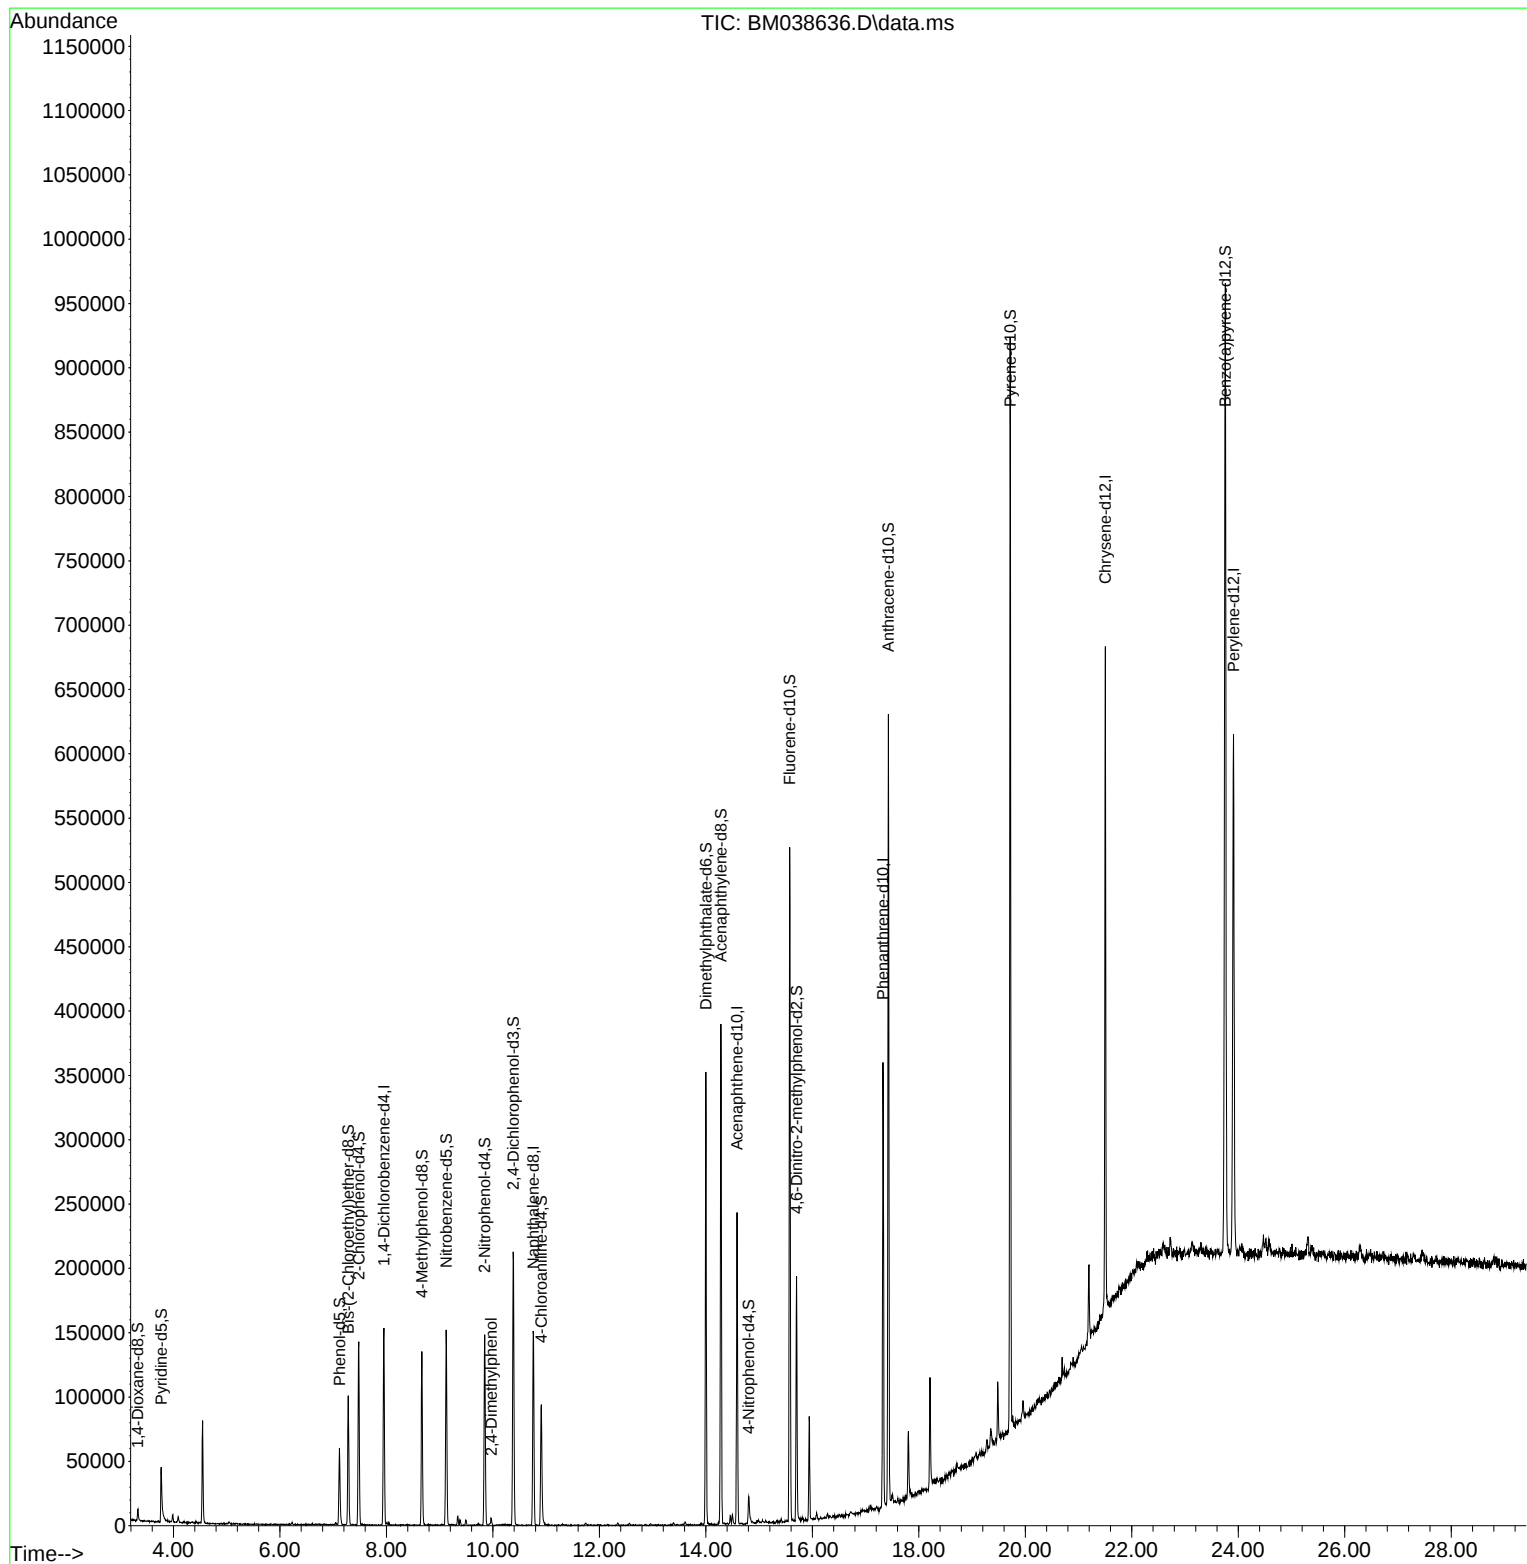

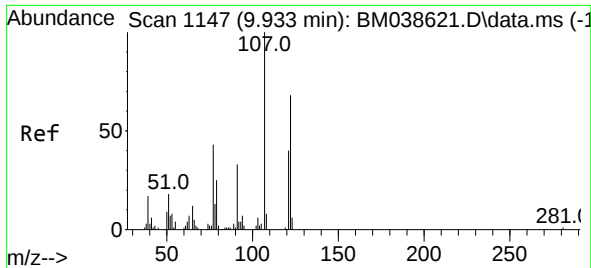

#26
 2,4-Dimethylphenol
 Concen: 1.129 ng/ul
 RT: 9.969 min Scan# 1147
 Delta R.T. 0.029 min
 Lab File: BM038636.D
 Acq: 01 Feb 2023 01:19

Instrument :
 BNA_M
 ClientSampleId :
 EX9H0

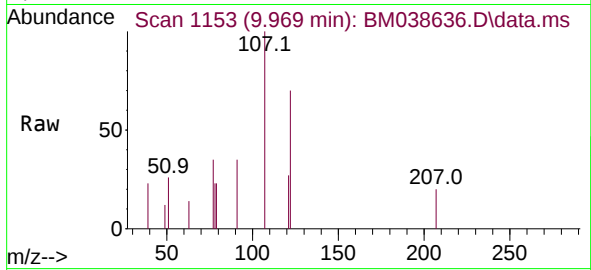

Tgt Ion:	107	Resp:	2368
Ion	Ratio	Lower	Upper
107	100		
121	27.3	32.6	48.8#
122	69.7	54.8	82.2

