

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038614.D
 Acq On : 31 Jan 2023 11:45
 Operator : CG/JU
 Sample : PB150488BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	22	25	29	rVB3	8114	9355	0.92%	0.125%
2	3.557	61	63	65	rBV3	967	1045	0.10%	0.014%
3	3.763	94	98	113	rBV	103939	158610	15.63%	2.125%
4	4.022	140	142	144	rBV2	1282	1225	0.12%	0.016%
5	4.093	149	154	158	rBV5	3190	4795	0.47%	0.064%
6	4.187	169	170	176	rBV3	726	1308	0.13%	0.018%
7	4.393	201	205	208	rBV4	1208	1758	0.17%	0.024%
8	4.428	208	211	214	rBV4	1580	1590	0.16%	0.021%
9	4.675	248	253	254	rBV3	836	1174	0.12%	0.016%
10	5.775	437	440	442	rVV2	1067	1184	0.12%	0.016%
11	6.340	532	536	537	rBV2	776	1065	0.10%	0.014%
12	6.887	625	629	631	rBV3	740	1063	0.10%	0.014%
13	7.010	648	650	655	rVB2	718	1067	0.11%	0.014%
14	7.116	663	668	675	rBV	119882	181521	17.89%	2.431%
15	7.287	691	697	707	rVB	71897	114786	11.31%	1.538%
16	7.422	717	720	723	rBV2	807	1169	0.12%	0.016%
17	7.481	723	730	738	rBV	130899	198037	19.52%	2.653%
18	7.951	804	810	820	rBV	119510	179716	17.71%	2.407%
19	8.410	883	888	890	rBV	557	1054	0.10%	0.014%
20	8.669	926	932	943	rVB	128434	201831	19.89%	2.704%
21	9.128	1004	1010	1021	rVB	109662	171345	16.89%	2.295%
22	9.845	1127	1132	1142	rVB	104677	171958	16.95%	2.303%
23	10.386	1217	1224	1235	rBV	151988	246365	24.28%	3.300%
24	10.763	1279	1288	1295	rBV	119945	189108	18.64%	2.533%
25	10.910	1307	1313	1320	rBV	111425	186319	18.36%	2.496%
26	12.363	1556	1560	1564	rVB2	1190	1578	0.16%	0.021%
27	14.004	1833	1839	1851	rVB	223541	309372	30.49%	4.144%
28	14.286	1880	1887	1896	rBV	239213	337586	33.27%	4.522%
29	14.586	1933	1938	1946	rVB	180869	253080	24.94%	3.390%
30	14.798	1968	1974	1987	rBV	83702	142527	14.05%	1.909%
31	15.580	2101	2107	2115	rBV	340232	457832	45.12%	6.133%
32	15.704	2123	2128	2135	rBV	126993	166389	16.40%	2.229%
33	17.062	2358	2359	2365	rVB3	684	1174	0.12%	0.016%
34	17.333	2399	2405	2412	rVB	252084	344887	33.99%	4.620%
35	17.433	2415	2422	2432	rVV	386380	536258	52.85%	7.183%
36	17.698	2465	2467	2470	rBV2	1189	1266	0.12%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038614.D
 Acq On : 31 Jan 2023 11:45
 Operator : CG/JU
 Sample : PB150488BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	17.974	2509	2514	2517	rBV3	718	1095	0.11%	0.015%
38	18.051	2524	2527	2530	rBV2	970	1228	0.12%	0.016%
39	18.215	2551	2555	2557	rBV4	1041	1760	0.17%	0.024%
40	18.309	2569	2571	2575	rVB3	1181	1272	0.13%	0.017%
41	18.492	2598	2602	2606	rVB3	1237	1579	0.16%	0.021%
42	18.656	2627	2630	2632	rBV4	1164	1635	0.16%	0.022%
43	18.786	2648	2652	2654	rBV3	1294	1413	0.14%	0.019%
44	18.974	2679	2684	2687	rBV5	1486	2401	0.24%	0.032%
45	19.251	2729	2731	2733	rBV3	1143	1224	0.12%	0.016%
46	19.286	2733	2737	2742	rVV5	4953	7404	0.73%	0.099%
47	19.356	2746	2749	2754	rVB3	3393	5513	0.54%	0.074%
48	19.509	2773	2775	2776	rBV2	1612	1196	0.12%	0.016%
49	19.721	2805	2811	2817	rBV	522417	687152	67.72%	9.204%
50	19.915	2842	2844	2845	rBV2	1910	1079	0.11%	0.014%
51	20.127	2878	2880	2882	rBV3	2689	2292	0.23%	0.031%
52	21.503	3109	3114	3122	rBV	391983	477396	47.05%	6.395%
53	23.756	3490	3497	3508	rBV2	550607	1014652	100.00%	13.591%
54	23.909	3517	3523	3535	rVB	355925	674812	66.51%	9.039%




Sum of corrected areas: 7465500

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038614.D
Acq On : 31 Jan 2023 11:45
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

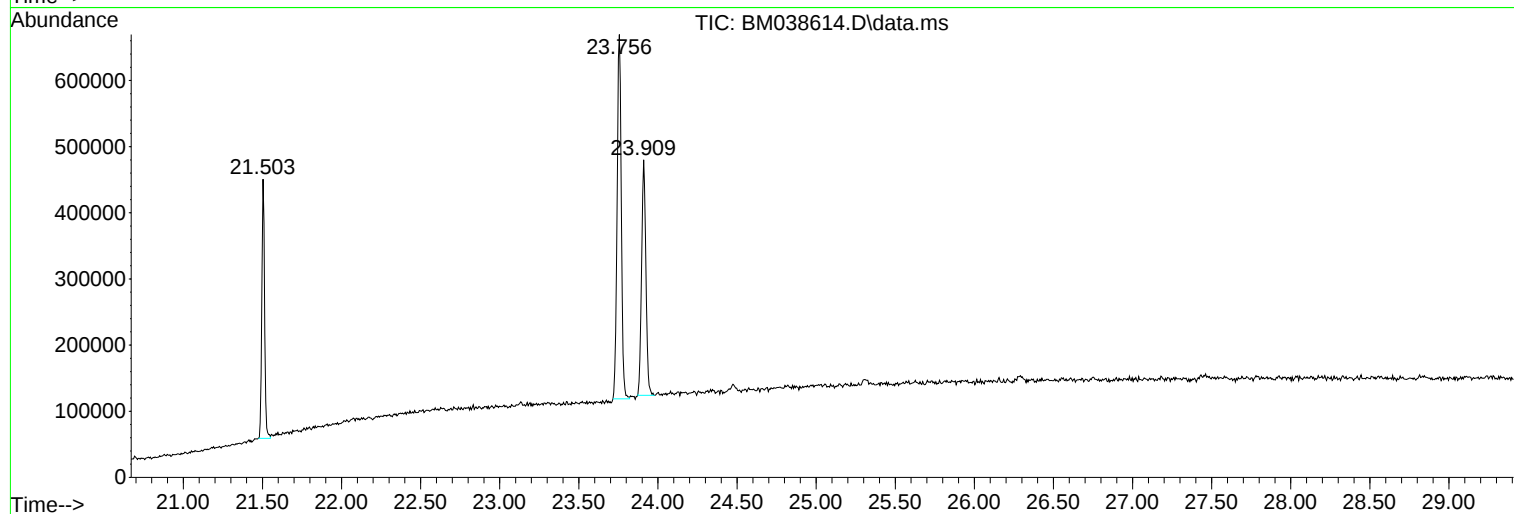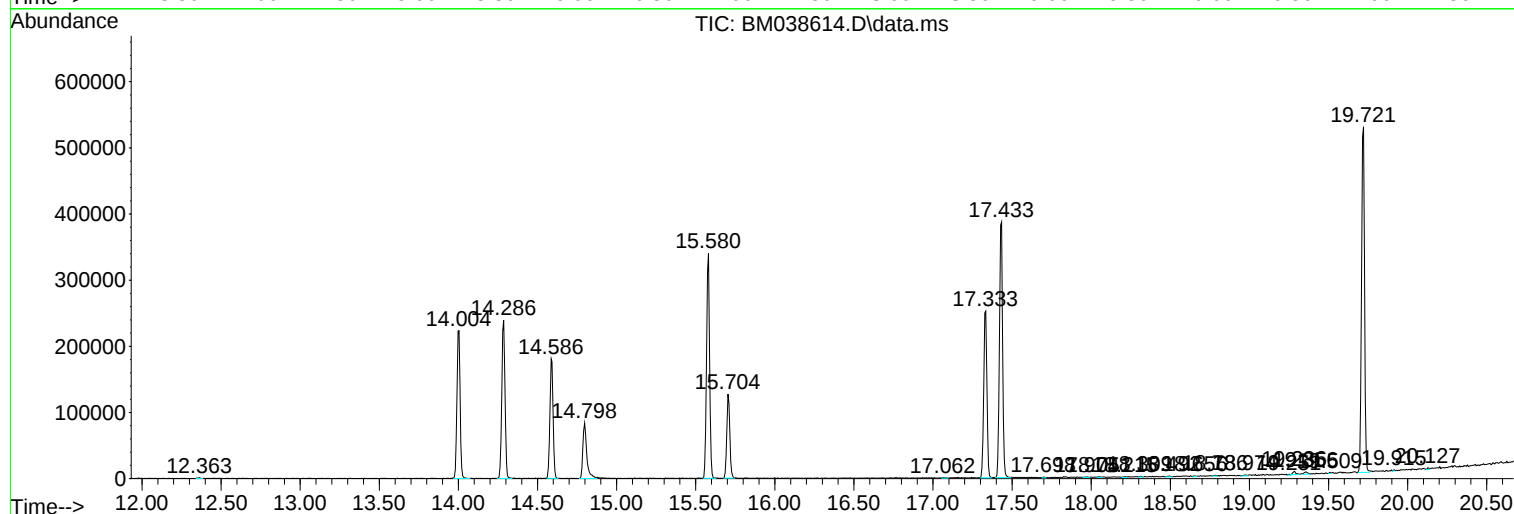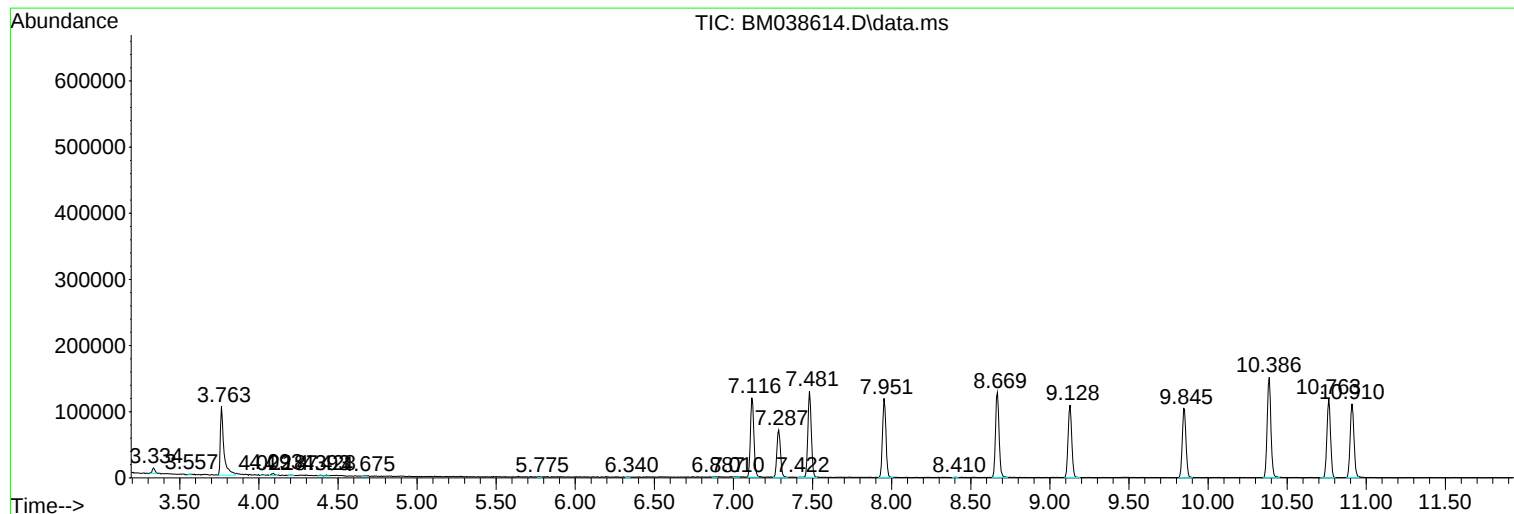

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038614.D
Acq On : 31 Jan 2023 11:45
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038614.D
Acq On : 31 Jan 2023 11:45
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc