

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038619.D
 Acq On : 31 Jan 2023 14:51
 Operator : CG/JU
 Sample : 01311-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	22	25	33	rVB	20671	29569	2.51%	0.245%
2	3.781	98	101	117	rBV	33378	76232	6.47%	0.632%
3	3.946	127	129	131	rVB3	2398	1644	0.14%	0.014%
4	3.987	132	136	141	rVB2	9429	14798	1.26%	0.123%
5	4.087	150	153	158	rVB3	7014	9245	0.78%	0.077%
6	4.587	237	238	241	rVB3	1767	1234	0.10%	0.010%
7	5.045	312	316	322	rVB	11058	16168	1.37%	0.134%
8	5.093	322	324	327	rVB3	2005	1412	0.12%	0.012%
9	5.334	364	365	368	rBV2	1014	1338	0.11%	0.011%
10	5.675	421	423	425	rVB3	1350	1198	0.10%	0.010%
11	5.945	468	469	472	rBV3	1195	1269	0.11%	0.011%
12	6.092	493	494	497	rBV3	1141	1298	0.11%	0.011%
13	6.251	517	521	524	rVB4	989	1447	0.12%	0.012%
14	6.298	526	529	532	rVB3	1087	1231	0.10%	0.010%
15	6.640	584	587	588	rBV3	1948	2097	0.18%	0.017%
16	6.687	594	595	598	rBV3	1509	1433	0.12%	0.012%
17	6.728	598	602	604	rVV4	1191	1725	0.15%	0.014%
18	7.045	652	656	662	rVV	7469	11929	1.01%	0.099%
19	7.092	662	664	665	rVV2	2944	2285	0.19%	0.019%
20	7.116	665	668	675	rVB	53380	83646	7.10%	0.693%
21	7.287	691	697	706	rVB	88569	134749	11.44%	1.116%
22	7.481	724	730	737	rVV	116347	177372	15.05%	1.469%
23	7.951	804	810	818	rBV	154870	235775	20.01%	1.953%
24	8.669	926	932	939	rBV2	82064	127532	10.82%	1.057%
25	9.128	1004	1010	1024	rBV	157175	246868	20.95%	2.045%
26	9.498	1066	1073	1079	rVB2	12871	18708	1.59%	0.155%
27	9.851	1126	1133	1141	rVB	138687	228449	19.39%	1.893%
28	10.269	1202	1204	1209	rBV2	780	1529	0.13%	0.013%
29	10.386	1217	1224	1232	rBV	176521	294397	24.99%	2.439%
30	10.669	1268	1272	1279	rBV4	2929	6386	0.54%	0.053%
31	10.763	1282	1288	1295	rBV	408199	610320	51.80%	5.056%
32	10.910	1306	1313	1326	rBV	253219	457044	38.79%	3.786%
33	11.986	1491	1496	1500	rVB3	3360	4946	0.42%	0.041%
34	12.092	1511	1514	1519	rVB4	1180	2078	0.18%	0.017%
35	12.163	1524	1526	1530	rVB4	1303	1285	0.11%	0.011%
36	12.233	1535	1538	1542	rVB6	1199	2053	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038619.D
 Acq On : 31 Jan 2023 14:51
 Operator : CG/JU
 Sample : 01311-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	12.345	1554	1557	1564	rBV3	4686	7777	0.66%	0.064%
38	13.110	1684	1687	1689	rBV4	1080	1506	0.13%	0.012%
39	13.192	1696	1701	1705	rBV5	904	1849	0.16%	0.015%
40	13.398	1730	1736	1741	rBV5	3412	4046	0.34%	0.034%
41	13.963	1829	1832	1833	rBV	1645	1506	0.13%	0.012%
42	14.004	1833	1839	1848	rVV	576382	788482	66.92%	6.532%
43	14.286	1880	1887	1896	rBV	664902	961114	81.58%	7.962%
44	14.586	1931	1938	1950	rBV	531208	762956	64.76%	6.321%
45	14.804	1970	1975	1987	rBV	28217	65364	5.55%	0.542%
46	14.998	2004	2008	2013	rVB3	2933	4084	0.35%	0.034%
47	15.104	2023	2026	2031	rVB3	3389	4897	0.42%	0.041%
48	15.362	2067	2070	2074	rVB	3049	4071	0.35%	0.034%
49	15.404	2074	2077	2082	rVB5	1110	1253	0.11%	0.010%
50	15.580	2101	2107	2115	rBV	788538	1092125	92.70%	9.048%
51	15.704	2122	2128	2138	rBV	322577	450474	38.23%	3.732%
52	15.821	2145	2148	2153	rVB3	3354	4773	0.41%	0.040%
53	15.945	2165	2169	2175	rVB	41922	55076	4.67%	0.456%
54	16.627	2283	2285	2287	rVB2	1882	1508	0.13%	0.012%
55	16.768	2306	2309	2312	rVB3	1470	1847	0.16%	0.015%
56	17.109	2365	2367	2370	rBV4	1298	1625	0.14%	0.013%
57	17.327	2398	2404	2411	rBV	494921	709652	60.23%	5.879%
58	17.427	2415	2421	2438	rVV	821810	1178187	100.00%	9.761%
59	17.609	2447	2452	2457	rVB4	3578	5869	0.50%	0.049%
60	17.656	2457	2460	2462	rBV4	1586	1852	0.16%	0.015%
61	17.727	2470	2472	2475	rVB4	1581	1558	0.13%	0.013%
62	17.968	2511	2513	2515	rVB2	2718	2628	0.22%	0.022%
63	17.986	2515	2516	2519	rBV3	3144	2012	0.17%	0.017%
64	18.009	2519	2520	2522	rBV2	1850	1926	0.16%	0.016%
65	18.045	2522	2526	2527	rVV3	1190	1384	0.12%	0.011%
66	18.109	2535	2537	2539	rVB3	2028	1425	0.12%	0.012%
67	18.133	2539	2541	2543	rBV3	1230	1361	0.12%	0.011%
68	18.209	2550	2554	2561	rBV3	21624	30602	2.60%	0.254%
69	18.286	2561	2567	2570	rBV3	5326	8218	0.70%	0.068%
70	18.462	2595	2597	2599	rVV2	1746	1813	0.15%	0.015%
71	18.509	2601	2605	2608	rVV4	2090	3206	0.27%	0.027%
72	18.627	2623	2625	2628	rBV3	1531	1315	0.11%	0.011%
73	18.774	2649	2650	2654	rBV4	2430	2881	0.24%	0.024%
74	19.068	2698	2700	2702	rBV3	2245	2190	0.19%	0.018%
75	19.174	2716	2718	2720	rBV2	5715	6942	0.59%	0.058%
76	19.286	2734	2737	2742	rVB7	6584	7960	0.68%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038619.D
 Acq On : 31 Jan 2023 14:51
 Operator : CG/JU
 Sample : 01311-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

77	19.362	2746	2750	2756	rBV4	9542	20172	1.71%	0.167%
78	19.486	2767	2771	2778	rBV8	11992	20186	1.71%	0.167%
79	19.674	2801	2803	2804	rVB	11005	7520	0.64%	0.062%
80	19.721	2804	2811	2815	rBV	624290	759432	64.46%	6.292%
81	19.862	2833	2835	2836	rVB	3526	2311	0.20%	0.019%
82	19.939	2846	2848	2849	rVB	3464	2248	0.19%	0.019%
83	19.968	2851	2853	2854	rVV2	3104	1934	0.16%	0.016%
84	21.503	3109	3114	3121	rBV	381231	467314	39.66%	3.872%
85	23.756	3490	3497	3507	rVB	582749	1071970	90.98%	8.881%
86	23.915	3517	3524	3531	rBV2	312520	617744	52.43%	5.118%
87	26.156	3903	3905	3908	rVB2	36678	35087	2.98%	0.291%
88	26.185	3908	3910	3914	rBV2	31527	35825	3.04%	0.297%
89	26.250	3919	3921	3923	rBV2	29618	28820	2.45%	0.239%


Sum of corrected areas: 12070566

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038619.D
Acq On : 31 Jan 2023 14:51
Operator : CG/JU
Sample : 01311-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

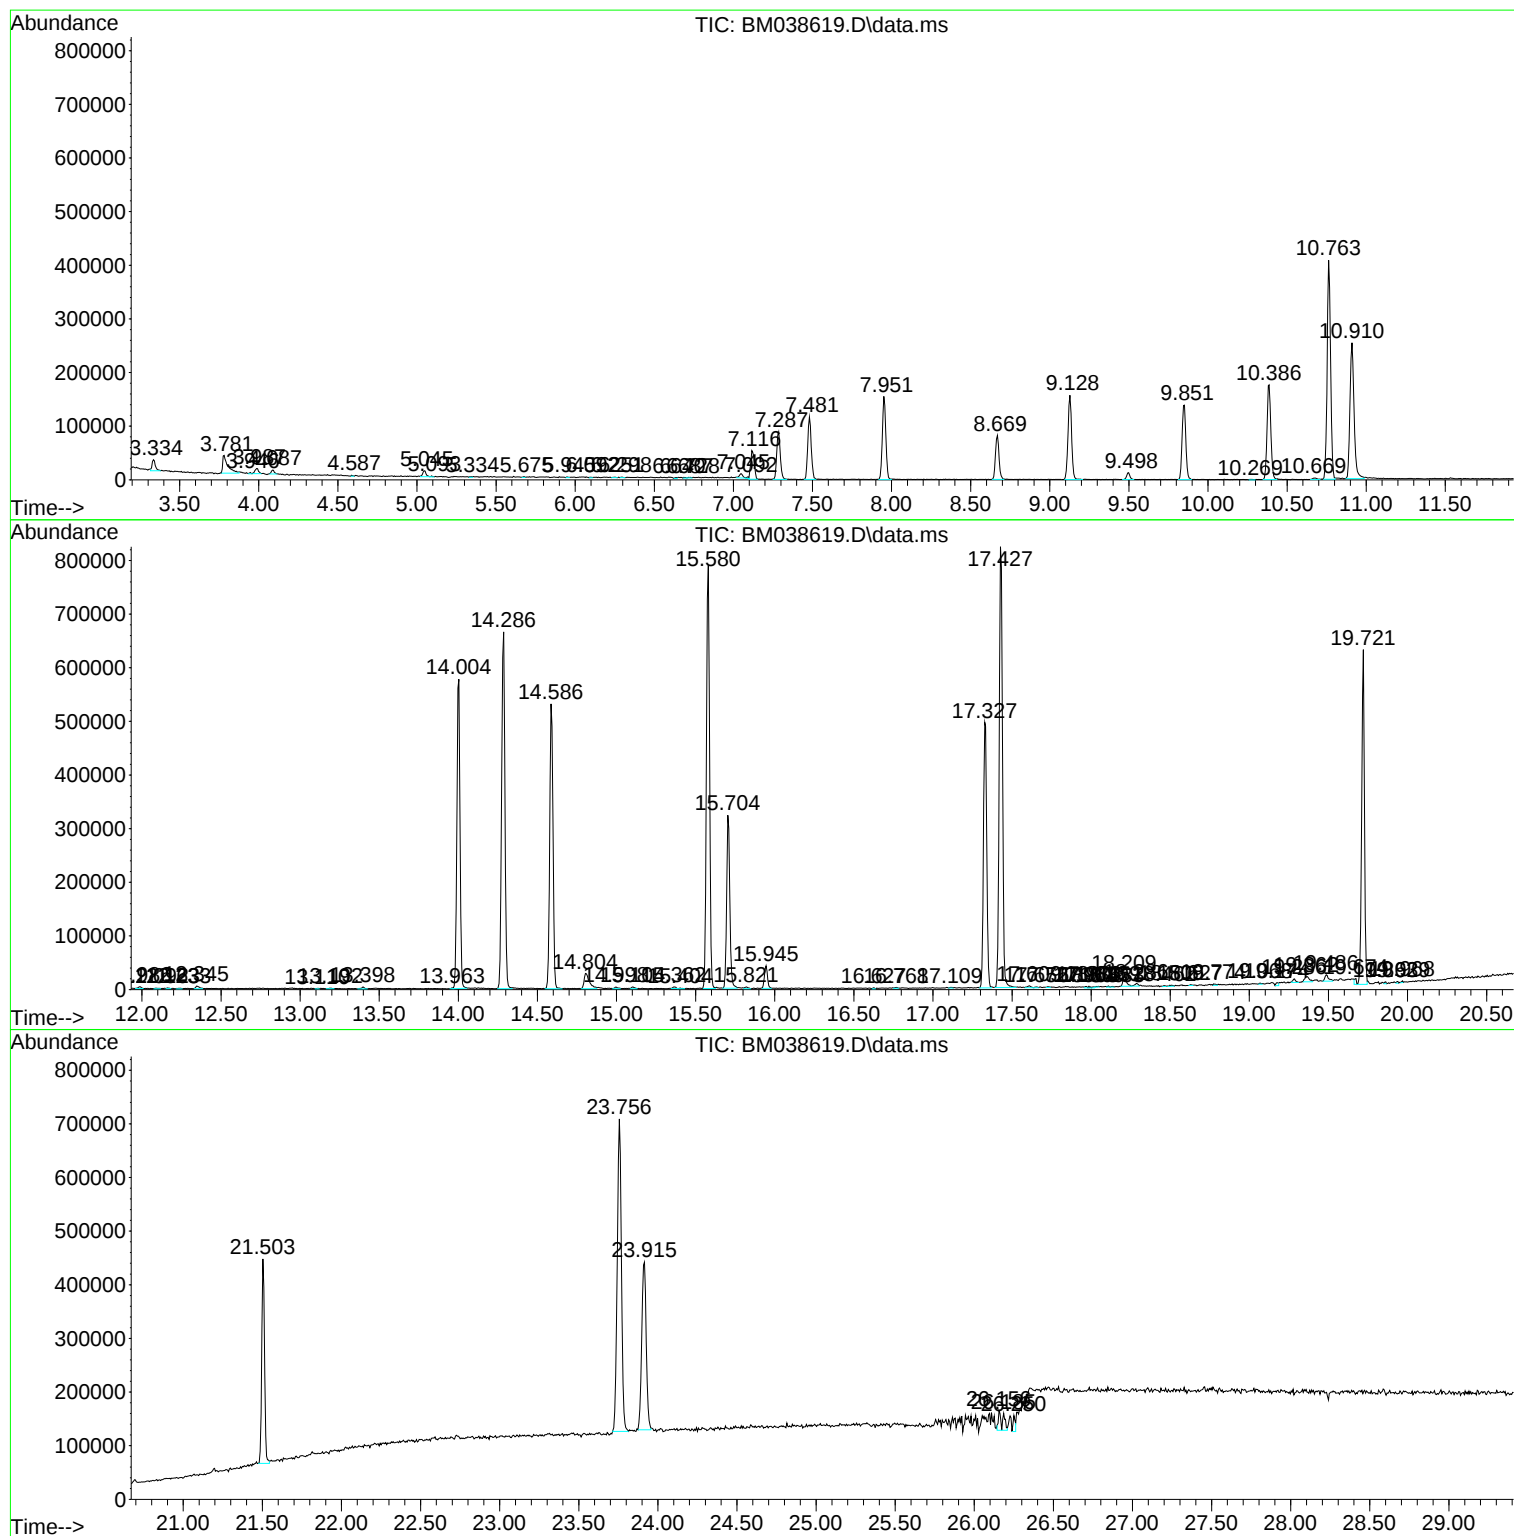

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038619.D
Acq On : 31 Jan 2023 14:51
Operator : CG/JU
Sample : 01311-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038619.D
Acq On : 31 Jan 2023 14:51
Operator : CG/JU
Sample : 01311-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc