

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038620.D
 Acq On : 31 Jan 2023 15:28
 Operator : CG/JU
 Sample : 01311-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	22	25	32	rVB	21575	27297	2.48%	0.248%
2	3.775	96	100	115	rBV	61359	123015	11.17%	1.116%
3	3.987	132	136	142	rVB	11740	18393	1.67%	0.167%
4	4.087	149	153	160	rVB2	10247	13919	1.26%	0.126%
5	4.316	190	192	193	rBV2	1747	1309	0.12%	0.012%
6	4.928	294	296	298	rVB2	1546	1324	0.12%	0.012%
7	5.046	312	316	322	rVB	16076	23608	2.14%	0.214%
8	5.157	334	335	338	rBV2	1448	1602	0.15%	0.015%
9	5.210	341	344	346	rBV3	1687	2336	0.21%	0.021%
10	5.252	350	351	355	rBV3	1151	1375	0.12%	0.012%
11	5.428	379	381	383	rBV3	1386	1247	0.11%	0.011%
12	6.081	490	492	495	rBV3	1311	1597	0.15%	0.014%
13	6.122	495	499	503	rVB5	2216	3794	0.34%	0.034%
14	6.193	509	511	513	rBV3	2222	2608	0.24%	0.024%
15	6.328	531	534	535	rBV2	2014	2218	0.20%	0.020%
16	6.375	539	542	544	rBV3	802	1231	0.11%	0.011%
17	6.487	560	561	564	rBV2	1413	1339	0.12%	0.012%
18	6.699	595	597	598	rBV	1544	1179	0.11%	0.011%
19	7.022	649	652	653	rBV3	1008	1137	0.10%	0.010%
20	7.051	653	657	661	rVV4	3956	6241	0.57%	0.057%
21	7.116	661	668	682	rVB	71962	118816	10.79%	1.078%
22	7.287	690	697	708	rBV	260187	400901	36.42%	3.636%
23	7.481	723	730	740	rBV	285361	441344	40.09%	4.003%
24	7.551	740	742	744	rVB3	2757	2103	0.19%	0.019%
25	7.834	787	790	792	rBV3	1467	1625	0.15%	0.015%
26	7.951	804	810	817	rBV	269779	422198	38.35%	3.829%
27	8.016	817	821	822	rVB3	4942	5548	0.50%	0.050%
28	8.163	842	846	847	rVB2	1144	1176	0.11%	0.011%
29	8.222	847	856	858	rBV3	725	1446	0.13%	0.013%
30	8.440	891	893	896	rVV2	922	1237	0.11%	0.011%
31	8.563	911	914	915	rVB2	1674	1209	0.11%	0.011%
32	8.575	915	916	920	rBV	1002	1278	0.12%	0.012%
33	8.657	926	930	942	rBV2	80767	120675	10.96%	1.094%
34	8.963	978	982	983	rBV3	1206	1410	0.13%	0.013%
35	8.981	983	985	987	rVB	1520	1376	0.12%	0.012%
36	9.016	987	991	992	rBV2	1113	1521	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038620.D
 Acq On : 31 Jan 2023 15:28
 Operator : CG/JU
 Sample : 01311-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	9.063	995	999	1000	rBV2	2207	2860	0.26%	0.026%
38	9.128	1003	1010	1023	rVV	325530	532456	48.37%	4.829%
39	9.498	1068	1073	1079	rVB	11945	18110	1.65%	0.164%
40	9.845	1125	1132	1145	rVV	271125	459006	41.69%	4.163%
41	9.945	1147	1149	1154	rVB4	1385	1941	0.18%	0.018%
42	10.034	1162	1164	1166	rBV3	945	1147	0.10%	0.010%
43	10.381	1217	1223	1237	rVV	335099	574676	52.20%	5.212%
44	10.675	1269	1273	1275	rVV3	1156	1424	0.13%	0.013%
45	10.763	1281	1288	1295	rBV	312123	511560	46.47%	4.640%
46	10.910	1306	1313	1330	rBV	306449	538819	48.94%	4.887%
47	11.216	1362	1365	1368	rVB3	1222	1554	0.14%	0.014%
48	11.363	1389	1390	1395	rBV4	883	1423	0.13%	0.013%
49	11.881	1473	1478	1483	rBV4	1397	2572	0.23%	0.023%
50	11.992	1494	1497	1501	rVB2	2279	2320	0.21%	0.021%
51	12.351	1552	1558	1566	rBV3	4615	9008	0.82%	0.082%
52	12.716	1614	1620	1623	rBV4	935	1874	0.17%	0.017%
53	12.969	1658	1663	1664	rBV2	1695	2234	0.20%	0.020%
54	12.981	1664	1665	1670	rVB2	1483	1727	0.16%	0.016%
55	13.033	1672	1674	1676	rBV2	1182	1274	0.12%	0.012%
56	13.439	1741	1743	1746	rVB2	2046	1759	0.16%	0.016%
57	13.486	1750	1751	1754	rBV3	1338	1464	0.13%	0.013%
58	13.998	1827	1838	1848	rBV	552933	769804	69.93%	6.982%
59	14.069	1848	1850	1854	rVV2	1452	1818	0.17%	0.016%
60	14.139	1856	1862	1864	rVV4	2249	3873	0.35%	0.035%
61	14.286	1880	1887	1897	rBV	638912	950573	86.35%	8.621%
62	14.586	1932	1938	1946	rVB	421121	594517	54.00%	5.392%
63	14.804	1969	1975	1985	rVV3	31025	71298	6.48%	0.647%
64	14.880	1987	1988	1990	rVV	3019	1632	0.15%	0.015%
65	14.898	1990	1991	1994	rVB2	1231	1138	0.10%	0.010%
66	15.363	2068	2070	2074	rBV	836	1106	0.10%	0.010%
67	15.580	2101	2107	2114	rBV	326932	435081	39.52%	3.946%
68	15.704	2123	2128	2137	rBV	124465	167502	15.22%	1.519%
69	16.769	2305	2309	2314	rVB3	913	1644	0.15%	0.015%
70	17.327	2399	2404	2410	rBV	195449	256084	23.26%	2.323%
71	17.427	2415	2421	2431	rVV	398580	522827	47.49%	4.742%
72	18.210	2551	2554	2557	rVB2	1791	2078	0.19%	0.019%
73	18.292	2564	2568	2571	rVV	1952	2183	0.20%	0.020%
74	18.339	2574	2576	2578	rBV	1277	1201	0.11%	0.011%
75	18.533	2606	2609	2611	rVB2	1334	1138	0.10%	0.010%
76	18.592	2617	2619	2620	rVB2	2411	1154	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038620.D
 Acq On : 31 Jan 2023 15:28
 Operator : CG/JU
 Sample : 01311-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

77	18.721	2637	2641	2643	rBV3	1022	1559	0.14%	0.014%
78	18.774	2648	2650	2654	rBV4	1600	2547	0.23%	0.023%
79	19.286	2733	2737	2742	rVB4	3844	5114	0.46%	0.046%
80	19.357	2744	2749	2754	rVV2	3808	6640	0.60%	0.060%
81	19.398	2754	2756	2759	rVV3	1274	1252	0.11%	0.011%
82	19.486	2769	2771	2774	rBV4	2643	2699	0.25%	0.024%
83	19.574	2784	2786	2792	rBV5	1464	2795	0.25%	0.025%
84	19.715	2805	2810	2817	rBV	569330	725350	65.89%	6.578%
85	19.974	2852	2854	2855	rBV2	2143	1908	0.17%	0.017%
86	20.262	2901	2903	2906	rBV4	2915	2429	0.22%	0.022%
87	20.580	2955	2957	2958	rBV	3288	1896	0.17%	0.017%
88	20.692	2974	2976	2979	rVB4	7716	5697	0.52%	0.052%
89	21.503	3109	3114	3121	rBV	312812	395031	35.88%	3.583%
90	23.756	3490	3497	3507	rBV2	589621	1100881	100.00%	9.984%
91	23.915	3517	3524	3531	rBV2	279498	553883	50.31%	5.023%


Sum of corrected areas: 11026172

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038620.D
Acq On : 31 Jan 2023 15:28
Operator : CG/JU
Sample : 01311-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

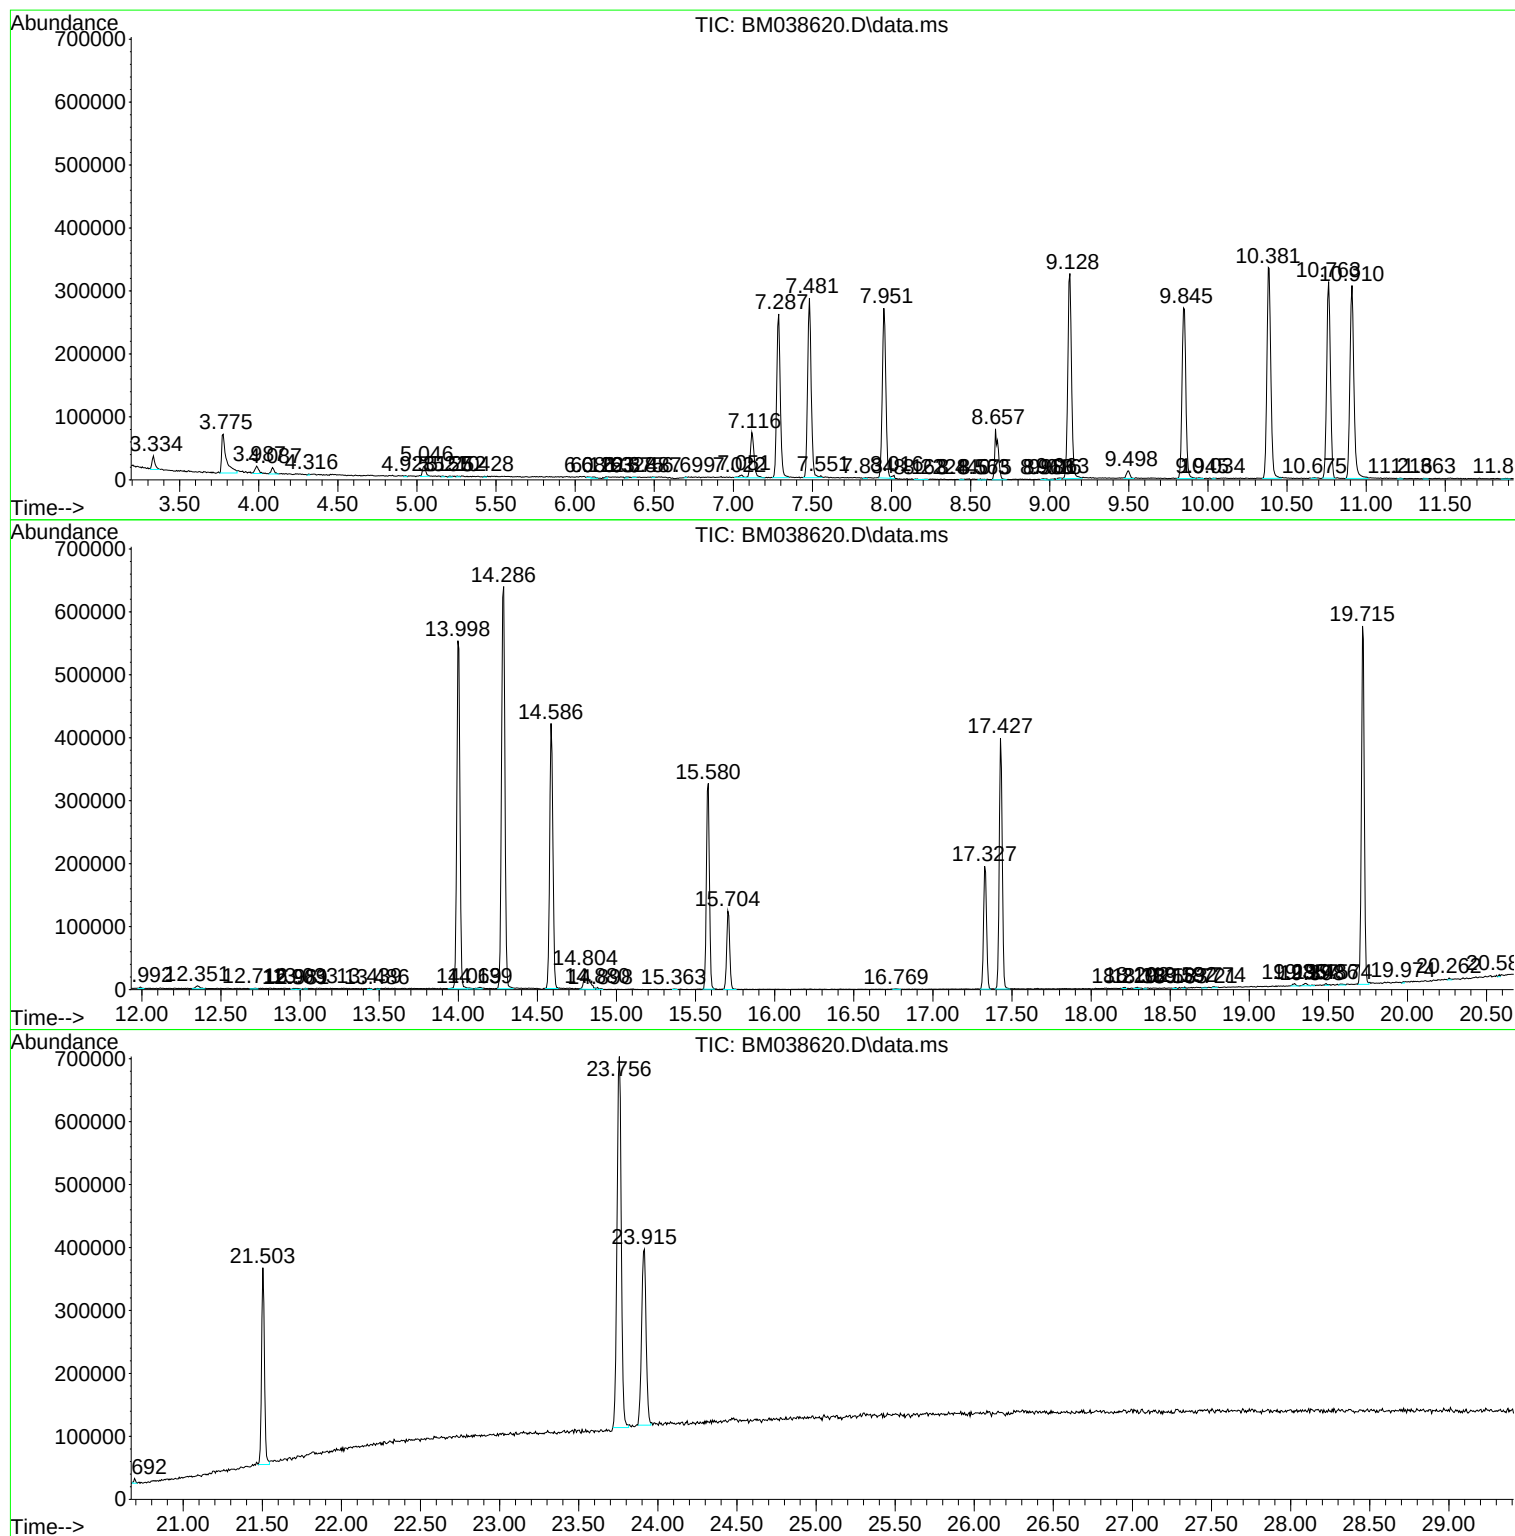

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038620.D
Acq On : 31 Jan 2023 15:28
Operator : CG/JU
Sample : 01311-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038620.D
Acq On : 31 Jan 2023 15:28
Operator : CG/JU
Sample : 01311-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc