

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038622.D
 Acq On : 31 Jan 2023 16:42
 Operator : CG/JU
 Sample : PB150488BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	12	14	16	rBV3	1443	1568	0.13%	0.017%
2	3.334	21	25	33	rVB4	11042	15728	1.34%	0.170%
3	3.622	72	74	76	rBV2	1283	1644	0.14%	0.018%
4	3.763	95	98	114	rBV	132625	203271	17.29%	2.193%
5	4.081	149	152	158	rVB3	3035	4592	0.39%	0.050%
6	4.281	182	186	187	rBV4	1042	1189	0.10%	0.013%
7	4.469	215	218	222	rVV5	1189	1747	0.15%	0.019%
8	4.710	256	259	262	rBV5	1359	1612	0.14%	0.017%
9	4.998	306	308	312	rVB4	1112	1251	0.11%	0.013%
10	6.028	480	483	487	rBV2	1453	1953	0.17%	0.021%
11	6.287	524	527	532	rVB4	1269	1594	0.14%	0.017%
12	6.710	596	599	605	rBV3	993	1563	0.13%	0.017%
13	6.881	624	628	633	rVB2	1154	1409	0.12%	0.015%
14	7.116	662	668	677	rVV2	159187	239985	20.41%	2.589%
15	7.287	690	697	706	rBV	96576	147659	12.56%	1.593%
16	7.481	724	730	737	rBV	169672	258042	21.95%	2.784%
17	7.951	803	810	817	rBV	158616	238706	20.30%	2.575%
18	8.669	926	932	943	rBV	168726	269679	22.94%	2.909%
19	9.128	1003	1010	1020	rBV	146493	228249	19.41%	2.462%
20	9.845	1125	1132	1142	rVB2	141371	227116	19.32%	2.450%
21	10.386	1217	1224	1232	rBV	200099	327614	27.86%	3.535%
22	10.763	1281	1288	1297	rVB	161367	250908	21.34%	2.707%
23	10.910	1306	1313	1327	rBV	150418	253335	21.55%	2.733%
24	12.357	1554	1559	1565	rVB3	1192	2049	0.17%	0.022%
25	13.998	1833	1838	1849	rVB	306590	400968	34.10%	4.326%
26	14.286	1880	1887	1897	rBV	315906	445759	37.91%	4.809%
27	14.586	1933	1938	1946	rVB	238192	329218	28.00%	3.552%
28	14.798	1968	1974	1991	rBV	110172	189001	16.07%	2.039%
29	15.580	2100	2107	2113	rBV	442042	589019	50.09%	6.355%
30	15.704	2123	2128	2136	rBV	160675	213857	18.19%	2.307%
31	15.815	2143	2147	2151	rVB2	1398	1495	0.13%	0.016%
32	17.121	2366	2369	2373	rBV2	925	1251	0.11%	0.013%
33	17.333	2399	2405	2413	rVB	302742	421180	35.82%	4.544%
34	17.427	2415	2421	2431	rBV2	483779	660497	56.17%	7.126%
35	17.639	2455	2457	2461	rBV3	1052	1611	0.14%	0.017%
36	18.392	2581	2585	2586	rVV3	1219	1448	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038622.D
 Acq On : 31 Jan 2023 16:42
 Operator : CG/JU
 Sample : PB150488BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	18.433	2588	2592	2594	rVB3	1212	1698	0.14%	0.018%
38	18.686	2633	2635	2639	rVB4	1095	1217	0.10%	0.013%
39	18.756	2646	2647	2649	rBV	1968	1553	0.13%	0.017%
40	18.968	2680	2683	2685	rBV2	1169	1308	0.11%	0.014%
41	19.286	2733	2737	2740	rBV4	4826	8046	0.68%	0.087%
42	19.356	2745	2749	2753	rVV3	4708	6353	0.54%	0.069%
43	19.574	2782	2786	2787	rBV4	1785	2408	0.20%	0.026%
44	19.721	2805	2811	2818	rVB	625183	819386	69.69%	8.840%
45	21.503	3109	3114	3121	rBV	457567	553332	47.06%	5.970%
46	23.756	3490	3497	3509	rBV2	630969	1175810	100.00%	12.685%
47	23.909	3517	3523	3535	rVB2	376313	760118	64.65%	8.201%




Sum of corrected areas: 9268996

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038622.D
Acq On : 31 Jan 2023 16:42
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

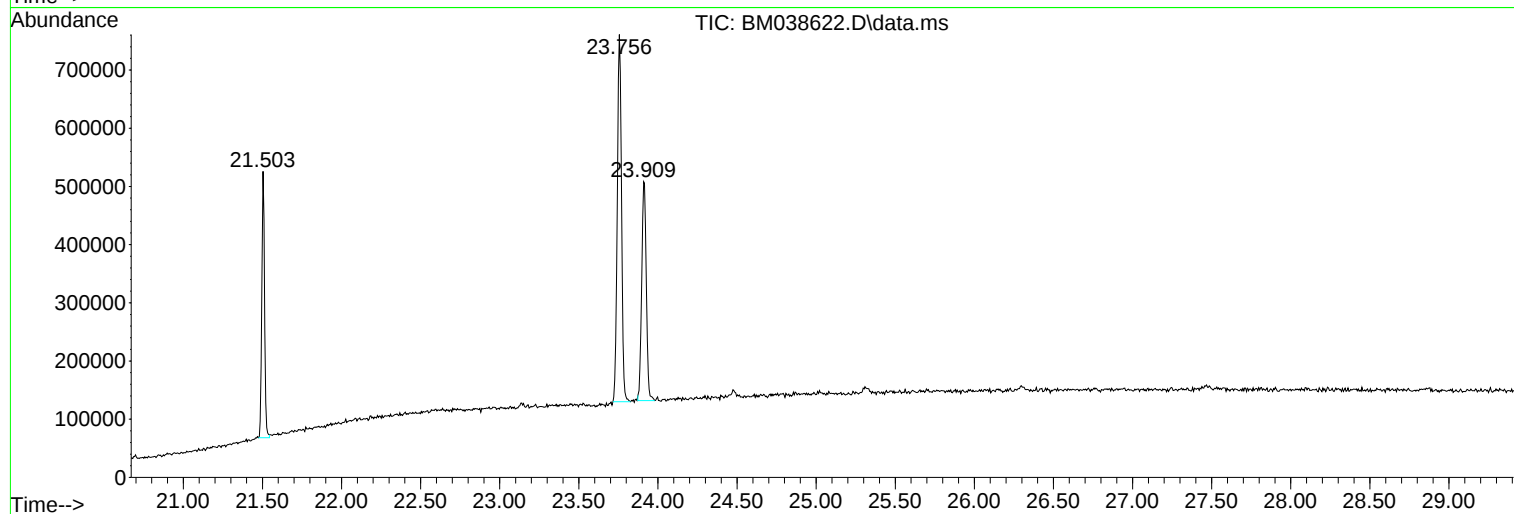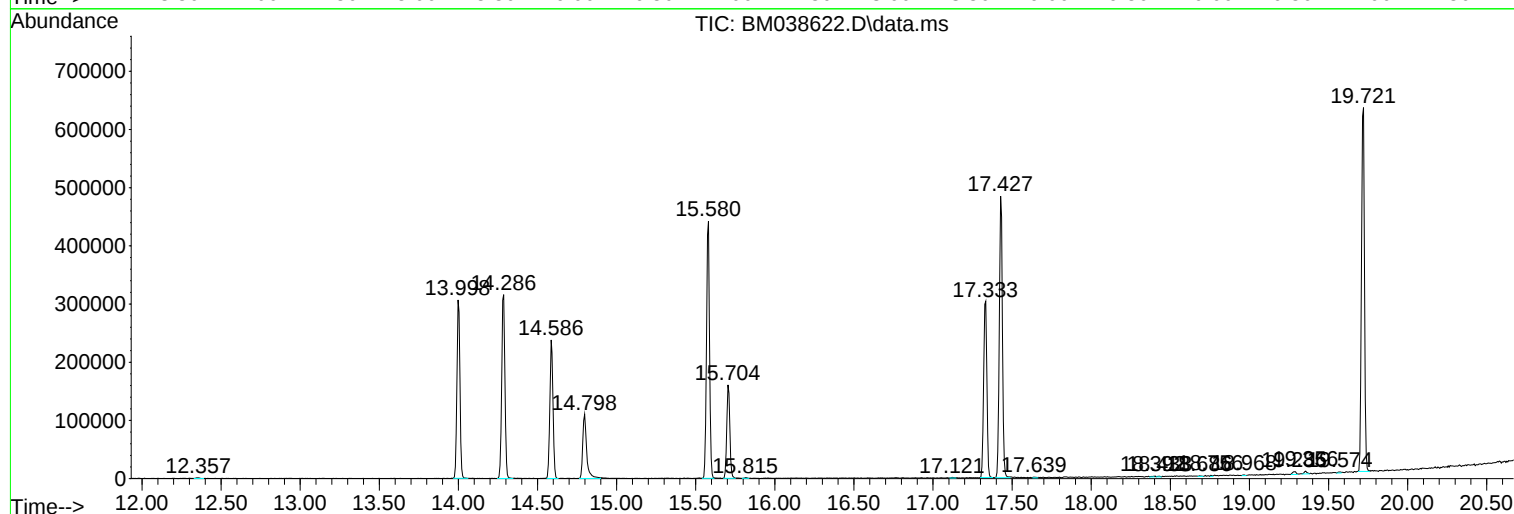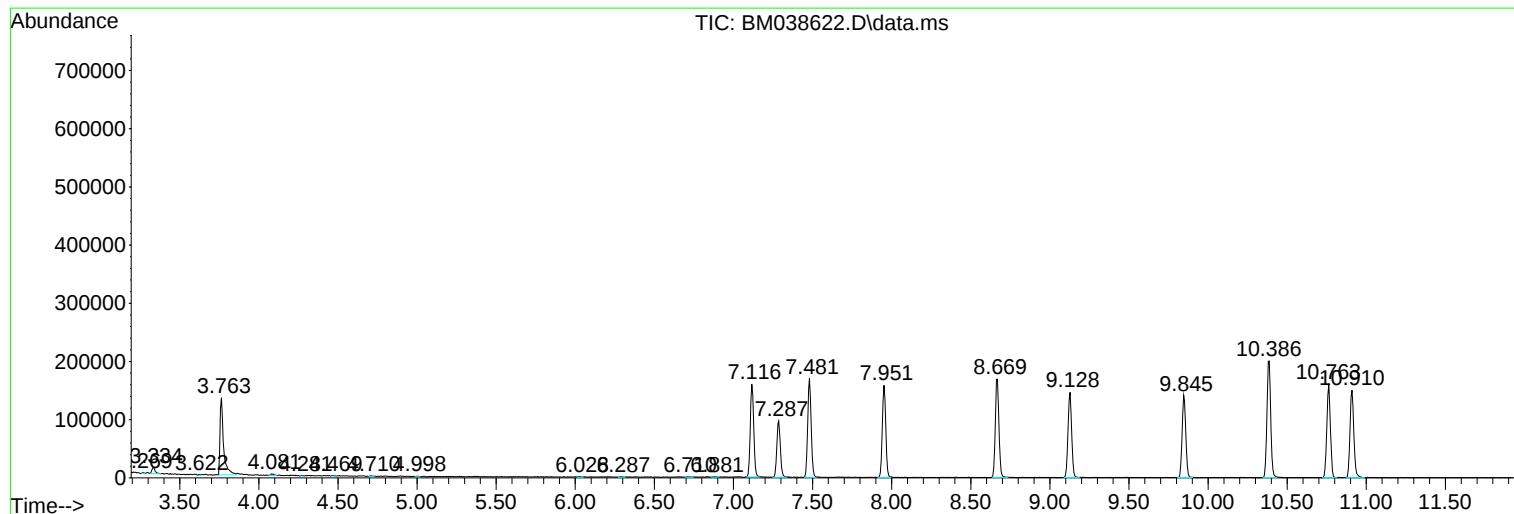

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038622.D
Acq On : 31 Jan 2023 16:42
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038622.D
Acq On : 31 Jan 2023 16:42
Operator : CG/JU
Sample : PB150488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc