

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038625.D
 Acq On : 31 Jan 2023 18:34
 Operator : CG/JU
 Sample : 01311-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	22	25	29	rVB2	9328	10428	0.89%	0.125%
2	3.610	68	72	75	rVB3	1801	2519	0.21%	0.030%
3	3.781	98	101	110	rBV	14677	29315	2.50%	0.353%
4	3.987	132	136	139	rVB3	4308	4861	0.41%	0.058%
5	4.087	148	153	155	rBV3	2867	3211	0.27%	0.039%
6	4.210	173	174	177	rVB2	1568	1272	0.11%	0.015%
7	4.252	179	181	184	rVB2	1346	1541	0.13%	0.019%
8	5.046	312	316	322	rBV2	4250	5548	0.47%	0.067%
9	5.204	339	343	344	rBV2	1137	1399	0.12%	0.017%
10	7.045	651	656	662	rVB2	7804	10275	0.88%	0.124%
11	7.116	663	668	675	rVB	25192	39560	3.37%	0.476%
12	7.281	689	696	707	rVB	91841	146010	12.43%	1.757%
13	7.481	724	730	738	rBV	119958	185102	15.76%	2.227%
14	7.698	764	767	772	rBV2	811	1321	0.11%	0.016%
15	7.951	804	810	818	rBV	148132	223266	19.01%	2.686%
16	8.010	818	820	825	rVB4	855	1209	0.10%	0.015%
17	8.663	924	931	939	rBV	75540	119972	10.22%	1.443%
18	9.128	1003	1010	1022	rVB	140444	228559	19.47%	2.750%
19	9.498	1067	1073	1077	rVB	12270	17971	1.53%	0.216%
20	9.845	1126	1132	1142	rVB	131970	213064	18.15%	2.563%
21	10.381	1217	1223	1232	rBV	171714	287172	24.46%	3.455%
22	10.669	1267	1272	1276	rBV	4242	6412	0.55%	0.077%
23	10.763	1280	1288	1294	rBV	153198	237216	20.20%	2.854%
24	10.910	1307	1313	1323	rBV	103945	175206	14.92%	2.108%
25	11.980	1493	1495	1501	rVB4	2420	3224	0.27%	0.039%
26	12.339	1554	1556	1563	rBV2	1560	2599	0.22%	0.031%
27	12.739	1620	1624	1628	rBV3	1079	1728	0.15%	0.021%
28	13.998	1833	1838	1848	rVB	316524	413873	35.25%	4.979%
29	14.280	1880	1886	1893	rBV	321369	456174	38.85%	5.488%
30	14.586	1932	1938	1946	rBV	235118	316104	26.92%	3.803%
31	14.804	1969	1975	1985	rBV2	11199	23454	2.00%	0.282%
32	15.098	2023	2025	2029	rBV	857	1193	0.10%	0.014%
33	15.363	2067	2070	2074	rVB2	1071	1276	0.11%	0.015%
34	15.527	2092	2098	2099	rBV2	1103	1426	0.12%	0.017%
35	15.574	2100	2106	2118	rVB	461648	628970	53.57%	7.567%
36	15.704	2123	2128	2135	rBV	173313	226608	19.30%	2.726%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038625.D
 Acq On : 31 Jan 2023 18:34
 Operator : CG/JU
 Sample : 01311-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	15.815	2145	2147	2150	rVB2	1357	1510	0.13%	0.018%
38	15.939	2164	2168	2175	rVB2	16487	23044	1.96%	0.277%
39	16.762	2303	2308	2309	rBV2	1182	1260	0.11%	0.015%
40	17.327	2399	2404	2415	rVB	288565	377676	32.16%	4.544%
41	17.427	2415	2421	2433	rBV	552335	742157	63.21%	8.929%
42	17.839	2489	2491	2493	rVB	1288	1175	0.10%	0.014%
43	18.209	2550	2554	2562	rVB4	6672	8256	0.70%	0.099%
44	18.286	2566	2567	2571	rVB4	1504	1570	0.13%	0.019%
45	18.633	2623	2626	2627	rBV	1872	1314	0.11%	0.016%
46	19.239	2727	2729	2731	rBV3	1328	1177	0.10%	0.014%
47	19.286	2733	2737	2740	rVV4	5744	7696	0.66%	0.093%
48	19.356	2745	2749	2753	rVV3	4517	6684	0.57%	0.080%
49	19.421	2758	2760	2764	rBV5	1524	1393	0.12%	0.017%
50	19.492	2768	2772	2775	rVV5	2932	3879	0.33%	0.047%
51	19.715	2805	2810	2816	rBV	711857	877729	74.75%	10.560%
52	20.692	2974	2976	2979	rVB3	8195	5433	0.46%	0.065%
53	21.503	3109	3114	3120	rBV	371611	457888	39.00%	5.509%
54	23.756	3490	3497	3506	rBV2	627231	1174198	100.00%	14.127%
55	23.909	3517	3523	3532	rVB2	303300	588653	50.13%	7.082%




Sum of corrected areas: 8311730

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038625.D
Acq On : 31 Jan 2023 18:34
Operator : CG/JU
Sample : 01311-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

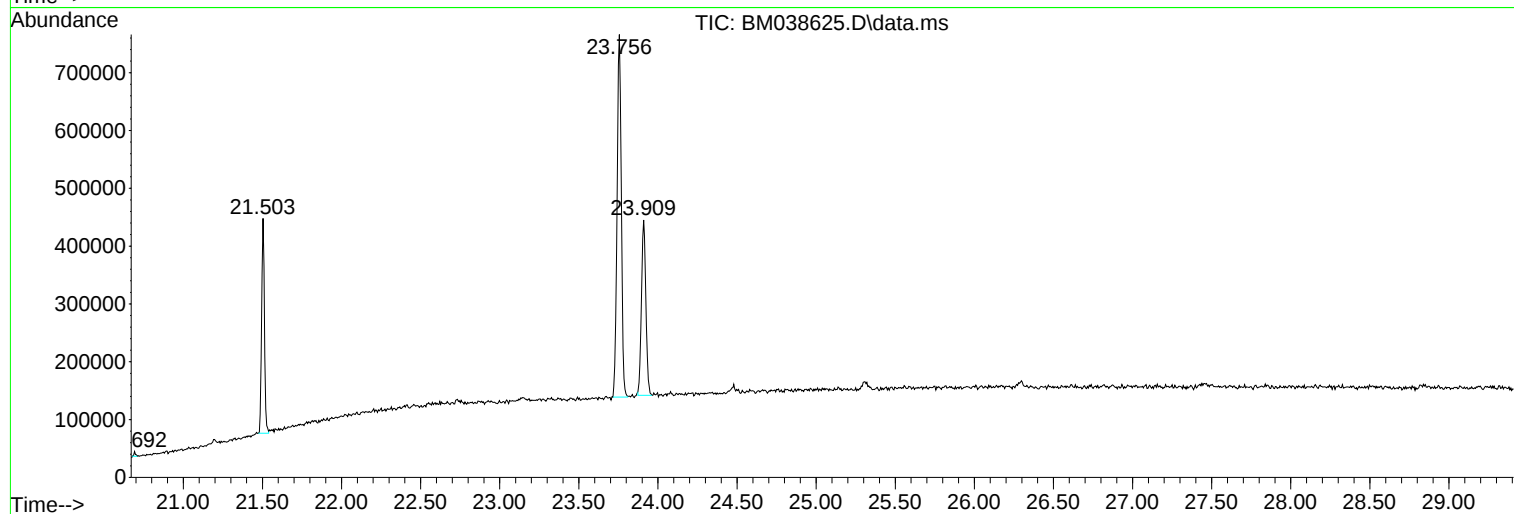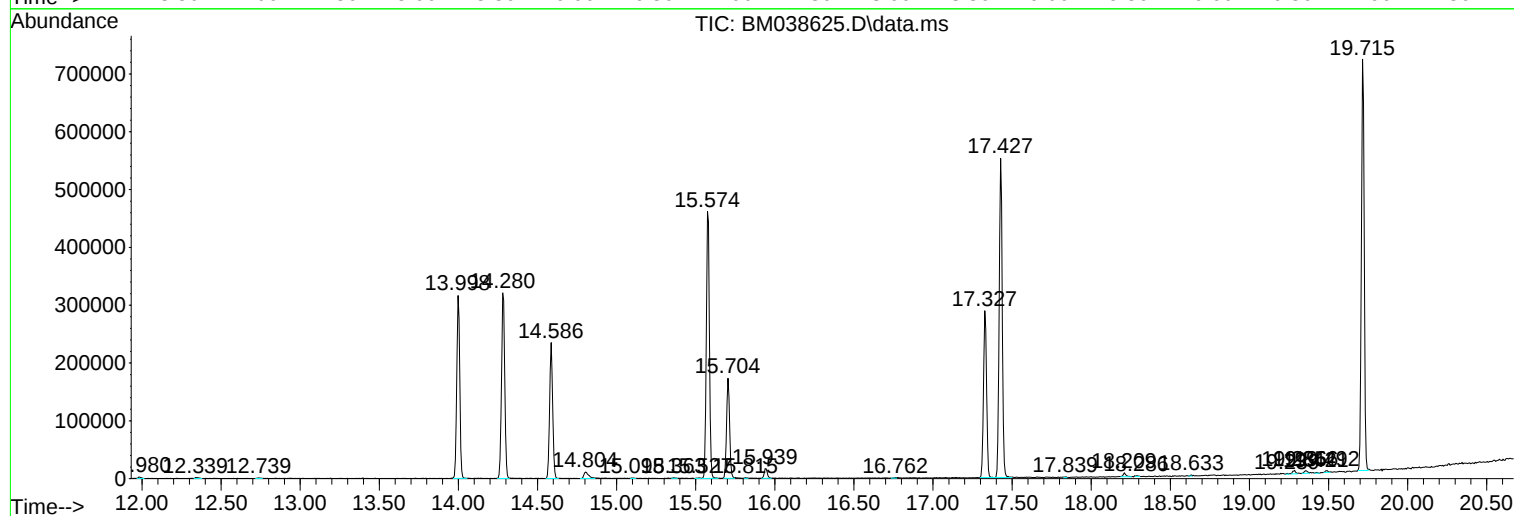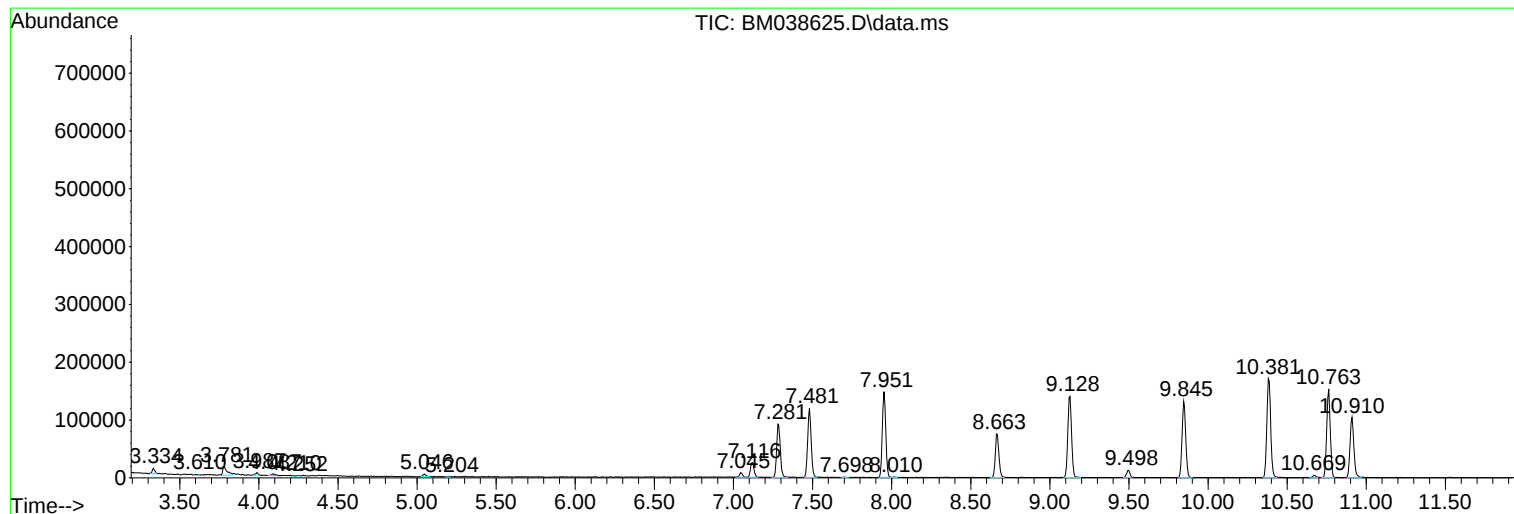

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038625.D
Acq On : 31 Jan 2023 18:34
Operator : CG/JU
Sample : 01311-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038625.D
Acq On : 31 Jan 2023 18:34
Operator : CG/JU
Sample : 01311-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------