

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038626.D
 Acq On : 31 Jan 2023 19:11
 Operator : CG/JU
 Sample : 01311-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	21	24	28	rBV2	5968	8115	0.69%	0.108%
2	3.769	96	99	106	rBV	25118	40233	3.42%	0.534%
3	3.840	109	111	117	rVB5	2252	3551	0.30%	0.047%
4	3.916	122	124	129	rVV3	1377	1978	0.17%	0.026%
5	3.987	129	136	140	rVV3	3671	7619	0.65%	0.101%
6	4.063	146	149	150	rBV3	1674	1611	0.14%	0.021%
7	4.087	150	153	159	rVV4	4016	4343	0.37%	0.058%
8	4.510	223	225	229	rVB3	1298	1691	0.14%	0.022%
9	5.005	305	309	312	rBV2	903	1529	0.13%	0.020%
10	5.046	312	316	321	rVV	5261	7367	0.63%	0.098%
11	5.381	370	373	375	rBV3	1302	1193	0.10%	0.016%
12	5.616	410	413	416	rBV3	1164	1182	0.10%	0.016%
13	5.828	444	449	453	rVB4	856	1640	0.14%	0.022%
14	5.881	453	458	460	rBV2	1191	1787	0.15%	0.024%
15	7.046	652	656	662	rVB2	4353	6568	0.56%	0.087%
16	7.116	662	668	678	rBV	27027	42958	3.66%	0.570%
17	7.281	691	696	706	rVB	89006	136018	11.58%	1.804%
18	7.481	724	730	738	rVB	116314	178275	15.17%	2.364%
19	7.557	740	743	747	rBV2	1011	1488	0.13%	0.020%
20	7.951	804	810	818	rBV	114343	171443	14.59%	2.273%
21	8.663	926	931	939	rBV	70587	112783	9.60%	1.496%
22	9.128	1003	1010	1017	rBV	130831	210067	17.88%	2.786%
23	9.498	1068	1073	1079	rVB2	9083	12903	1.10%	0.171%
24	9.845	1125	1132	1142	rBV	130542	201301	17.13%	2.669%
25	10.381	1216	1223	1236	rBV	162401	268412	22.85%	3.559%
26	10.675	1268	1273	1276	rBV3	1664	2829	0.24%	0.038%
27	10.763	1281	1288	1295	rVB	112043	182494	15.53%	2.420%
28	10.910	1306	1313	1324	rBV	116283	196391	16.72%	2.604%
29	12.345	1554	1557	1562	rVB	1583	2189	0.19%	0.029%
30	13.998	1831	1838	1847	rVB	282633	371278	31.60%	4.923%
31	14.280	1880	1886	1893	rBV	294324	416285	35.43%	5.520%
32	14.586	1932	1938	1946	rVB	171707	236677	20.15%	3.138%
33	14.804	1970	1975	1983	rBV3	11514	22287	1.90%	0.296%
34	15.574	2100	2106	2113	rBV	394545	550351	46.85%	7.298%
35	15.704	2123	2128	2138	rBV	150386	197350	16.80%	2.617%
36	15.816	2144	2147	2150	rVB2	1132	1226	0.10%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038626.D
 Acq On : 31 Jan 2023 19:11
 Operator : CG/JU
 Sample : 01311-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	16.768	2303	2309	2313	rBV2	968	1693	0.14%	0.022%
38	17.327	2399	2404	2414	rBV	227464	301075	25.63%	3.992%
39	17.427	2416	2421	2432	rVV2	495379	641006	54.56%	8.500%
40	17.604	2449	2451	2455	rVB2	1419	1771	0.15%	0.023%
41	18.210	2551	2554	2558	rBV5	2502	2866	0.24%	0.038%
42	18.280	2564	2566	2571	rBV4	1237	1583	0.13%	0.021%
43	18.698	2635	2637	2639	rBV3	1707	1837	0.16%	0.024%
44	18.739	2642	2644	2647	rVV3	1677	1641	0.14%	0.022%
45	18.780	2647	2651	2654	rVV4	2062	3184	0.27%	0.042%
46	18.845	2659	2662	2664	rBV2	991	1461	0.12%	0.019%
47	19.121	2705	2709	2710	rVB3	1637	1689	0.14%	0.022%
48	19.139	2710	2712	2713	rBV2	1947	1554	0.13%	0.021%
49	19.280	2733	2736	2739	rBV5	4535	5994	0.51%	0.079%
50	19.351	2745	2748	2754	rBV3	4315	6828	0.58%	0.091%
51	19.480	2768	2770	2771	rBV2	2347	2065	0.18%	0.027%
52	19.609	2789	2792	2793	rBV2	1915	2120	0.18%	0.028%
53	19.715	2805	2810	2817	rBV	663072	814952	69.37%	10.807%
54	20.692	2974	2976	2979	rBV3	7245	6458	0.55%	0.086%
55	21.503	3109	3114	3120	rBV	345898	408180	34.74%	5.413%
56	23.756	3490	3497	3509	rVB2	611499	1174813	100.00%	15.578%
57	23.909	3517	3523	3531	rBV2	296435	553131	47.08%	7.335%




Sum of corrected areas: 7541313

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038626.D
Acq On : 31 Jan 2023 19:11
Operator : CG/JU
Sample : 01311-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

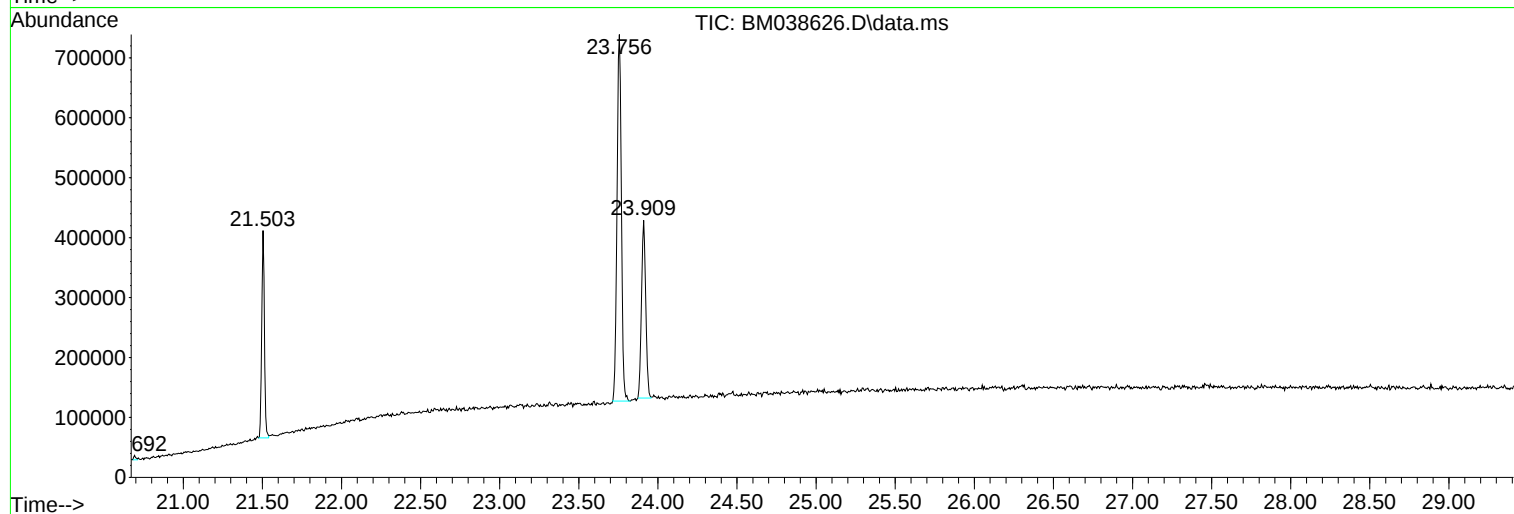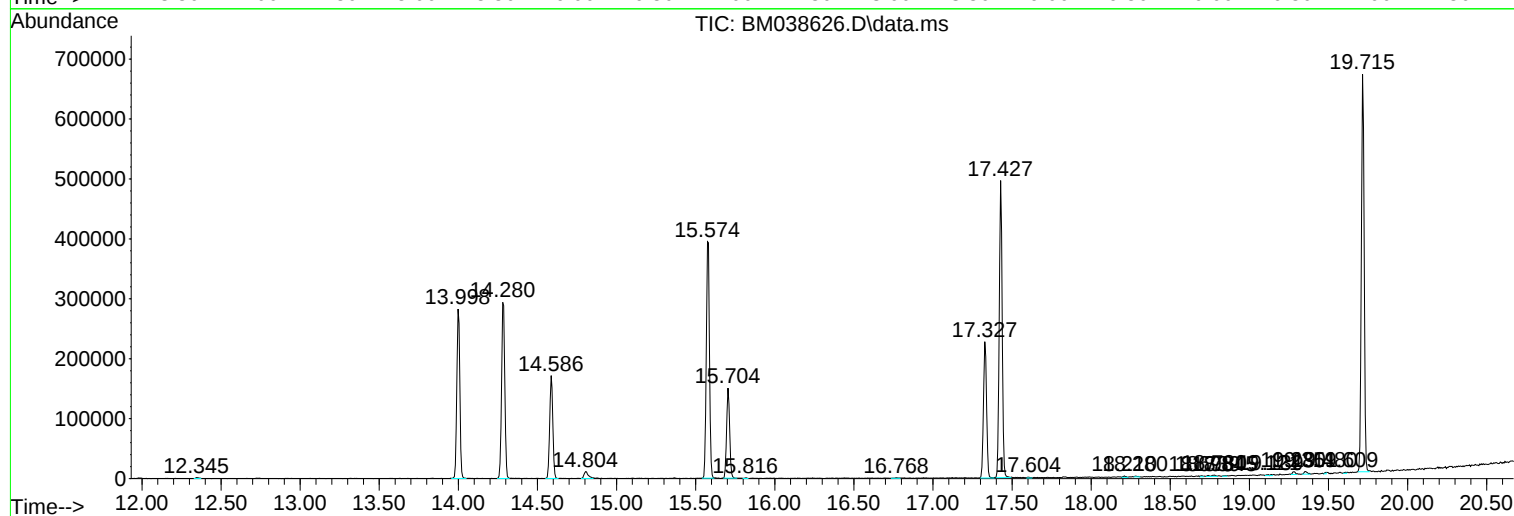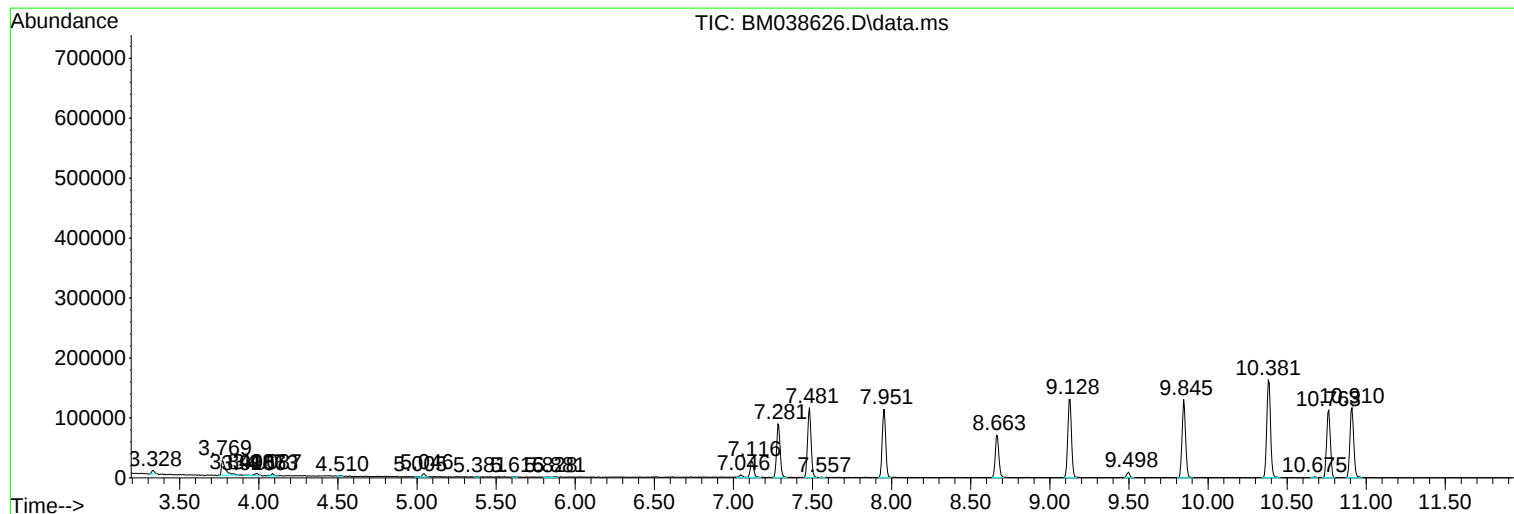

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038626.D
Acq On : 31 Jan 2023 19:11
Operator : CG/JU
Sample : 01311-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038626.D
Acq On : 31 Jan 2023 19:11
Operator : CG/JU
Sample : 01311-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------