

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038627.D
 Acq On : 31 Jan 2023 19:48
 Operator : CG/JU
 Sample : 01311-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	18	20	22	rBV	1512	1527	0.16%	0.020%
2	3.334	22	25	31	rVB	7569	9300	0.99%	0.125%
3	3.769	97	99	113	rBV	19985	42351	4.51%	0.568%
4	3.928	123	126	127	rVB2	1427	1133	0.12%	0.015%
5	3.987	131	136	139	rBV4	3924	6549	0.70%	0.088%
6	4.087	149	153	156	rVB5	2903	3656	0.39%	0.049%
7	4.122	156	159	160	rBV3	771	958	0.10%	0.013%
8	4.199	170	172	176	rVB3	934	1122	0.12%	0.015%
9	4.552	230	232	239	rVB4	1060	1781	0.19%	0.024%
10	4.640	245	247	251	rBV3	934	1176	0.13%	0.016%
11	4.875	285	287	291	rVB2	830	1008	0.11%	0.014%
12	6.275	520	525	527	rBV2	698	1102	0.12%	0.015%
13	7.045	651	656	663	rVB2	2339	3670	0.39%	0.049%
14	7.116	663	668	676	rBV	25858	39017	4.15%	0.523%
15	7.281	690	696	705	rBV	88984	135227	14.40%	1.812%
16	7.481	723	730	740	rVB	114013	175680	18.70%	2.354%
17	7.951	804	810	817	rBV	131776	199113	21.20%	2.668%
18	8.663	926	931	944	rBV	69396	111496	11.87%	1.494%
19	9.122	1003	1009	1017	rBV	132177	213894	22.77%	2.866%
20	9.498	1067	1073	1077	rVB2	5530	8632	0.92%	0.116%
21	9.845	1125	1132	1143	rVB	128589	201357	21.44%	2.698%
22	10.381	1217	1223	1236	rBV	166519	268321	28.57%	3.596%
23	10.763	1280	1288	1294	rBV	132985	219879	23.41%	2.946%
24	10.904	1307	1312	1321	rBV	122224	205566	21.88%	2.755%
25	11.986	1490	1496	1502	rBV2	2552	3472	0.37%	0.047%
26	12.345	1553	1557	1563	rBV3	1580	2335	0.25%	0.031%
27	13.998	1829	1838	1845	rBV	301673	399456	42.53%	5.353%
28	14.280	1880	1886	1895	rBV	309334	431671	45.96%	5.785%
29	14.586	1932	1938	1945	rVB	214638	293003	31.19%	3.926%
30	14.804	1970	1975	1985	rBV3	9194	18490	1.97%	0.248%
31	14.874	1985	1987	1994	rVB	879	1170	0.12%	0.016%
32	15.521	2092	2097	2100	rBV2	823	1374	0.15%	0.018%
33	15.574	2101	2106	2114	rVV	427747	591381	62.96%	7.925%
34	15.704	2123	2128	2136	rBV	149657	196794	20.95%	2.637%
35	15.816	2144	2147	2151	rBV3	938	1093	0.12%	0.015%
36	16.668	2289	2292	2294	rBV2	1060	1093	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038627.D
 Acq On : 31 Jan 2023 19:48
 Operator : CG/JU
 Sample : 01311-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBQM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	16.721	2297	2301	2304	rVV3	667	965	0.10%	0.013%
38	16.986	2341	2346	2349	rBV2	829	1568	0.17%	0.021%
39	17.327	2399	2404	2412	rBV	266513	352943	37.57%	4.730%
40	17.427	2415	2421	2434	rVB	514285	665421	70.84%	8.917%
41	17.598	2449	2450	2455	rVB3	987	1187	0.13%	0.016%
42	18.204	2552	2553	2559	rVB4	1265	1681	0.18%	0.023%
43	18.292	2563	2568	2571	rBV4	1889	2793	0.30%	0.037%
44	18.745	2642	2645	2647	rBV3	1657	1841	0.20%	0.025%
45	19.115	2707	2708	2710	rBV2	1258	1006	0.11%	0.013%
46	19.256	2730	2732	2733	rBV2	1577	1523	0.16%	0.020%
47	19.280	2733	2736	2740	rVV5	5085	6452	0.69%	0.086%
48	19.327	2743	2744	2746	rBV2	2182	1679	0.18%	0.022%
49	19.356	2746	2749	2752	rBV3	4001	4769	0.51%	0.064%
50	19.480	2768	2770	2771	rBV	2283	1645	0.18%	0.022%
51	19.527	2777	2778	2780	rBV2	1474	1178	0.13%	0.016%
52	19.715	2805	2810	2817	rBV	609566	764336	81.37%	10.242%
53	20.239	2898	2899	2902	rBV3	3495	3655	0.39%	0.049%
54	20.380	2921	2923	2927	rBV5	3582	5080	0.54%	0.068%
55	21.503	3110	3114	3123	rBV	314956	393595	41.90%	5.274%
56	23.756	3490	3497	3506	rBV	514486	939333	100.00%	12.587%
57	23.909	3517	3523	3531	rBV	260328	514971	54.82%	6.901%




Sum of corrected areas: 7462468

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038627.D
Acq On : 31 Jan 2023 19:48
Operator : CG/JU
Sample : 01311-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

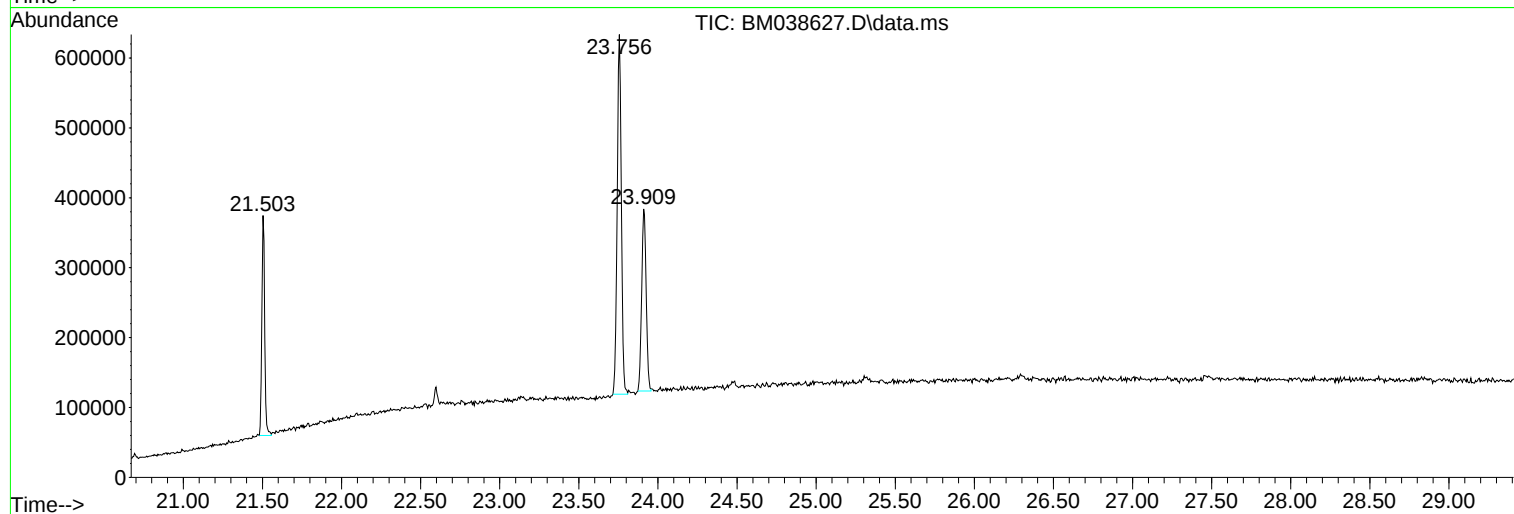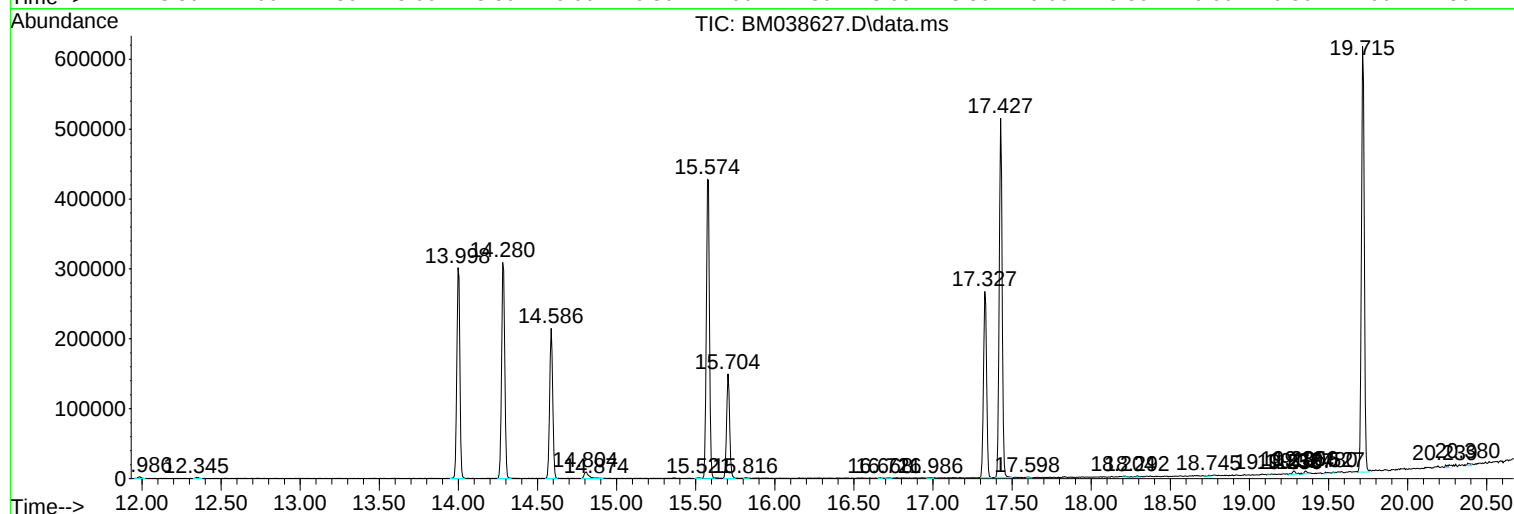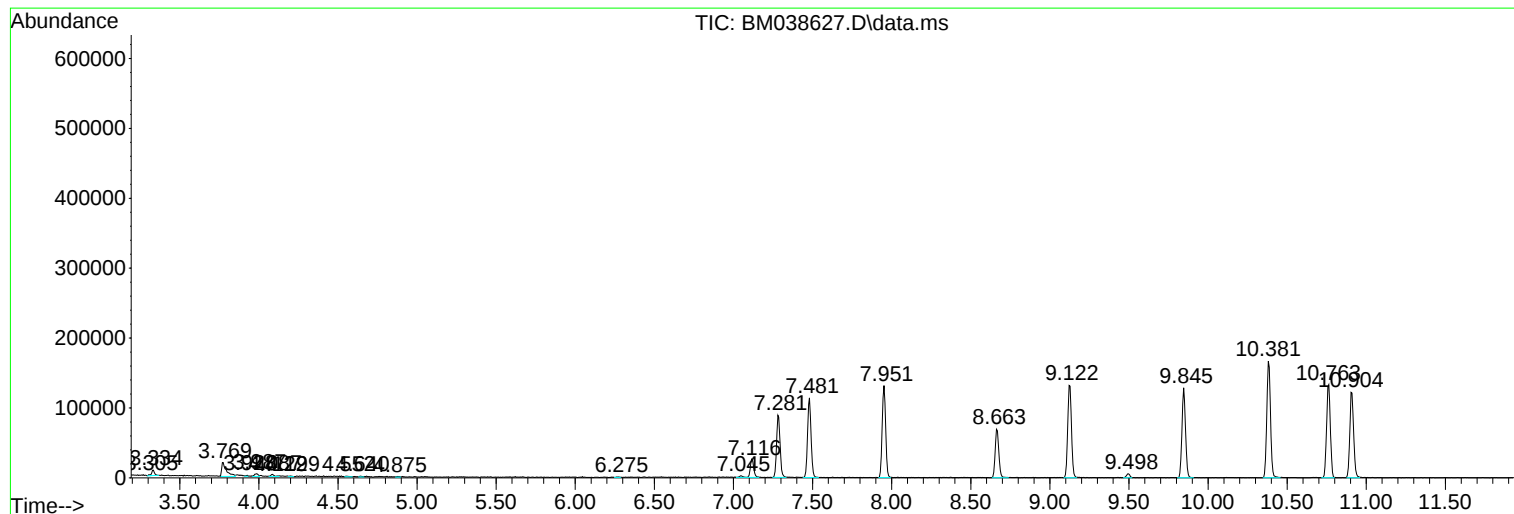

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038627.D
Acq On : 31 Jan 2023 19:48
Operator : CG/JU
Sample : 01311-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038627.D
Acq On : 31 Jan 2023 19:48
Operator : CG/JU
Sample : 01311-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBQM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------