

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038635.D
 Acq On : 01 Feb 2023 00:43
 Operator : CG/JU
 Sample : 01277-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	20	24	32	rVB	10865	14845	1.06%	0.136%
2	3.769	96	99	109	rBV	46918	77722	5.57%	0.710%
3	3.987	129	136	143	rVB2	6664	10750	0.77%	0.098%
4	4.087	150	153	155	rBV2	3192	3752	0.27%	0.034%
5	4.651	244	249	252	rBV2	1051	1594	0.11%	0.015%
6	4.881	283	288	290	rVB3	1179	1894	0.14%	0.017%
7	4.904	290	292	295	rBV3	1107	1628	0.12%	0.015%
8	5.046	309	316	324	rVB3	3976	6941	0.50%	0.063%
9	7.051	654	657	662	rBV4	1426	1458	0.10%	0.013%
10	7.116	662	668	678	rVB2	47841	73351	5.26%	0.670%
11	7.281	690	696	704	rBV	127521	192867	13.82%	1.762%
12	7.345	704	707	713	rVB3	1089	1634	0.12%	0.015%
13	7.481	724	730	737	rBV	165746	260176	18.64%	2.377%
14	7.951	804	810	819	rVB	162767	249380	17.87%	2.278%
15	8.663	925	931	939	rBV	133054	207768	14.89%	1.898%
16	9.122	1003	1009	1018	rBV	191663	305774	21.91%	2.793%
17	9.228	1025	1027	1030	rBV3	1766	1904	0.14%	0.017%
18	9.492	1067	1072	1078	rVB2	3695	5947	0.43%	0.054%
19	9.845	1125	1132	1141	rBV	190462	298541	21.39%	2.727%
20	10.310	1208	1211	1216	rBV2	2735	4010	0.29%	0.037%
21	10.381	1216	1223	1236	rBV	278444	442497	31.71%	4.042%
22	10.757	1281	1287	1296	rVB	166515	268099	19.21%	2.449%
23	10.910	1306	1313	1321	rBV	145766	251030	17.99%	2.293%
24	11.986	1489	1496	1500	rVB2	1073	1735	0.12%	0.016%
25	12.339	1553	1556	1558	rBV	2448	2771	0.20%	0.025%
26	13.998	1832	1838	1845	rBV	472064	609773	43.70%	5.570%
27	14.280	1880	1886	1894	rBV	513636	700102	50.17%	6.396%
28	14.510	1920	1925	1929	rBV4	2403	3663	0.26%	0.033%
29	14.586	1932	1938	1946	rVB	269322	368263	26.39%	3.364%
30	14.804	1970	1975	1988	rBV3	19557	37447	2.68%	0.342%
31	15.574	2099	2106	2113	rBV	687057	930545	66.68%	8.501%
32	15.704	2122	2128	2139	rBV	233942	301934	21.64%	2.758%
33	15.810	2143	2146	2150	rBV3	2185	2619	0.19%	0.024%
34	15.945	2165	2169	2176	rVV	13997	19214	1.38%	0.176%
35	16.627	2282	2285	2290	rVB3	951	1622	0.12%	0.015%
36	17.080	2357	2362	2364	rBV3	1651	2824	0.20%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
 Data File : BM038635.D
 Acq On : 01 Feb 2023 00:43
 Operator : CG/JU
 Sample : 01277-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX9G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
 Title : SVOA CALIBRATION

37	17.121	2366	2369	2373	rVV3	970	1426	0.10%	0.013%
38	17.327	2398	2404	2410	rBV	341738	456057	32.68%	4.166%
39	17.427	2415	2421	2432	rVV	759850	981965	70.37%	8.970%
40	17.504	2432	2434	2437	rVB2	3034	2844	0.20%	0.026%
41	17.609	2449	2452	2454	rVB4	1433	1485	0.11%	0.014%
42	17.833	2487	2490	2496	rBV5	1797	2318	0.17%	0.021%
43	17.986	2513	2516	2520	rVV4	3061	2724	0.20%	0.025%
44	18.039	2522	2525	2526	rVB3	1980	1716	0.12%	0.016%
45	18.086	2526	2533	2534	rBV3	1974	3739	0.27%	0.034%
46	18.209	2546	2554	2560	rBV5	24409	35693	2.56%	0.326%
47	18.256	2560	2562	2565	rVV4	2559	2050	0.15%	0.019%
48	18.286	2565	2567	2572	rVB5	2759	3422	0.25%	0.031%
49	18.433	2590	2592	2595	rBV4	2854	3997	0.29%	0.037%
50	18.504	2603	2604	2607	rBV2	2610	2066	0.15%	0.019%
51	18.568	2610	2615	2617	rVV6	2207	3323	0.24%	0.030%
52	18.692	2634	2636	2638	rBV3	2172	2039	0.15%	0.019%
53	18.721	2638	2641	2646	rVV6	6277	9756	0.70%	0.089%
54	18.951	2678	2680	2681	rBV2	2255	1502	0.11%	0.014%
55	19.156	2713	2715	2716	rBV2	2433	1608	0.12%	0.015%
56	19.286	2732	2737	2740	rBV4	8649	14290	1.02%	0.131%
57	19.351	2745	2748	2753	rVB2	8917	12718	0.91%	0.116%
58	19.445	2762	2764	2766	rBV3	2509	1896	0.14%	0.017%
59	19.480	2766	2770	2775	rBV7	14235	21784	1.56%	0.199%
60	19.715	2805	2810	2817	rVB	903115	1124575	80.59%	10.273%
61	20.115	2876	2878	2886	rVB9	10935	16174	1.16%	0.148%
62	20.692	2974	2976	2979	rVB4	14906	12285	0.88%	0.112%
63	21.503	3109	3114	3118	rBV	432056	522843	37.47%	4.776%
64	23.750	3490	3496	3506	rVB2	740748	1395513	100.00%	12.748%
65	23.909	3517	3523	3530	rVB2	337386	638873	45.78%	5.836%


Sum of corrected areas: 10946755

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038635.D
Acq On : 01 Feb 2023 00:43
Operator : CG/JU
Sample : 01277-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

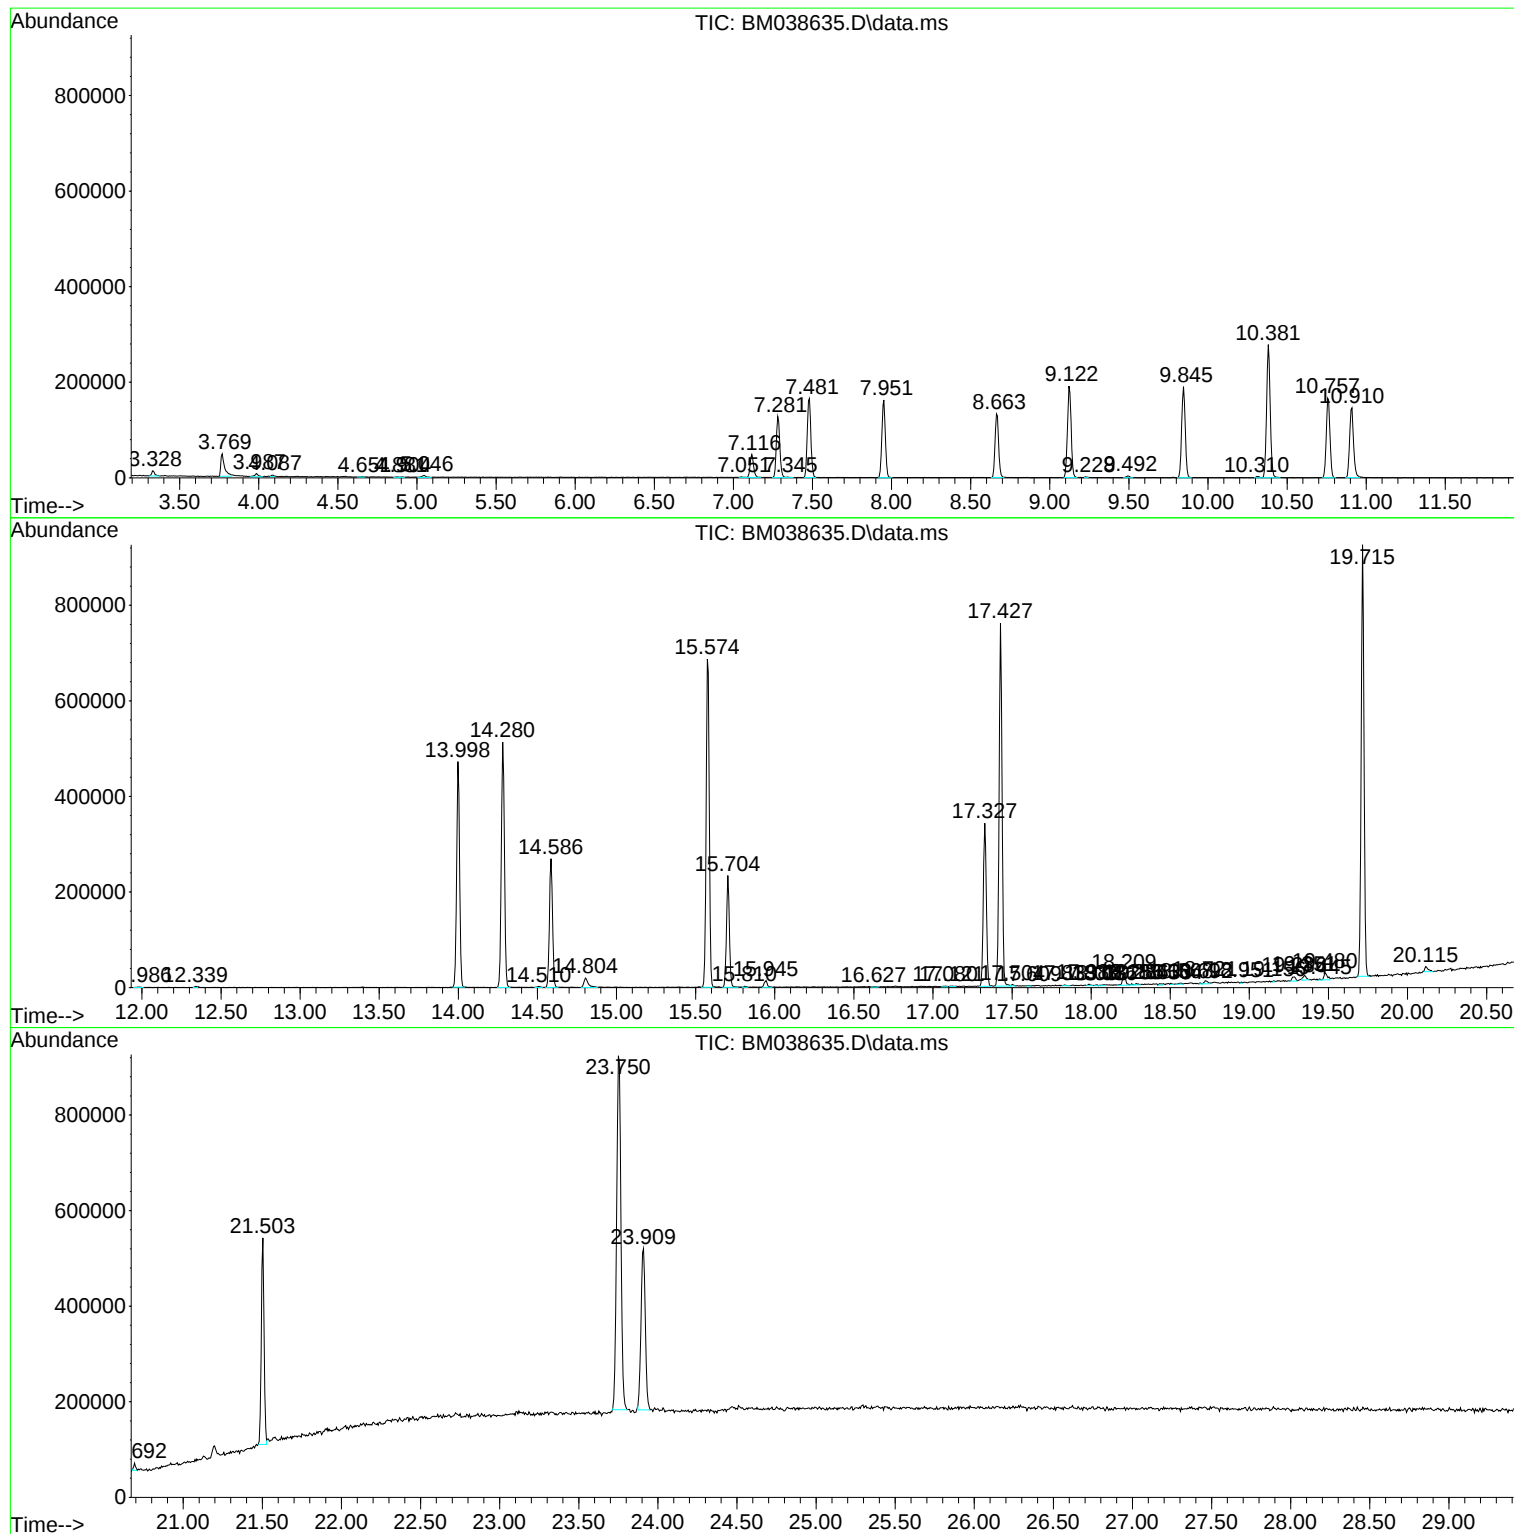

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038635.D
Acq On : 01 Feb 2023 00:43
Operator : CG/JU
Sample : 01277-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM013123\
Data File : BM038635.D
Acq On : 01 Feb 2023 00:43
Operator : CG/JU
Sample : 01277-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX9G9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013023.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc