

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020119\
 Data File : BM018713.D
 Acq On : 01 Feb 2019 19:25
 Operator : JU/SJ
 Sample : K1308-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-18(34.5-35)

Quant Time: Feb 01 22:17:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 22:01:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	249377	20.00	ng	-0.02
21) Naphthalene-d8	10.51	136	934940	20.00	ng	-0.02
39) Acenaphthene-d10	14.37	164	470301	20.00	ng	-0.02
64) Phenanthrene-d10	17.12	188	1006917	20.00	ng	-0.02
76) Chrysene-d12	21.32	240	1053754	20.00	ng	-0.02
87) Perylene-d12	23.57	264	1175812	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	2108916	156.15	ng	-0.02
7) Phenol-d6	6.90	99	2637008	153.73	ng	-0.01
23) Nitrobenzene-d5	8.89	82	1595469	98.93	ng	-0.02
42) 2,4,6-Tribromophenol	15.87	330	925999	154.64	ng	-0.02
45) 2-Fluorobiphenyl	12.99	172	3465210	96.14	ng	-0.02
79) Terphenyl-d14	19.76	244	4488966	89.80	ng	-0.01
Target Compounds						
15) Benzyl Alcohol	8.04	79	25071	2.024	ng	Qvalue # 49
50) Dimethylphthalate	13.83	163	241528	6.253	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020119\
Data File : BM018713.D
Acq On : 01 Feb 2019 19:25
Operator : JU/SJ
Sample : K1308-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-18(34.5-35)

Quant Time: Feb 01 22:17:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration




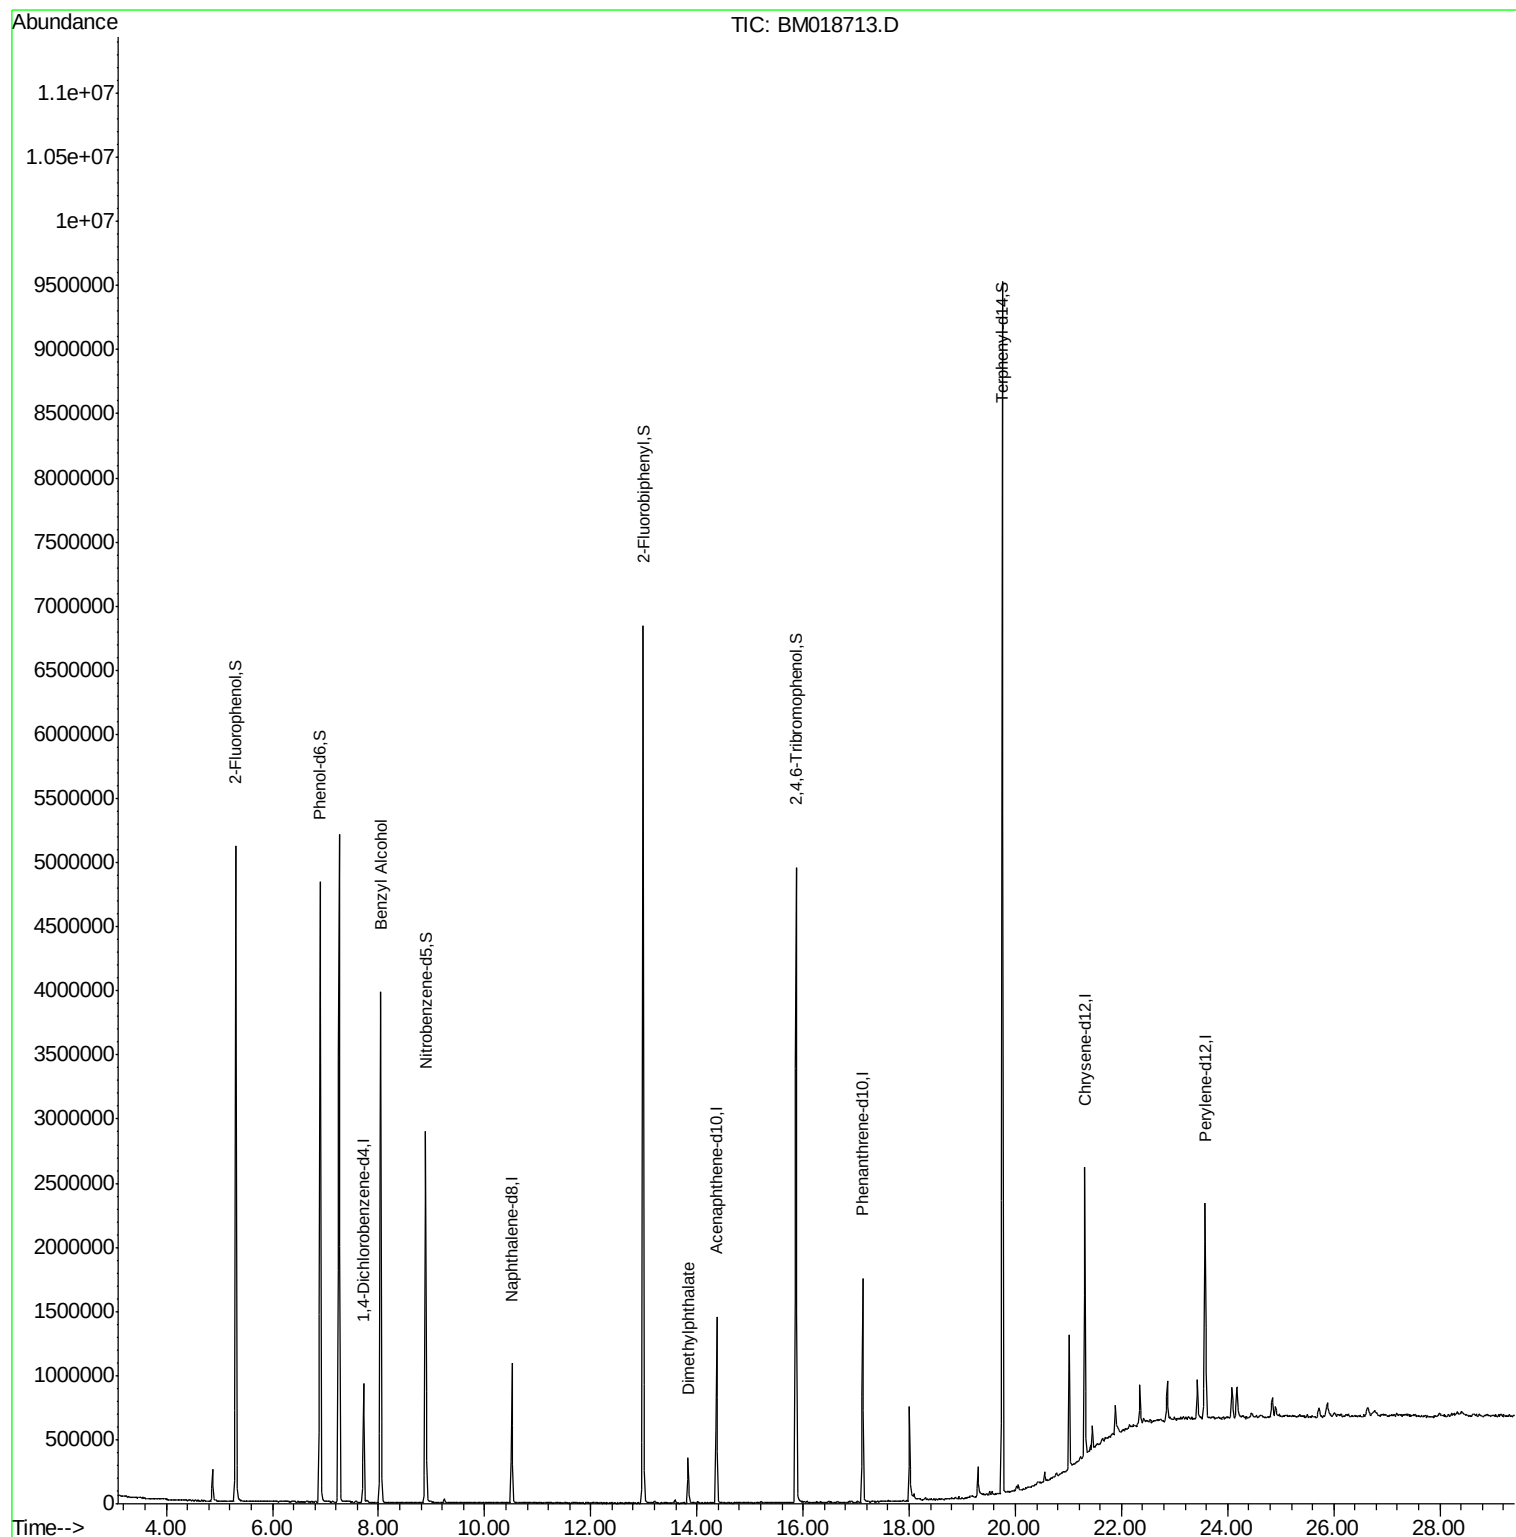


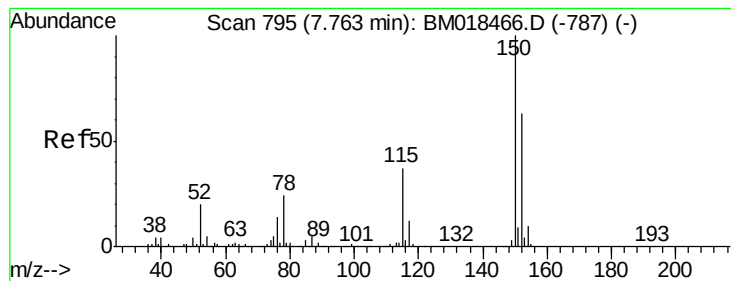

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.72 min Scan# 788
 Delta R.T. -0.02 min
 Lab File: BM018713.D
 Acq: 01 Feb 2019 19:25




Instrument :
 BNA_M
 ClientSampleId :
 SB-18(34.5-35)


Tgt Ion	Ratio	Lower	Upper
152	100		
150	157.2	126.9	190.3
115	58.0	45.5	68.3

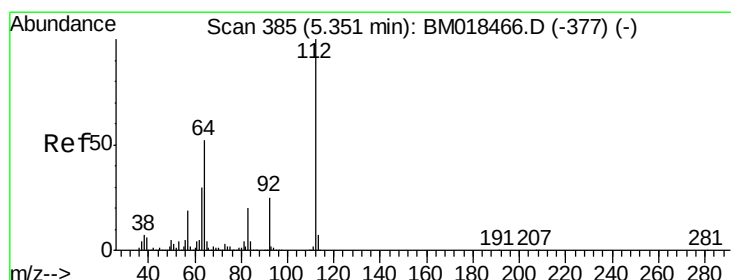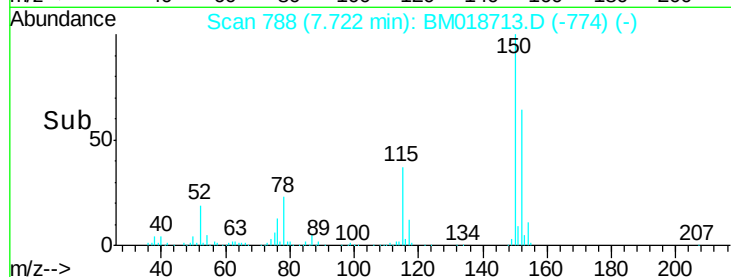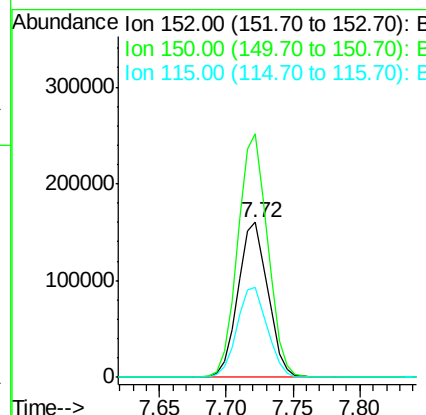

#5
 2-Fluorophenol
 Concen: 156.153 ng
 RT: 5.31 min Scan# 378
 Delta R.T. -0.02 min
 Lab File: BM018713.D
 Acq: 01 Feb 2019 19:25

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.5	46.5	69.7
63	29.3	25.2	37.8

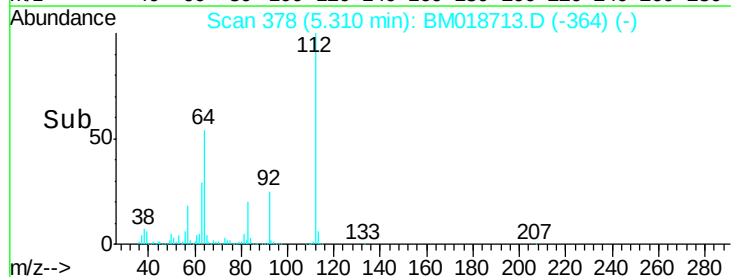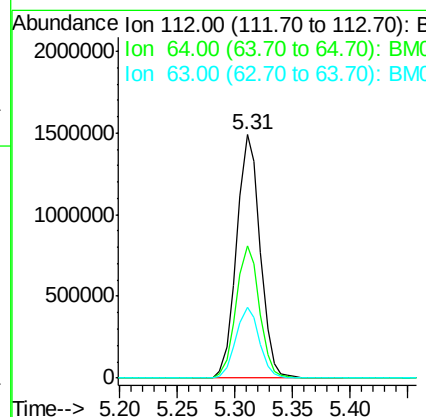

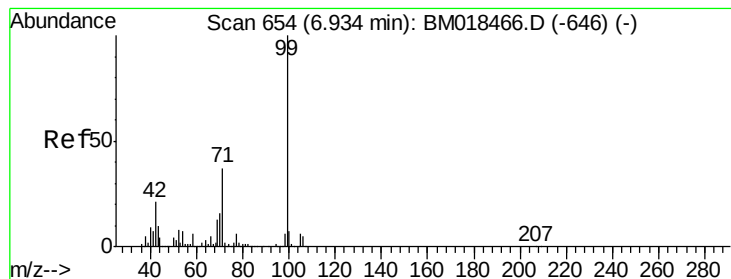

#7

Phenol-d6

Concen: 153.730 ng

RT: 6.90 min Scan# 648

Delta R.T. -0.01 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25

Instrument :

BNA_M

ClientSampleId :

SB-18(34.5-35)


Tgt Ion: 99 Resp: 2637008

Ion Ratio Lower Upper




99 100

42 19.6 17.3 25.9

71 35.4 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BM018713.D (-633) (-)

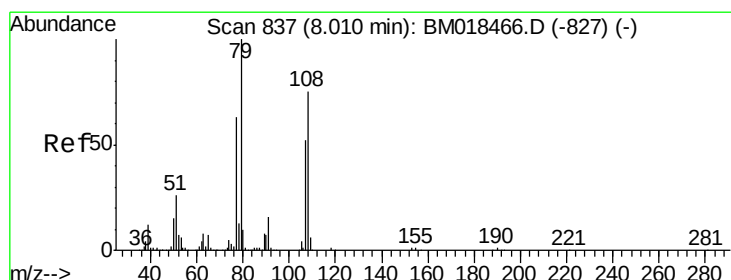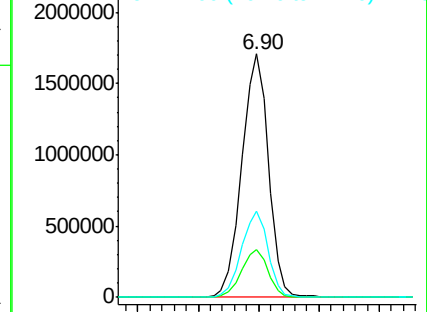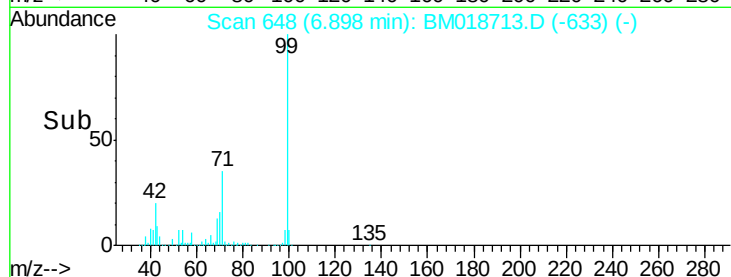

#15

Benzyl Alcohol

Concen: 2.024 ng

RT: 8.04 min Scan# 842

Delta R.T. 0.05 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25


Tgt Ion: 79 Resp: 25071

Ion Ratio Lower Upper



79 100


108 32.2 60.4 90.6#

77 107.7 53.4 80.2#



Abundance Ion 79.00 (78.70 to 79.70): BM018713.D (-816) (-)



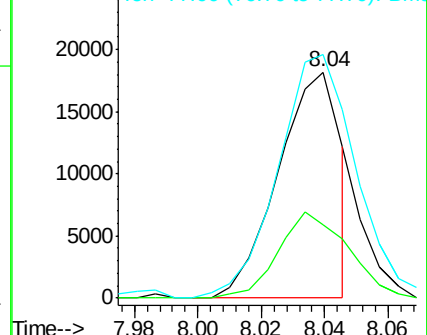
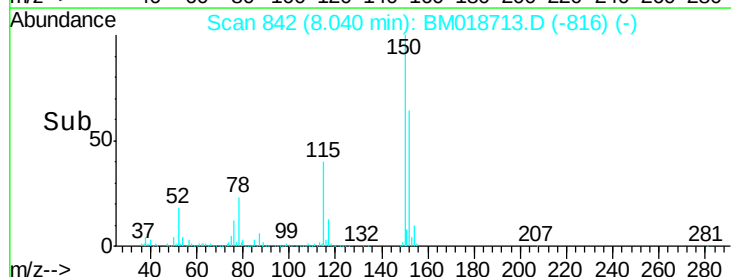


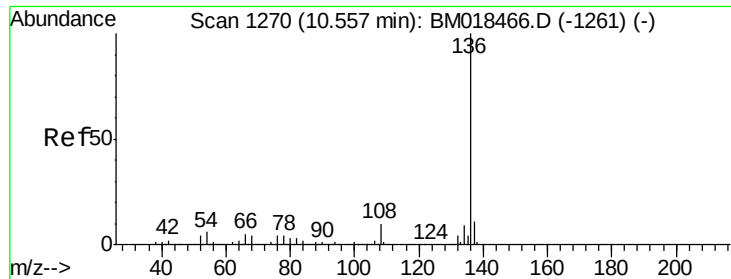

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.51 min Scan# 1262
Delta R.T. -0.02 min
Lab File: BM018713.D
Acq: 01 Feb 2019 19:25




Instrument :
BNA_M
ClientSampleId :
SB-18(34.5-35)


Tgt Ion:	136	Resp:	934940
Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.5	12.7
54	6.7	6.0	9.0
68	4.8	4.5	6.7

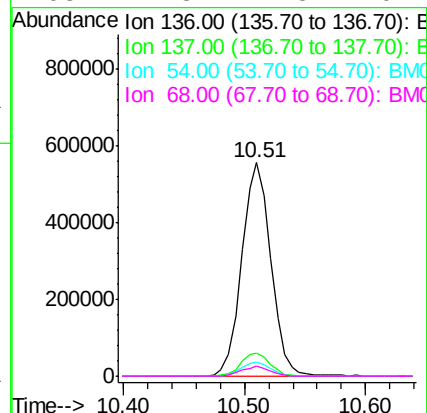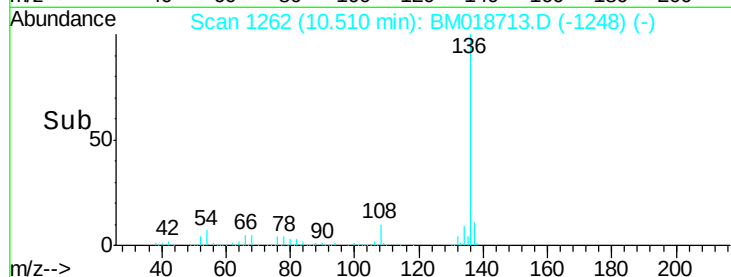

#23
Nitrobenzene-d5
Concen: 98.927 ng
RT: 8.89 min Scan# 986
Delta R.T. -0.02 min
Lab File: BM018713.D
Acq: 01 Feb 2019 19:25

Tgt Ion:	82	Resp:	1595469
Ion	Ratio	Lower	Upper
82	100		
128	45.7	36.3	54.5
54	48.6	41.7	62.5

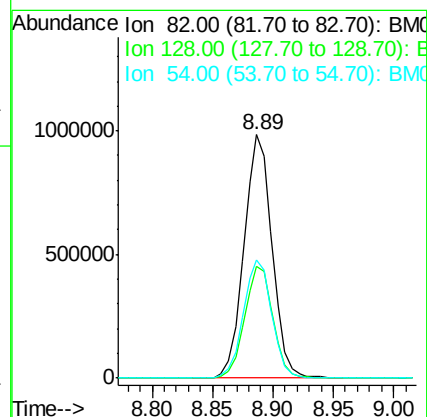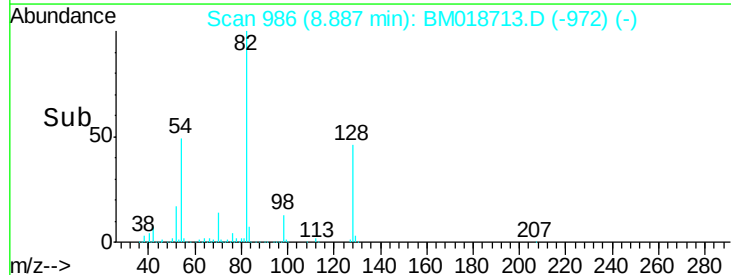

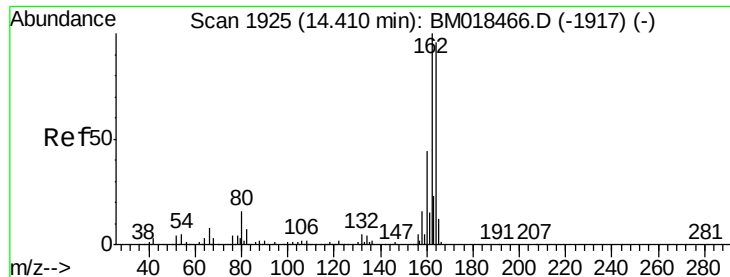

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.37 min Scan# 1918

Delta R.T. -0.02 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25

Instrument :

BNA_M

ClientSampleId :

SB-18(34.5-35)


Tgt Ion:164 Resp: 470301

Ion Ratio Lower Upper

164 100

162 104.6 83.0 124.4




160 46.1 37.1 55.7

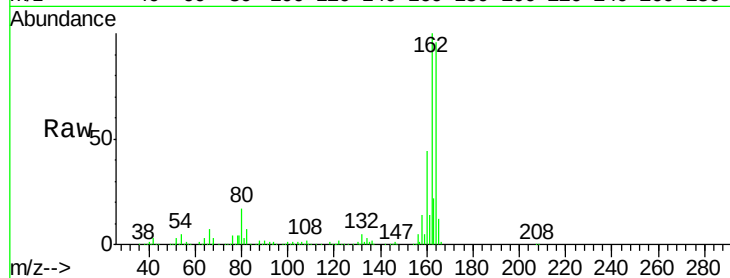

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

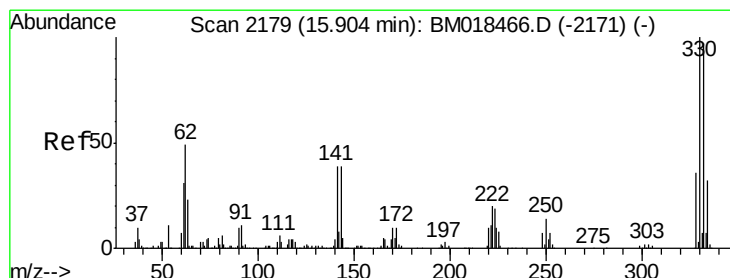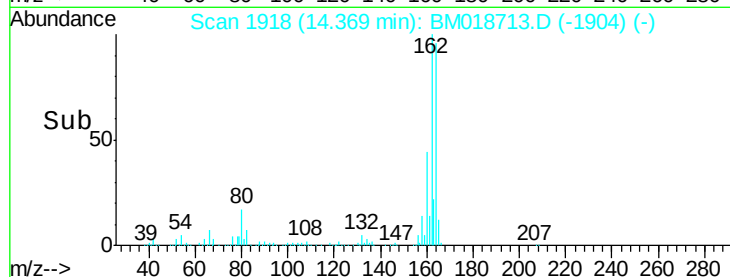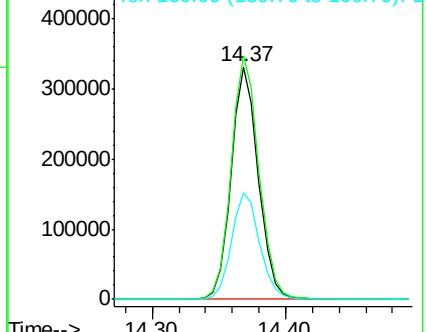

#42

2,4,6-Tribromophenol

Concen: 154.636 ng

RT: 15.87 min Scan# 2173

Delta R.T. -0.02 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25


Tgt Ion:330 Resp: 925999

Ion Ratio Lower Upper

330 100

332 97.2 77.6 116.4



141 37.5 31.7 47.5

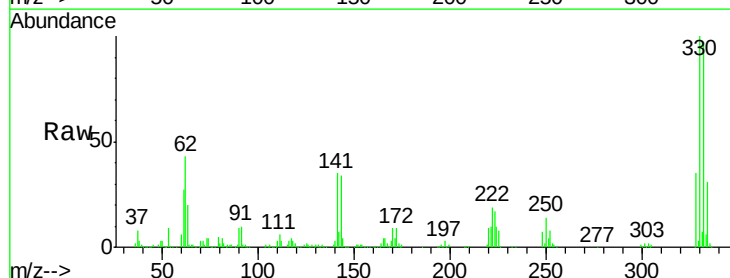


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



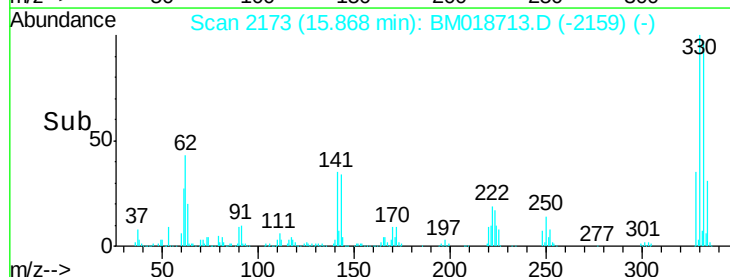
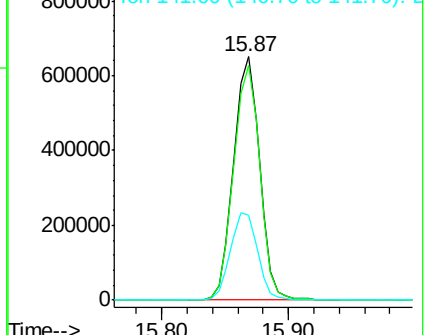


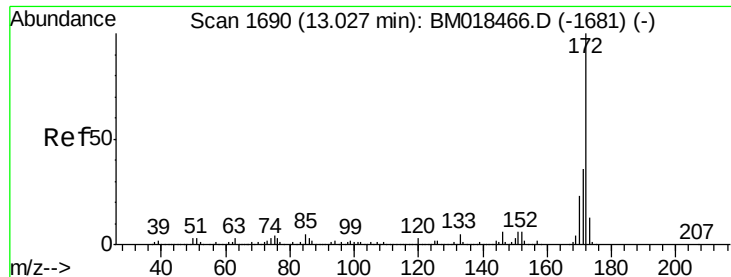

#45
2-Fluorobiphenyl
Concen: 96.143 ng
RT: 12.99 min Scan# 1683
Delta R.T. -0.02 min
Lab File: BM018713.D
Acq: 01 Feb 2019 19:25




Instrument :
BNA_M
ClientSampleId :
SB-18(34.5-35)


Tgt Ion:172 Resp: 3465210
Ion Ratio Lower Upper
172 100
171 35.7 28.2 42.4
170 23.1 18.9 28.3

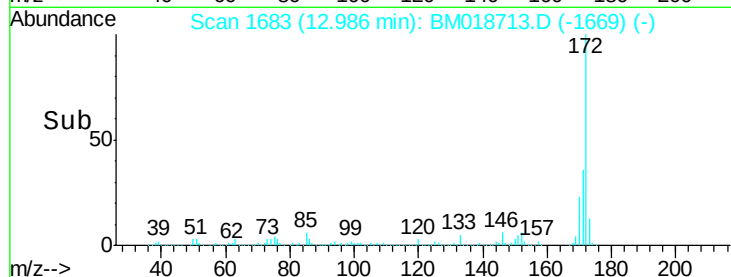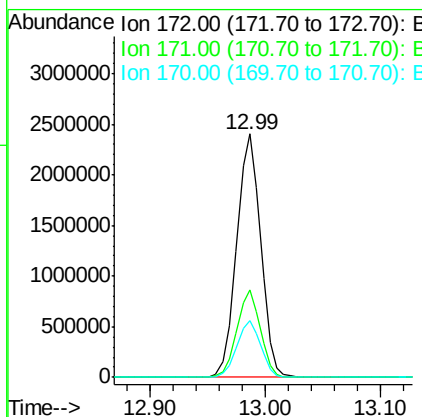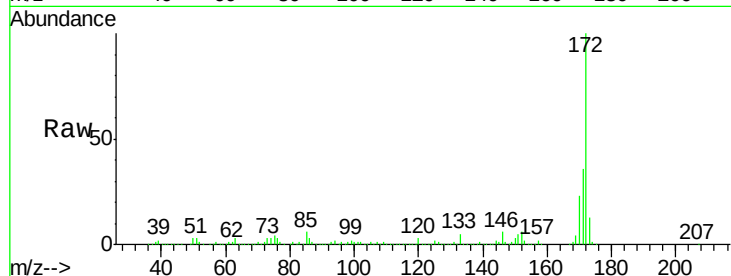

#50
Dimethylphthalate
Concen: 6.253 ng
RT: 13.83 min Scan# 1827
Delta R.T. -0.02 min
Lab File: BM018713.D
Acq: 01 Feb 2019 19:25

Tgt Ion:163 Resp: 241528
Ion Ratio Lower Upper
163 100
194 4.3 3.0 4.6
164 10.9 7.8 11.8

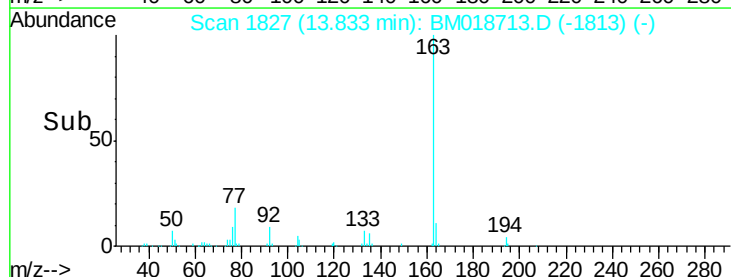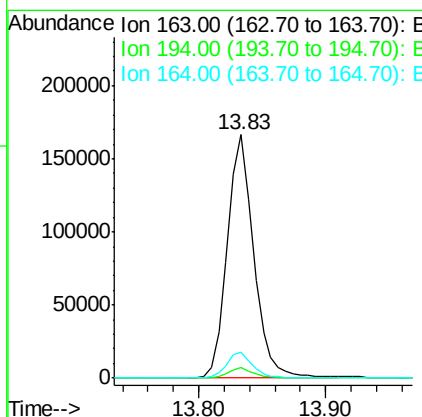

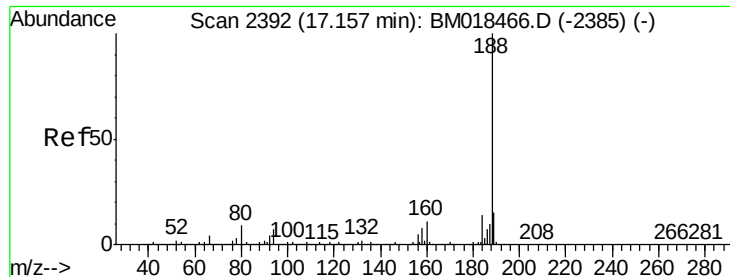

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.12 min Scan# 2386

Delta R.T. -0.02 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25

Instrument :

BNA_M

ClientSampleId :

SB-18(34.5-35)


Tgt Ion:188 Resp: 1006917

Ion Ratio Lower Upper

188 100

94 7.8 7.1 10.7




80 8.7 7.6 11.4

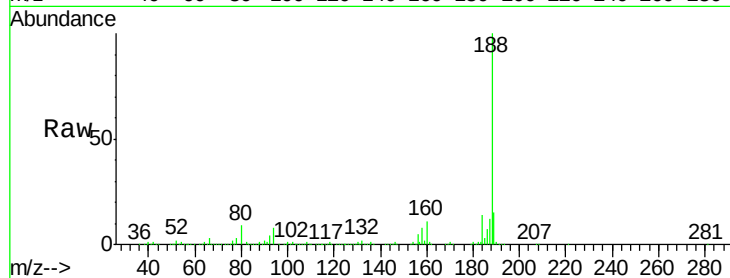

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

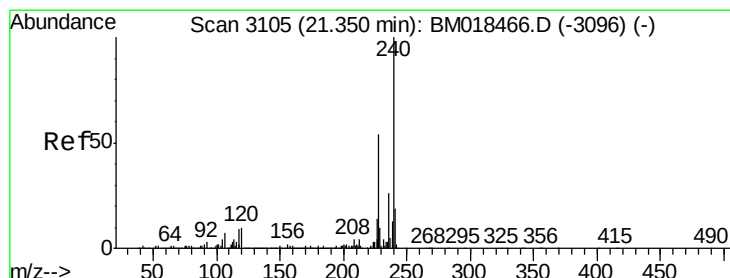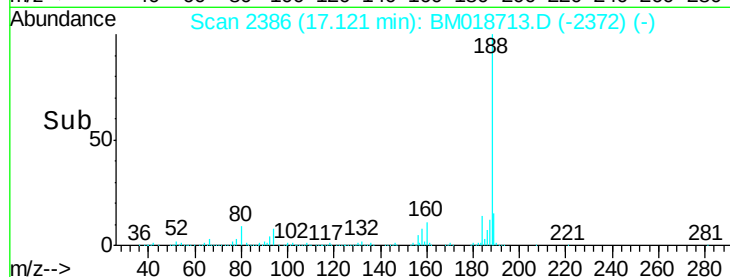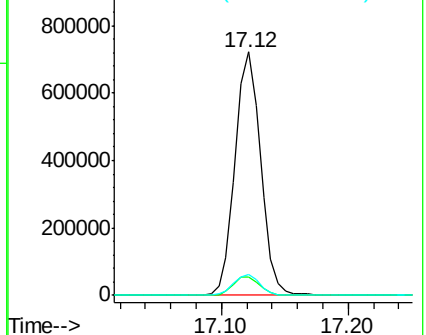

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.32 min Scan# 3099

Delta R.T. -0.02 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25


Tgt Ion:240 Resp: 1053754

Ion Ratio Lower Upper

240 100

120 9.6 8.4 12.6



236 25.6 20.7 31.1

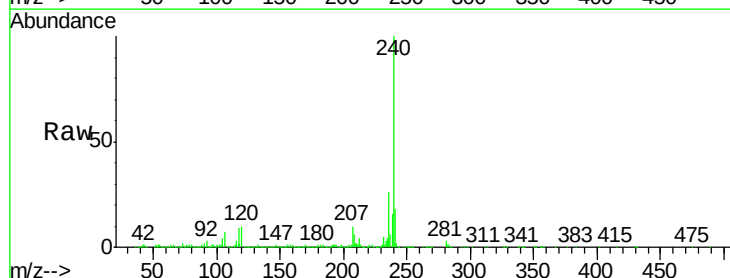


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

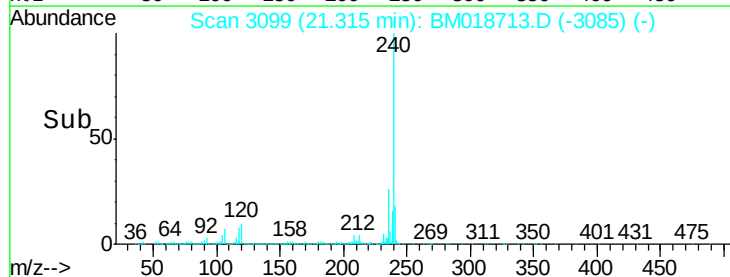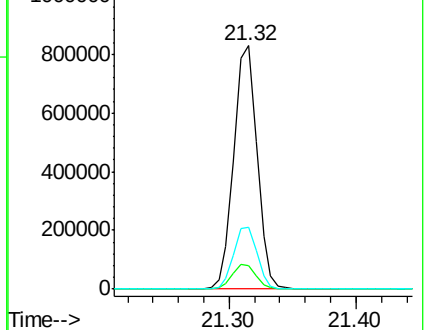

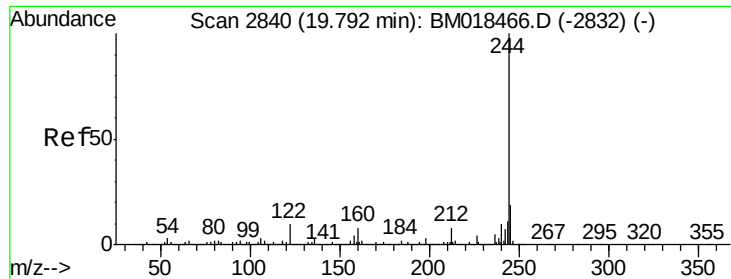

#79

Terphenyl-d14

Concen: 89.802 ng

RT: 19.76 min Scan# 2834

Delta R.T. -0.01 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25

Instrument :

BNA_M

ClientSampleId :

SB-18(34.5-35)


Tgt Ion:244 Resp: 4488966

Ion Ratio Lower Upper

244 100

212 7.5 5.9 8.9




122 9.4 9.0 13.4

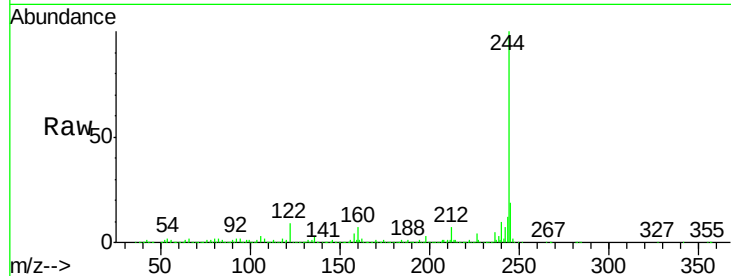

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

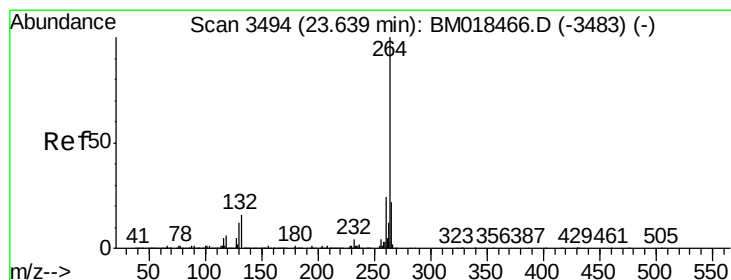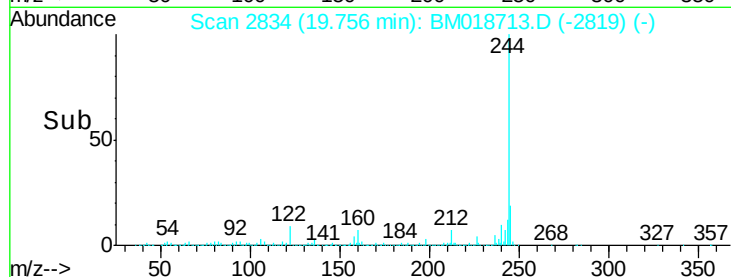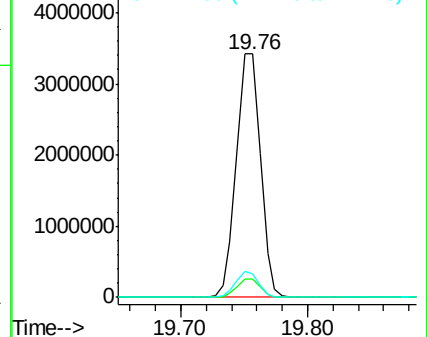

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.57 min Scan# 3483

Delta R.T. -0.03 min

Lab File: BM018713.D

Acq: 01 Feb 2019 19:25


Tgt Ion:264 Resp: 1175812

Ion Ratio Lower Upper

264 100

260 23.2 18.9 28.3

265 21.7 16.8 25.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

