
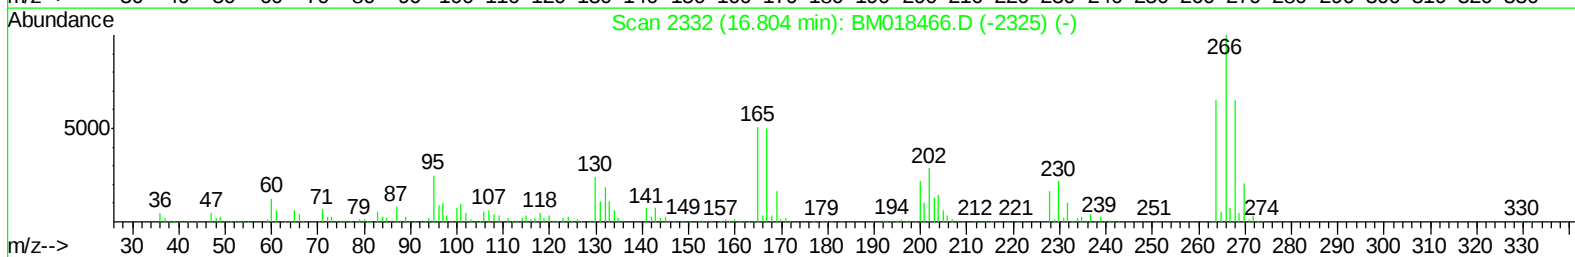
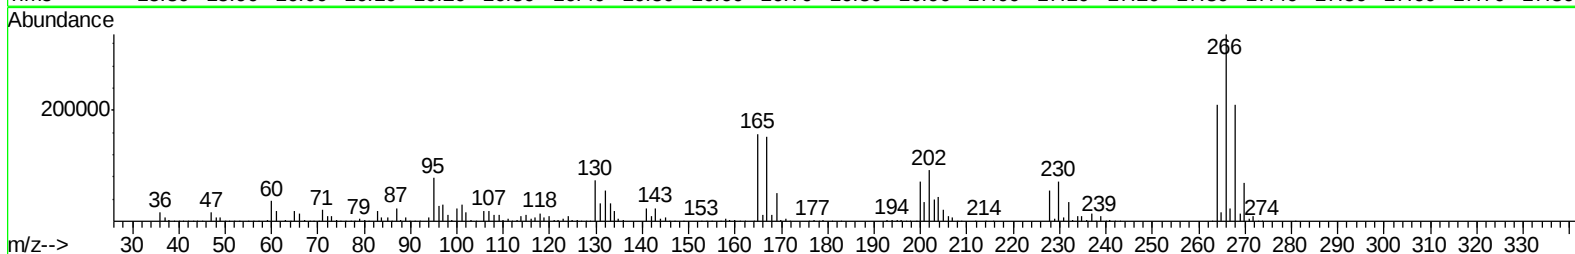


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020119\
Data File : BM018704.D
Acq On : 01 Feb 2019 10:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 22:30:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 22:01:30 2019
Response via : Initial Calibration

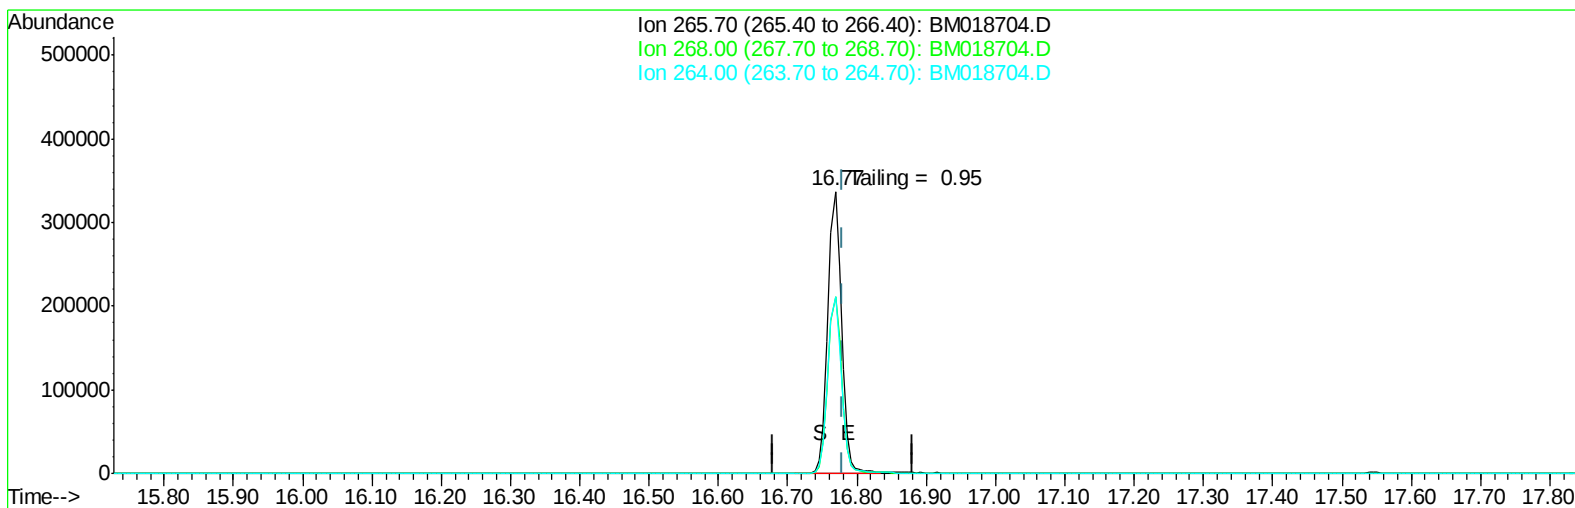

TIC: BM018704.D

(70) Pentachlorophenol (C)




16.768min (-0.012) 19909.49ng

response 464243

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.69
264.00	62.60	62.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020119\
 Data File : BM018704.D
 Acq On : 01 Feb 2019 10:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 22:30:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 22:01:30 2019
 Response via : Initial Calibration

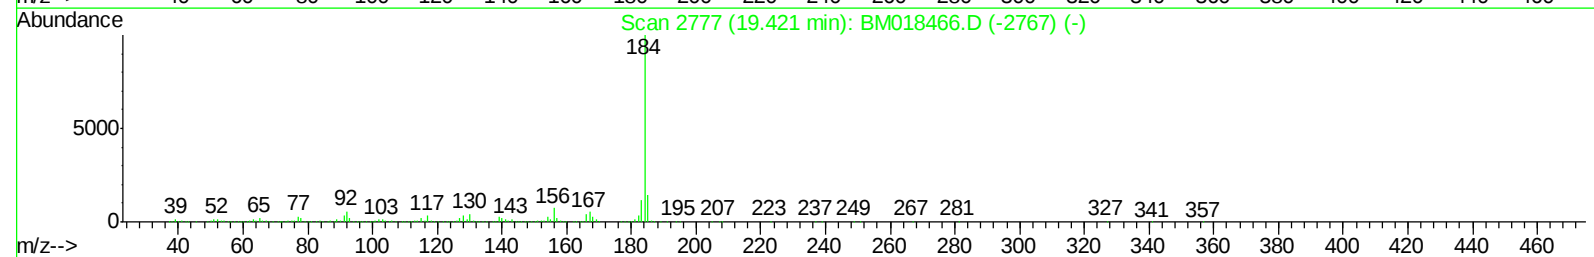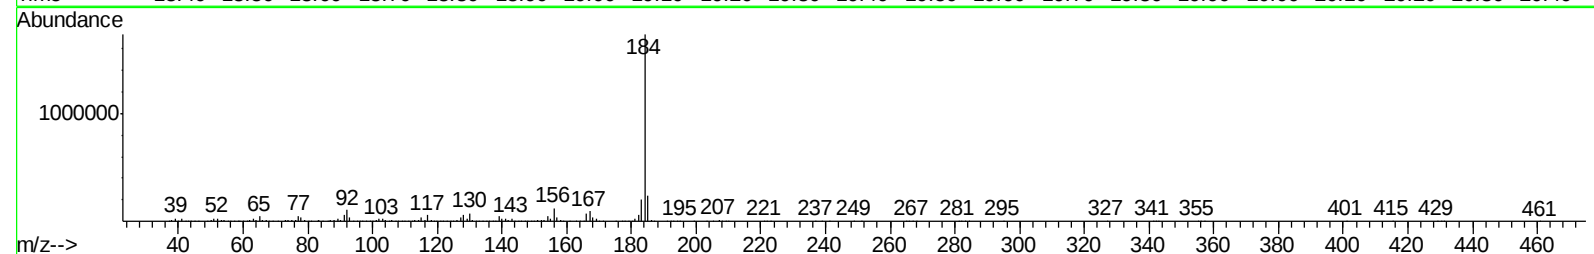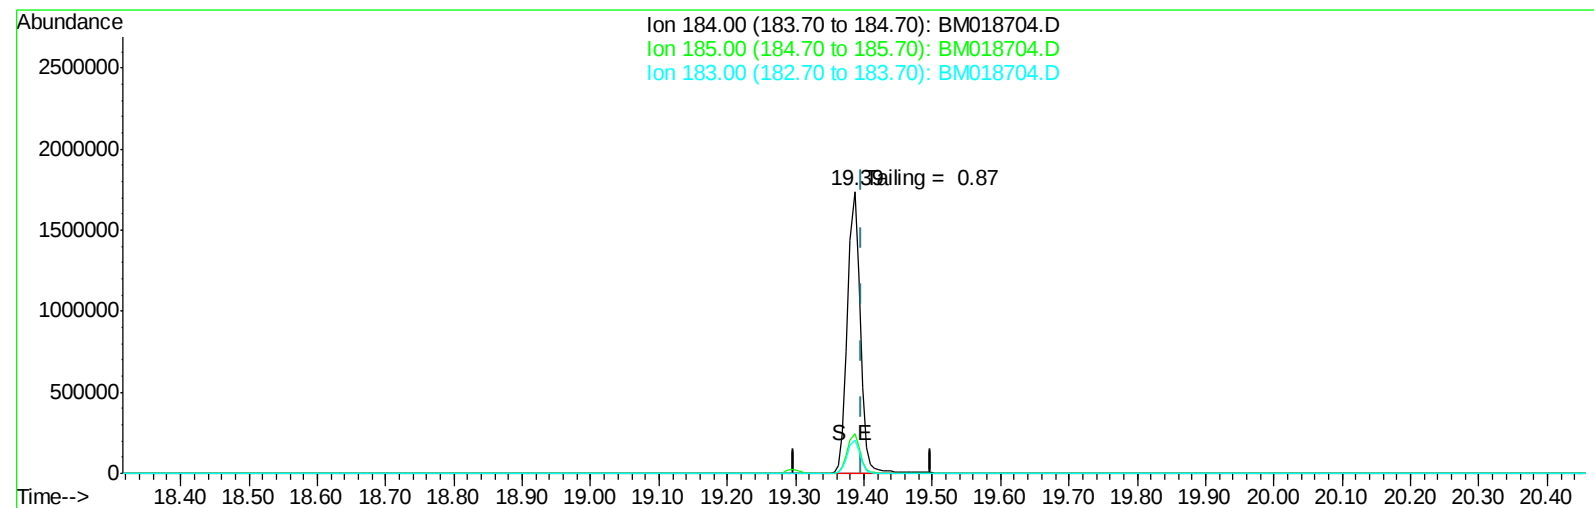

TIC: BM018704.D

(77) Benzidine

19.386min (-0.012) 1119.90ng

response 2230166

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.92
183.00	11.90	11.82
0.00	0.00	0.00