

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
 Data File : BM038660.D
 Acq On : 02 Feb 2023 12:57
 Operator : CG/JU
 Sample : PB150597BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150597BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	306	312	318	rBV	328043	450080	13.98%	3.024%
2	5.499	386	393	404	rBV	1054575	1441360	44.76%	9.684%
3	7.116	660	668	680	rBV	913073	1382762	42.94%	9.290%
4	7.928	799	806	814	rVB	217989	327244	10.16%	2.199%
5	9.104	999	1006	1015	rBV	546411	864542	26.85%	5.809%
6	10.739	1277	1284	1291	rBV	247769	391214	12.15%	2.628%
7	13.192	1695	1701	1715	rBV	1835761	2594846	80.58%	17.434%
8	14.569	1929	1935	1943	rVB	395922	547801	17.01%	3.681%
9	16.063	2183	2189	2202	rBV	1333139	1818341	56.47%	12.217%
10	17.310	2396	2401	2408	rBV	435748	590699	18.34%	3.969%
11	18.198	2545	2552	2560	rBV2	26554	48926	1.52%	0.329%
12	19.927	2841	2846	2852	rBV	2967360	3220123	100.00%	21.635%
13	21.486	3107	3111	3120	rBV	457030	581707	18.06%	3.908%
14	23.886	3513	3519	3525	rVB	318083	624015	19.38%	4.193%




Sum of corrected areas: 14883660

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
Data File : BM038660.D
Acq On : 02 Feb 2023 12:57
Operator : CG/JU
Sample : PB150597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150597BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

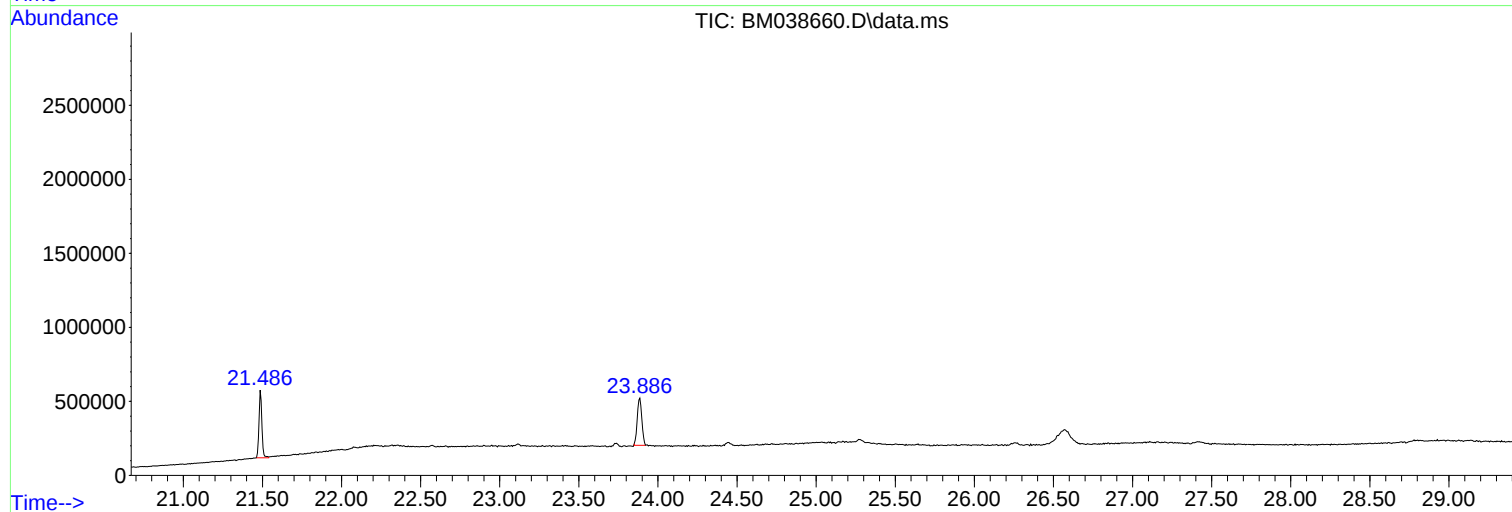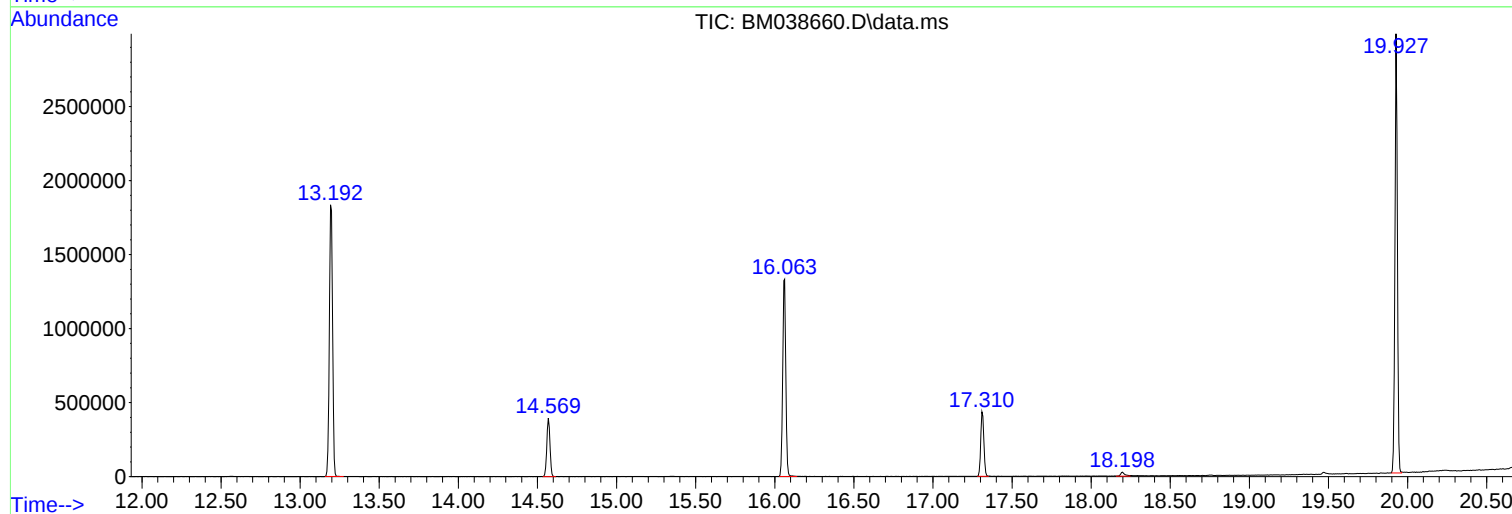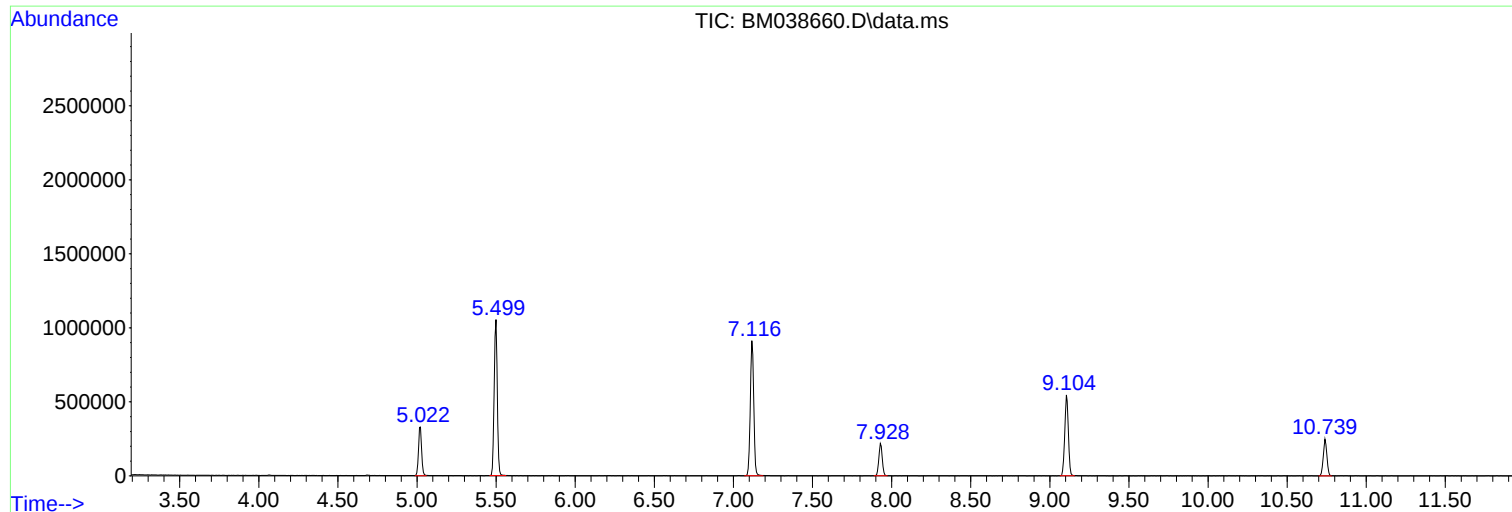

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
Data File : BM038660.D
Acq On : 02 Feb 2023 12:57
Operator : CG/JU
Sample : PB150597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150597BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.022	27.51 ng	450080	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	12		
3	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	12		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Acetamide, N-(cyanomethyl)-	98	C4H6N2O	004814-80-6	9		

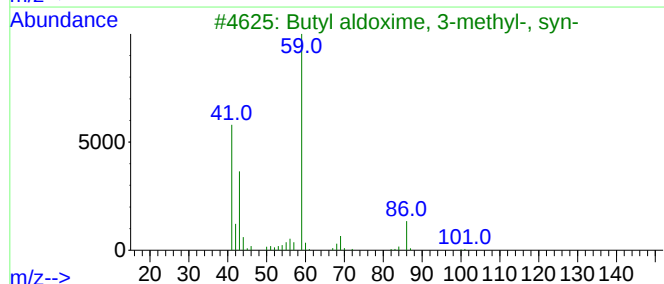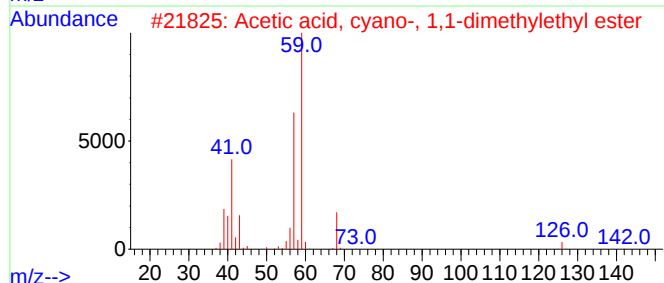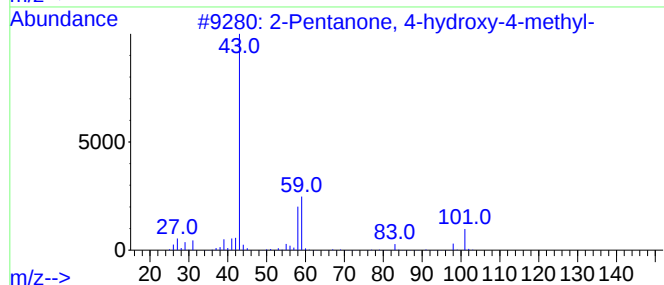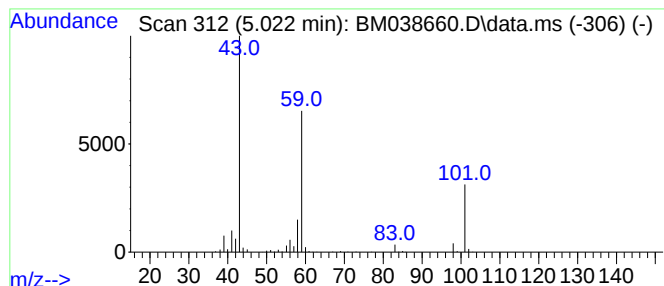

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
Data File : BM038660.D
Acq On : 02 Feb 2023 12:57
Operator : CG/JU
Sample : PB150597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150597BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.022	27.5	ng	450080	1	7.928	327244	20.0