
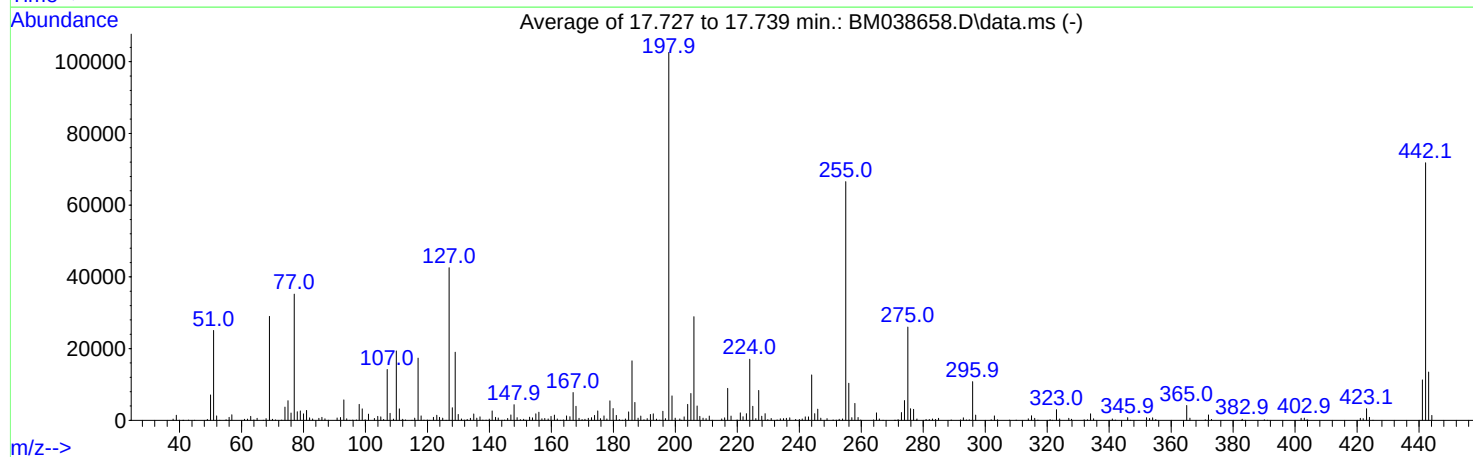


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
 Data File : BM038658.D
 Acq On : 02 Feb 2023 11:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 04 05:17:53 2023

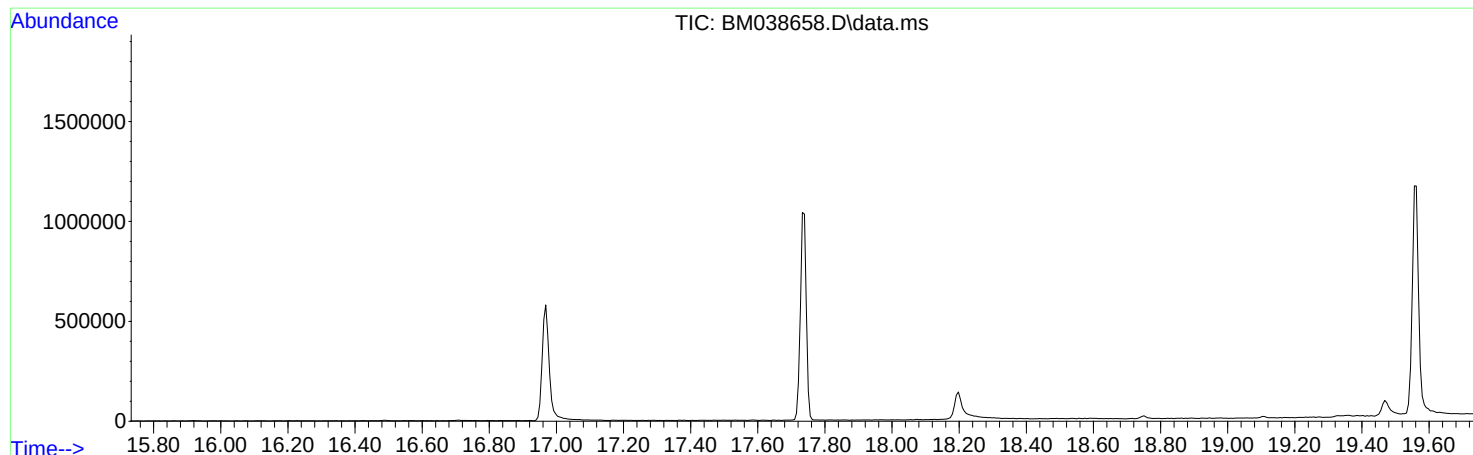

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	25067	PASS
68	69	0.00	2	1.6	472	PASS
69	198	0.00	100	28.3	29001	PASS
70	69	0.00	2	1.1	319	PASS
127	198	10	80	41.5	42576	PASS
197	198	0.00	2	0.5	483	PASS
198	198	100	100	100.0	102555	PASS
199	198	5	9	6.7	6846	PASS
275	198	10	60	25.4	26015	PASS
365	198	1	100	4.1	4172	PASS
441	198	0.01	100	11.0	11277	PASS
442	442	50	100	100.0	71800	PASS
443	442	15	24	18.8	13468	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/2/2023	BNA_M	<u>BM038658.D</u>
Compound Name	Response	Retention Time
DDT	357930	20.78
DDD	6755	20.344
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6755	364685	1.85

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
Data File : BM038658.D
Acq On : 02 Feb 2023 11:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 03 08:08:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

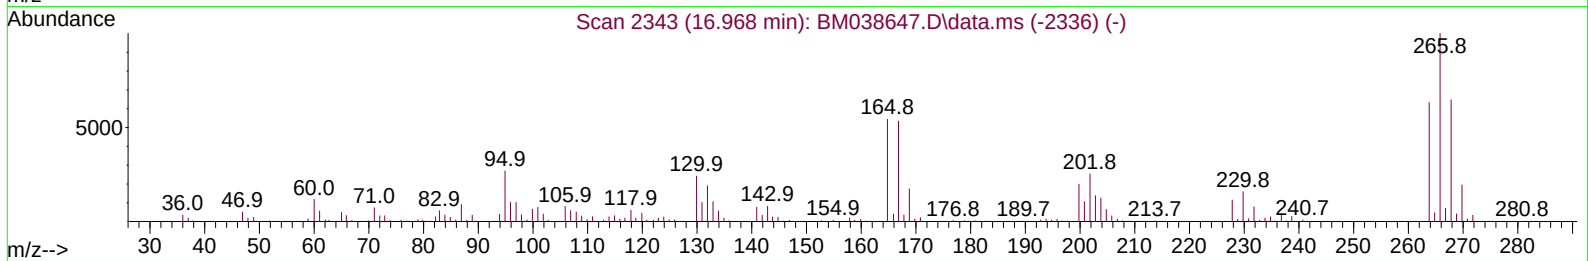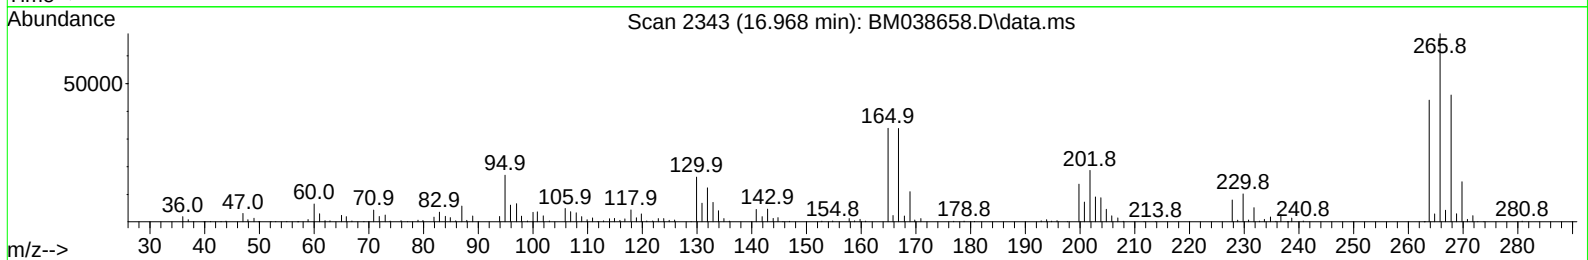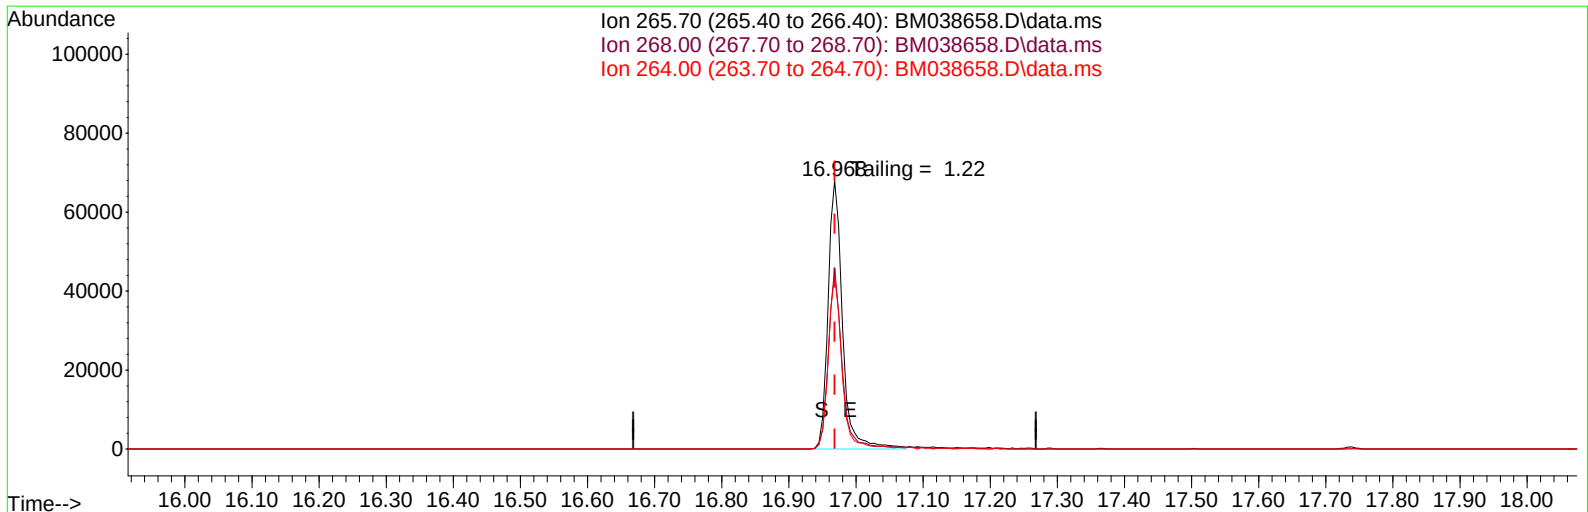

TIC: BM038658.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.000) 0.00 ng




response 101958

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.46
264.00	63.30	64.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020223\
Data File : BM038658.D
Acq On : 02 Feb 2023 11:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 03 08:08:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

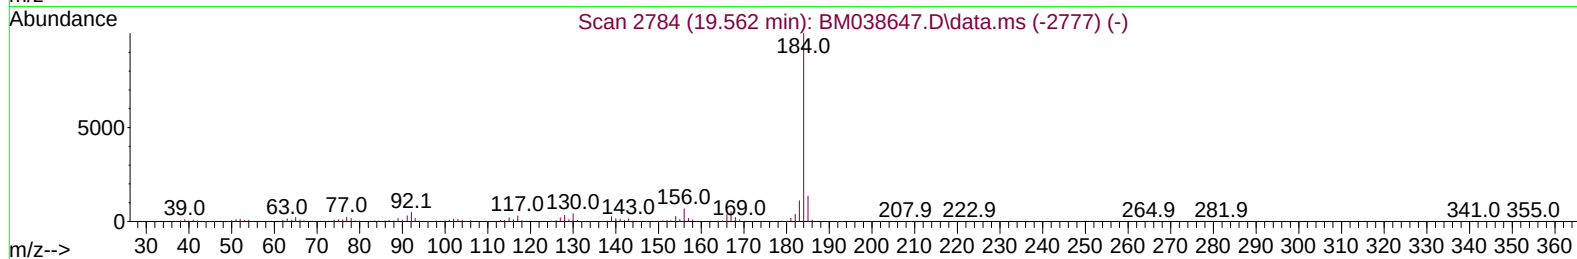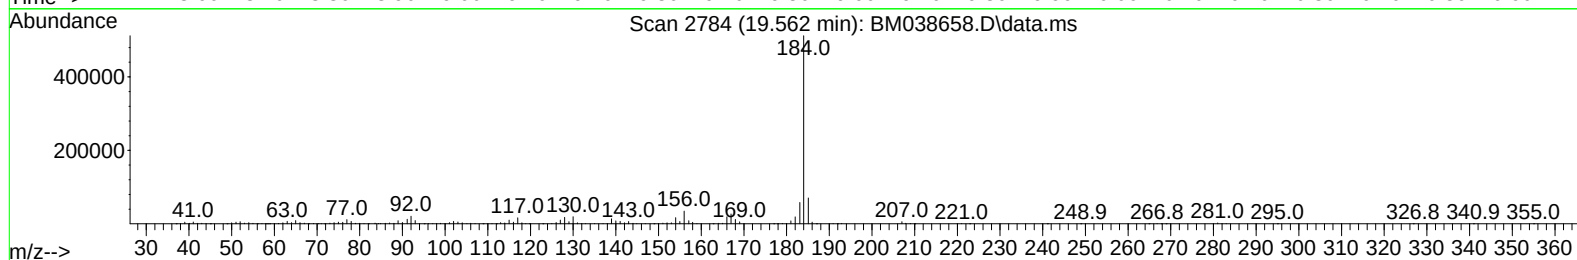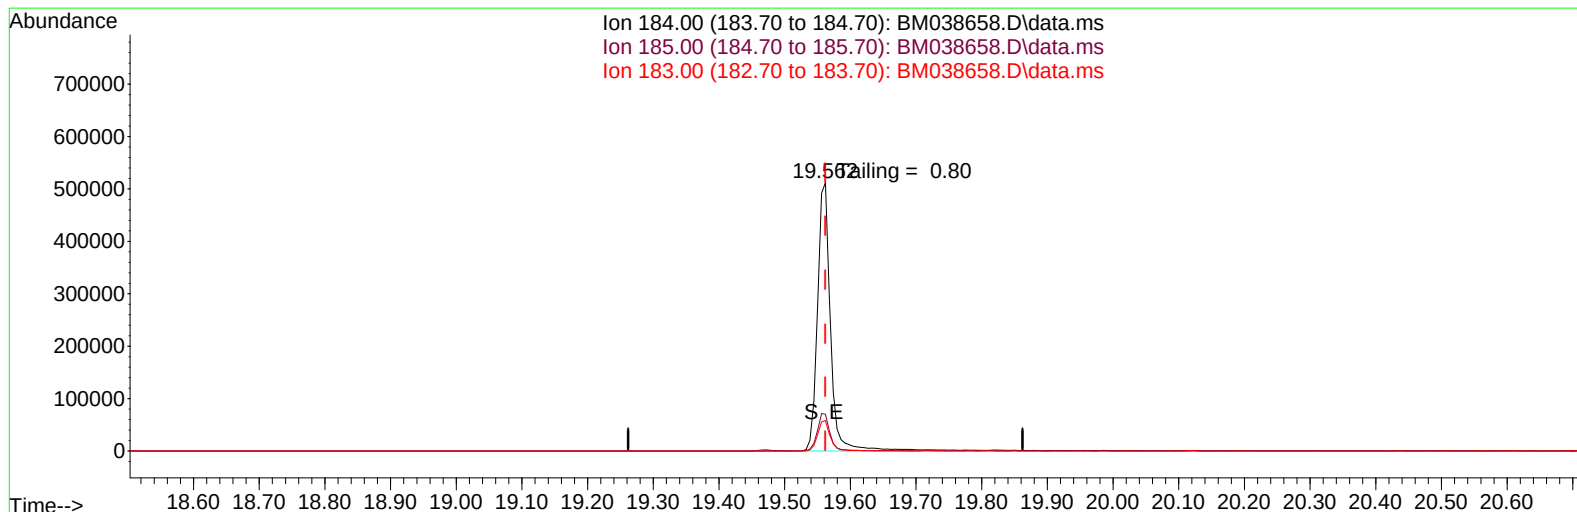

TIC: BM038658.D\data.ms

(77) Benzidine

19.562min (+ 0.000) 188703.54 ng

response 703255

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.74
183.00	11.00	11.35
0.00	0.00	0.00